

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022154.D
 Acq On : 17 Oct 2022 16:40
 Operator : CG/JU
 Sample : N5060-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 17 23:10:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 13 03:08:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	152153	20.000	ng/u1	0.00
20) Naphthalene-d8	10.787	136	716672	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.628	164	456428	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.386	188	956588	20.000	ng/u1	0.00
79) Chrysene-d12	21.580	240	797668	20.000	ng/u1	-0.01
88) Perylene-d12	24.051	264	661467	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	16273	4.054	ng/uL	0.00
4) Pyridine-d5	3.699	84	106812	8.554	ng/u1	0.00
7) Phenol-d5	7.111	99	94701	6.367	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	249606	26.779	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	228913	22.196	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	149819	12.676	ng/u1	0.00
21) Nitrobenzene-d5	9.134	128	159081	30.272	ng/u1	0.00
24) 2-Nitrophenol-d4	9.863	143	160210	29.744	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.399	165	256622	25.382	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.928	131	296427	17.933	ng/u1	0.00
46) Dimethylphthalate-d6	14.040	166	949370	29.839	ng/u1	0.00
49) Acenaphthylene-d8	14.322	160	1045136	29.416	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	34971	5.149	ng/u1	0.00
60) Fluorene-d10	15.622	176	782524	29.159	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	124815	22.871	ng/u1	0.00
73) Anthracene-d10	17.481	188	1222233	29.402	ng/u1	0.00
81) Pyrene-d10	19.780	212	1343145	33.820	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.892	264	1004526	30.966	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.293	88	7329	1.675	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022154.D
Acq On : 17 Oct 2022 16:40
Operator : CG/JU
Sample : N5060-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Oct 17 23:10:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 13 03:08:08 2022
Response via : Initial Calibration

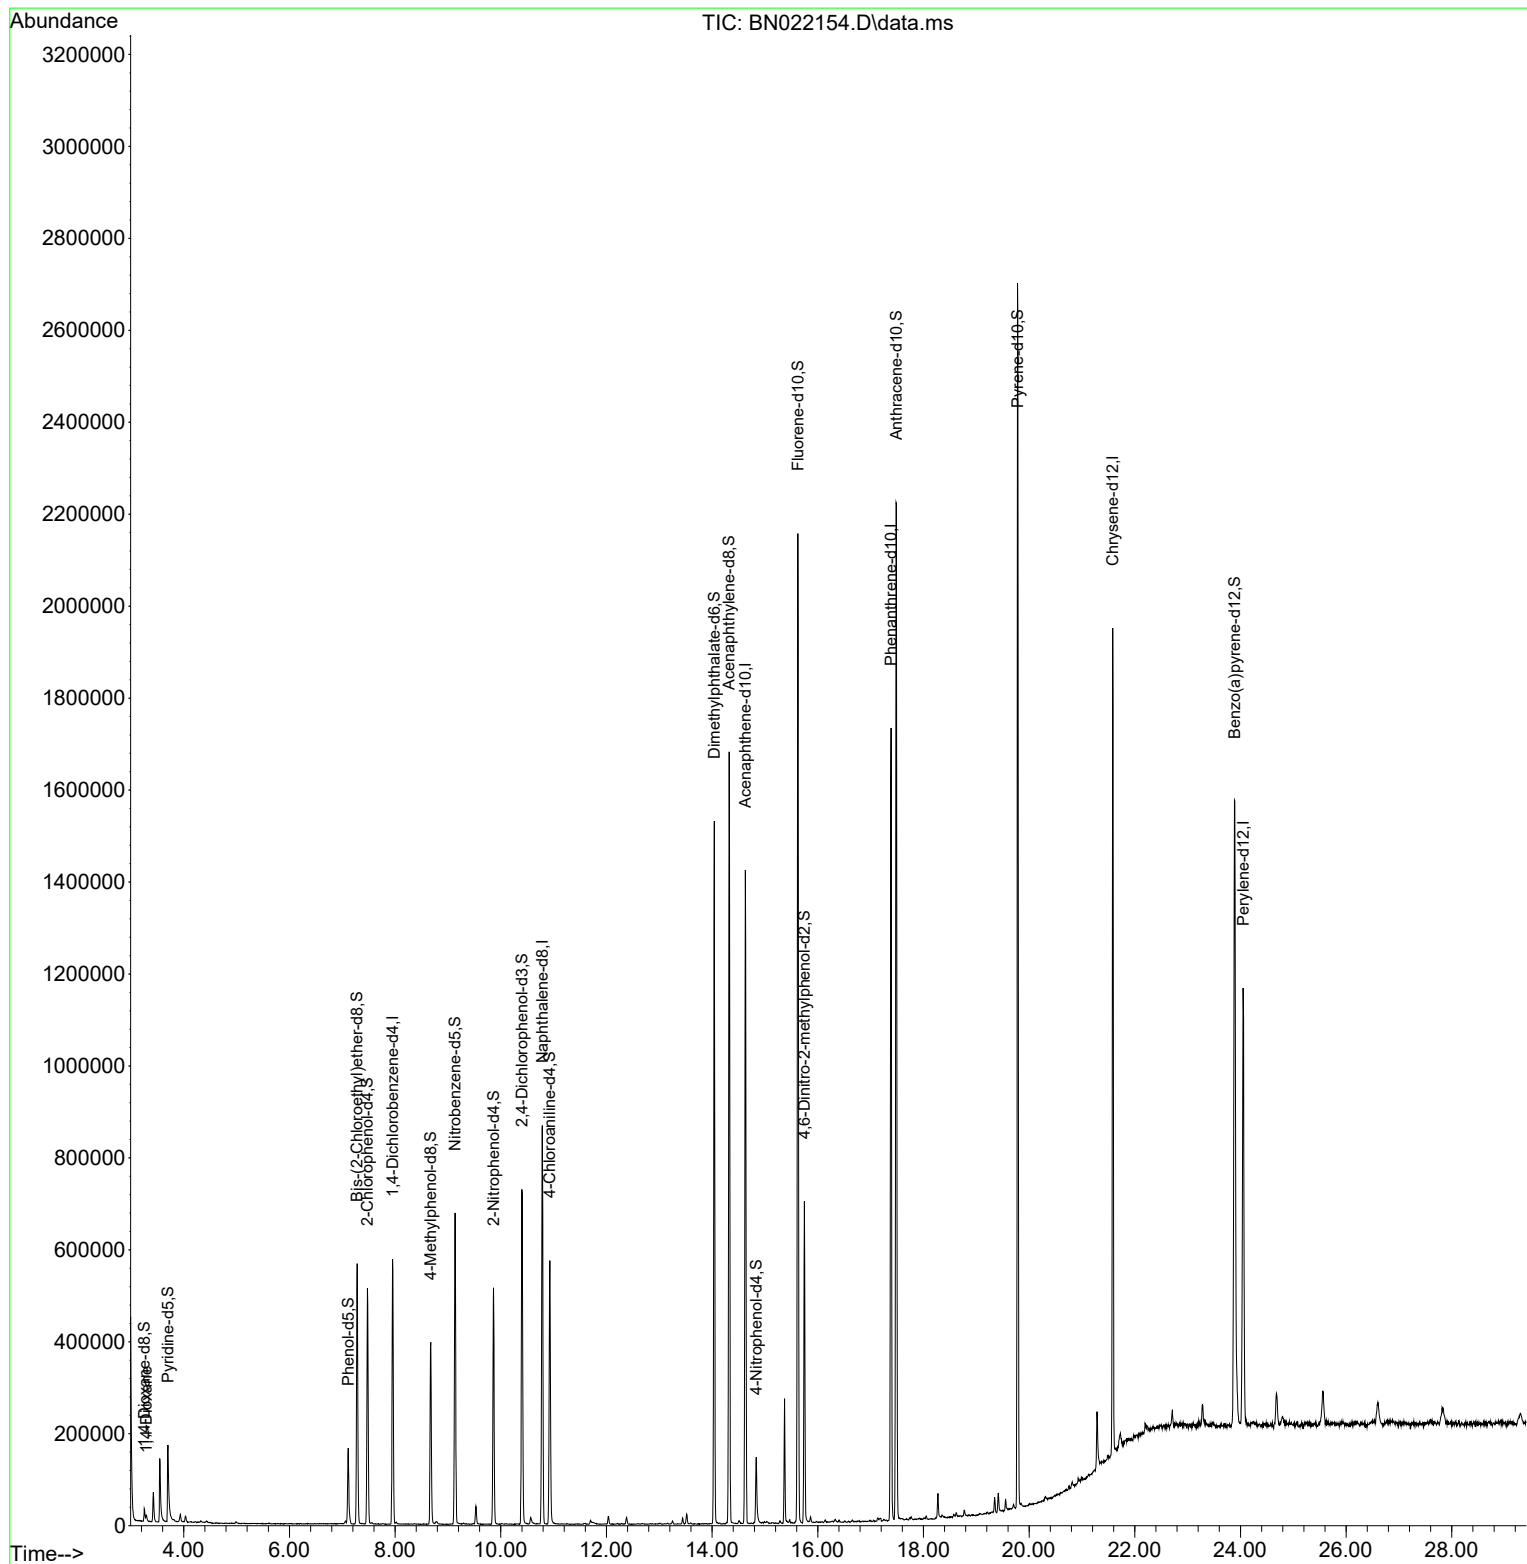

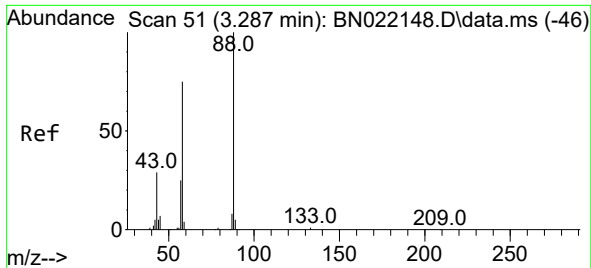

#2
 1,4-Dioxane
 Concen: 1.675 ng/uL
 RT: 3.293 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BN022154.D
 Acq: 17 Oct 2022 16:40

Instrument :
 BNA_N
 ClientSampleId :

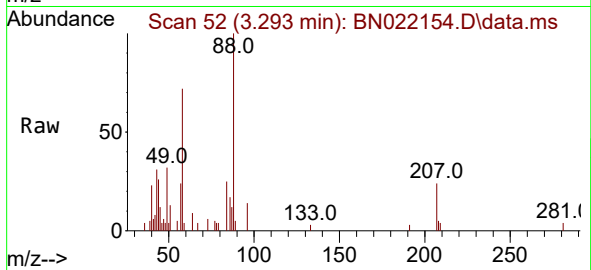

Tgt Ion: 88 Resp: 7329

Ion	Ratio	Lower	Upper
88	100		
43	30.6	22.6	34.0
58	71.6	59.9	89.9

