

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022155.D
 Acq On : 17 Oct 2022 17:18
 Operator : CG/JU
 Sample : N5060-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 17 23:10:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 13 03:08:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	169472	20.000	ng/u1	0.00
20) Naphthalene-d8	10.787	136	784071	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.628	164	487267	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.386	188	946577	20.000	ng/u1	0.00
79) Chrysene-d12	21.586	240	815932	20.000	ng/u1	0.00
88) Perylene-d12	24.057	264	679083	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	17108	3.826	ng/uL	0.00
4) Pyridine-d5	3.699	84	118802	8.541	ng/u1	0.00
7) Phenol-d5	7.110	99	105194	6.349	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	250865	24.164	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	251666	21.908	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	187611	14.251	ng/u1	0.00
21) Nitrobenzene-d5	9.134	128	160550	27.925	ng/u1	0.00
24) 2-Nitrophenol-d4	9.863	143	167082	28.354	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.404	165	302388	27.338	ng/u1	0.00
31) 4-Chloroaniline-d4	10.928	131	257528	14.240	ng/u1	0.00
46) Dimethylphthalate-d6	14.039	166	1003845	29.554	ng/u1	0.00
49) Acenaphthylene-d8	14.322	160	1133516	29.884	ng/u1	0.00
54) 4-Nitrophenol-d4	14.839	143	45045	6.213	ng/u1	0.00
60) Fluorene-d10	15.622	176	855162	29.849	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	132436	24.525	ng/u1	0.00
73) Anthracene-d10	17.480	188	1374012	33.402	ng/u1	0.00
81) Pyrene-d10	19.786	212	1452594	35.758	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.886	264	1095626	32.898	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.293	88	39430	8.091	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022155.D
Acq On : 17 Oct 2022 17:18
Operator : CG/JU
Sample : N5060-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Oct 17 23:10:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 13 03:08:08 2022
Response via : Initial Calibration

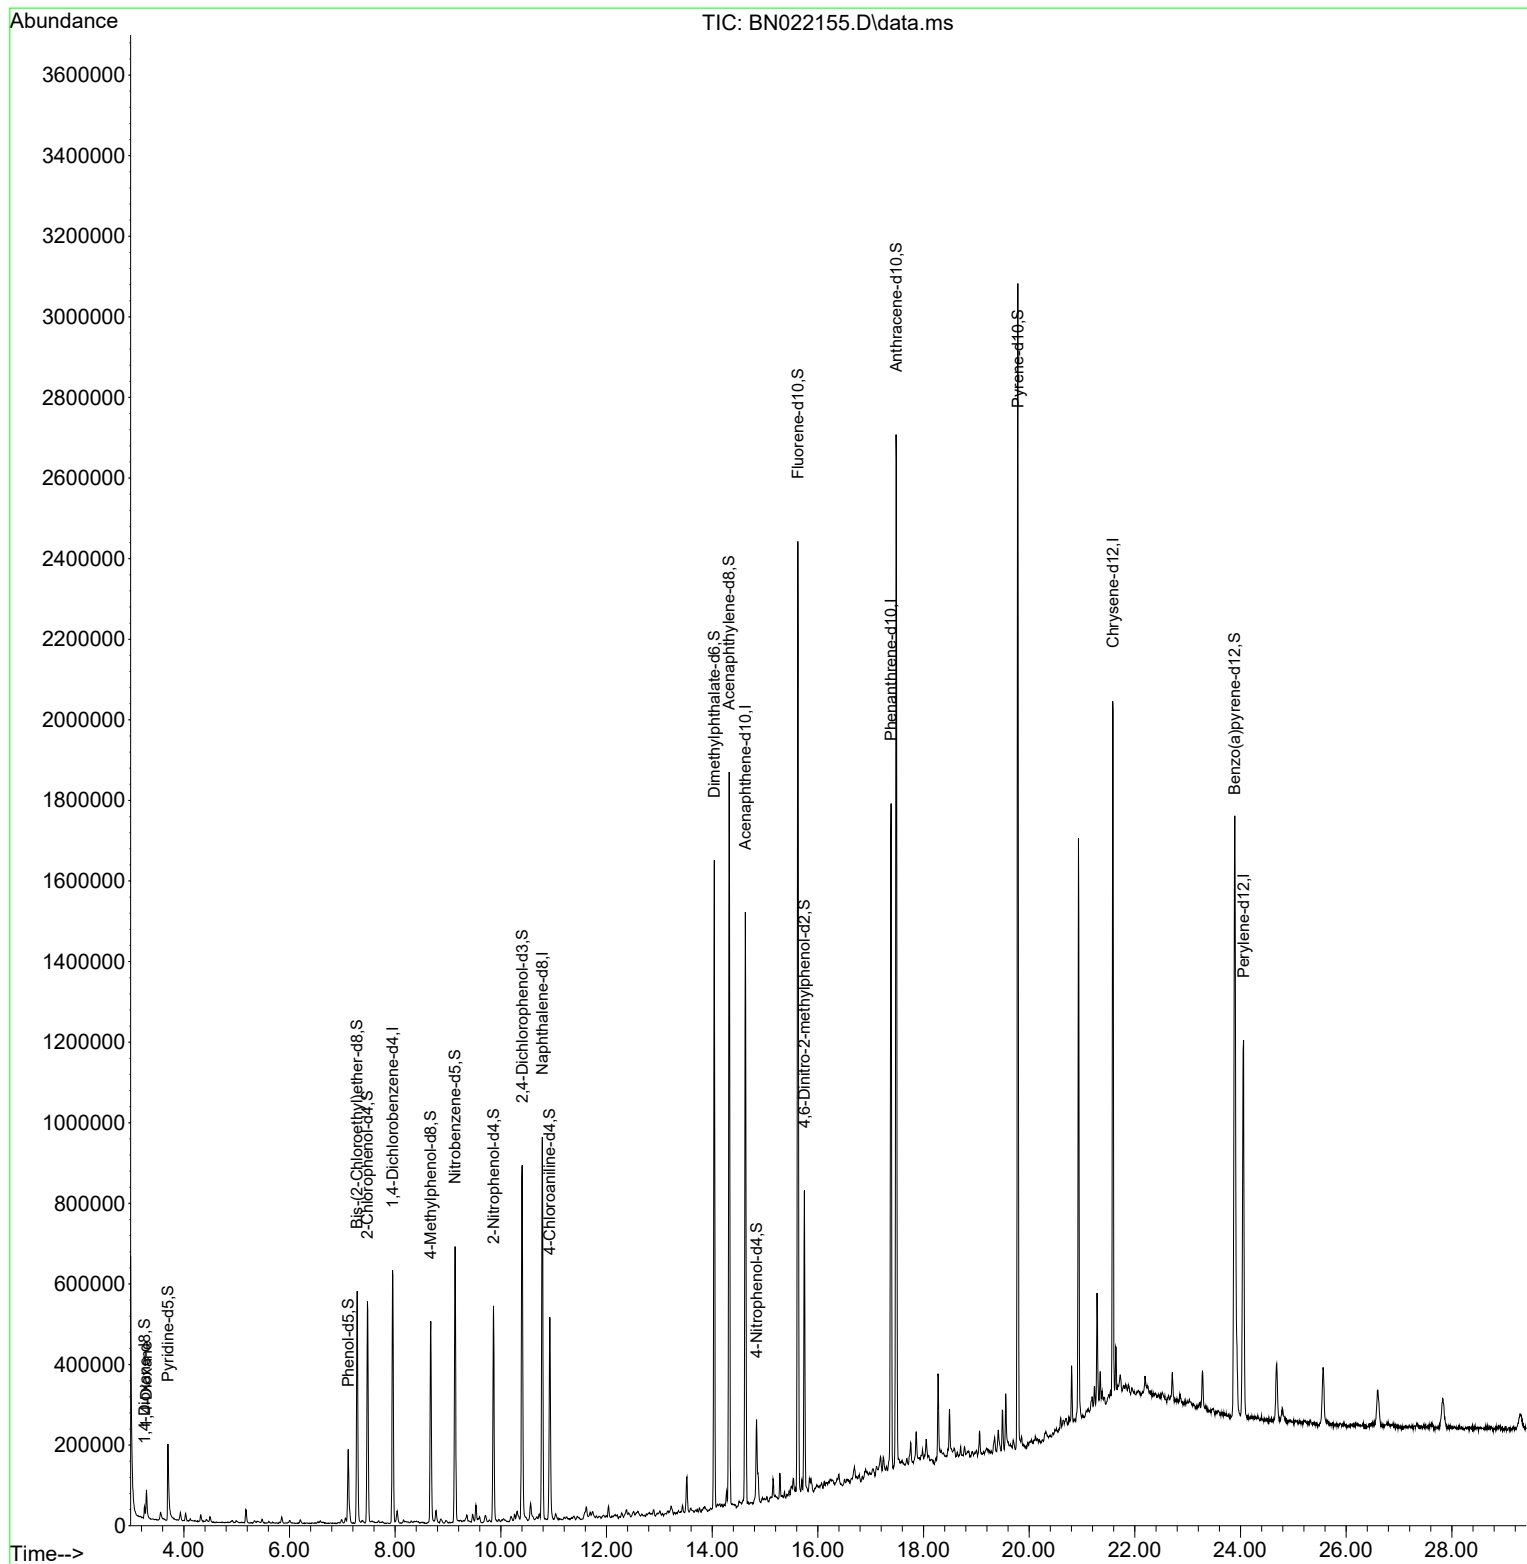

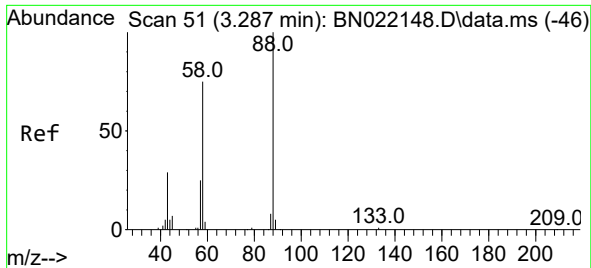

#2
 1,4-Dioxane
 Concen: 8.091 ng/uL
 RT: 3.293 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BN022155.D
 Acq: 17 Oct 2022 17:18

Instrument :
 BNA_N
 ClientSampleId :

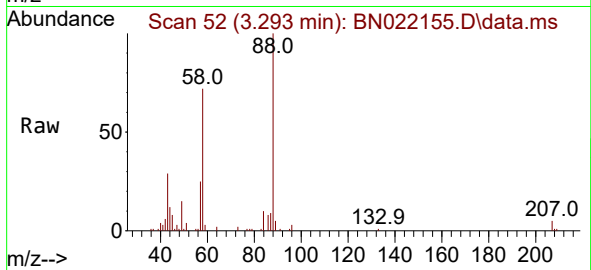

Tgt Ion: 88 Resp: 39430
 Ion Ratio Lower Upper
 88 100
 43 28.7 22.6 34.0
 58 71.8 59.9 89.9

