

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022153.D
 Acq On : 17 Oct 2022 16:02
 Operator : CG/JU
 Sample : N5060-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BC9

Quant Time: Oct 17 23:09:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 13 03:08:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	163034	20.000	ng/u1	0.00
20) Naphthalene-d8	10.787	136	776653	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.628	164	493074	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.387	188	1021201	20.000	ng/u1	0.00
79) Chrysene-d12	21.580	240	878711	20.000	ng/u1	-0.01
88) Perylene-d12	24.051	264	766292	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	17040	3.961	ng/uL	0.00
4) Pyridine-d5	3.699	84	118527	8.858	ng/u1	0.00
7) Phenol-d5	7.111	99	69914	4.387	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	263633	26.396	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	219275	19.842	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	140595	11.101	ng/u1	0.00
21) Nitrobenzene-d5	9.134	128	168978	29.672	ng/u1	0.00
24) 2-Nitrophenol-d4	9.863	143	168207	28.817	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.405	165	260431	23.769	ng/u1	0.00
31) 4-Chloroaniline-d4	10.928	131	379405	21.180	ng/u1	0.00
46) Dimethylphthalate-d6	14.040	166	997255	29.014	ng/u1	0.00
49) Acenaphthylene-d8	14.322	160	1125013	29.311	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	23962	3.266	ng/u1	0.00
60) Fluorene-d10	15.622	176	845769	29.174	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	129155	22.169	ng/u1	0.00
73) Anthracene-d10	17.481	188	1361767	30.686	ng/u1	0.00
81) Pyrene-d10	19.781	212	1481102	33.854	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.886	264	1134753	30.195	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.293	88	5083	1.084	ng/uL	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022153.D
Acq On : 17 Oct 2022 16:02
Operator : CG/JU
Sample : N5060-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BC9

Quant Time: Oct 17 23:09:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 13 03:08:08 2022
Response via : Initial Calibration

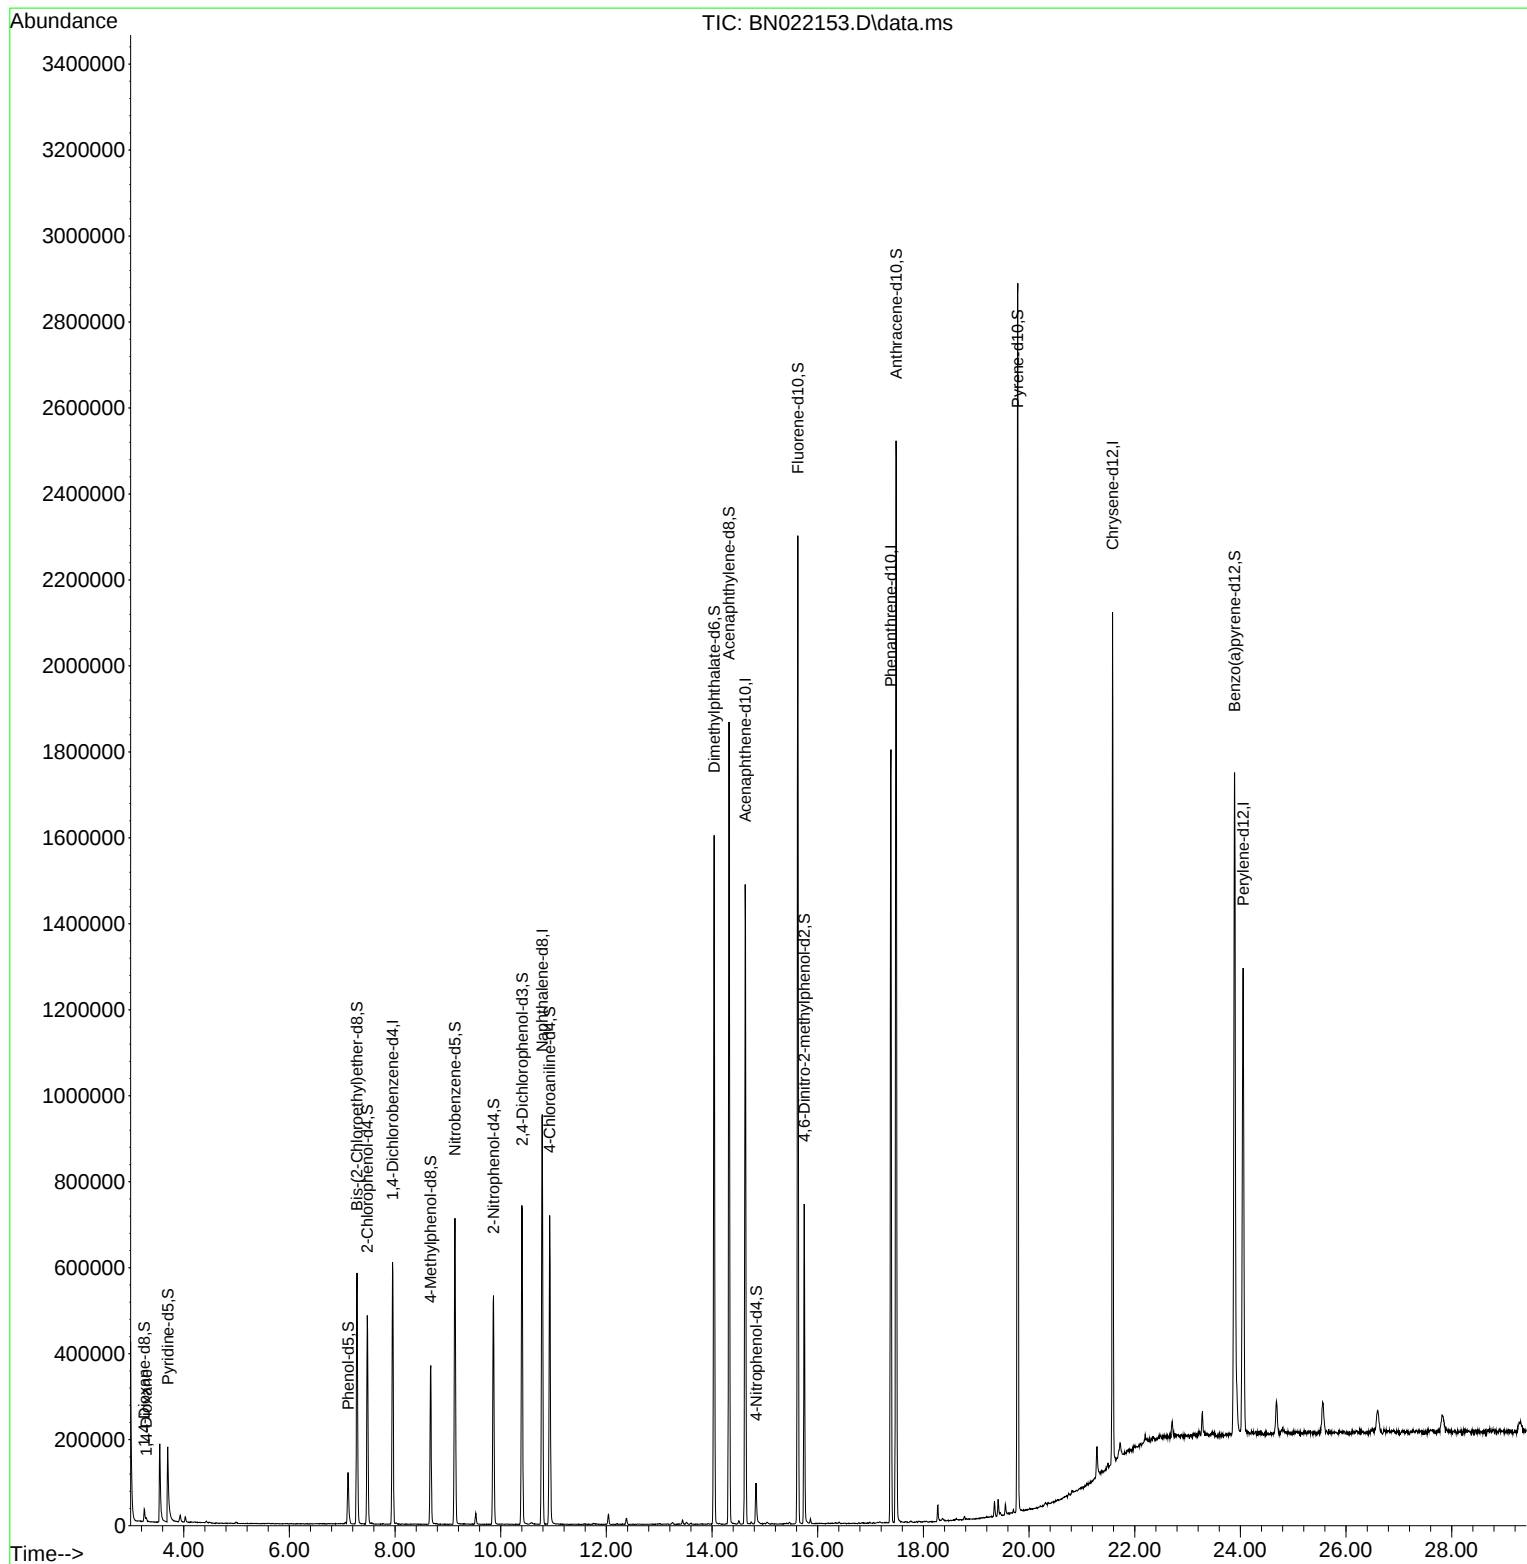

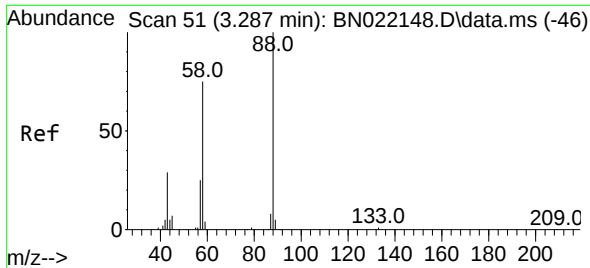

#2
 1,4-Dioxane
 Concen: 1.084 ng/uL
 RT: 3.293 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BN022153.D
 Acq: 17 Oct 2022 16:02

Instrument :
 BNA_N
 ClientSampleId :
 C1BC9

Tgt Ion: 88 Resp: 5083
 Ion Ratio Lower Upper
 88 100
 43 29.2 22.6 34.0
 58 74.3 59.9 89.9

