

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022149.D
 Acq On : 17 Oct 2022 13:31
 Operator : CG/JU
 Sample : PB148299BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK299

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022149.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	57	rVB	36160	58722	1.56%	0.140%
2	3.693	117	120	138	rBV	489432	848165	22.57%	2.027%
3	4.028	173	177	183	rVB	9971	15331	0.41%	0.037%
4	7.110	694	701	715	rVB	688587	1090273	29.02%	2.605%
5	7.281	723	730	743	rVB	543557	875584	23.30%	2.092%
6	7.475	756	763	774	rBV	664285	1060993	28.24%	2.535%
7	7.952	837	844	857	rVB	622599	987917	26.29%	2.360%
8	8.669	959	966	979	rBV	833781	1389027	36.97%	3.319%
9	9.134	1037	1045	1055	rBV	666908	1097940	29.22%	2.623%
10	9.857	1160	1168	1180	rBV	534661	916207	24.38%	2.189%
11	10.399	1253	1260	1272	rBV	858190	1416677	37.70%	3.385%
12	10.781	1318	1325	1333	rVB	938466	1593569	42.41%	3.808%
13	10.928	1342	1350	1366	rBV	844961	1446217	38.49%	3.456%
14	12.381	1592	1597	1604	rVB2	12245	20855	0.56%	0.050%
15	13.516	1785	1790	1794	rVB2	4193	6254	0.17%	0.015%
16	14.039	1872	1879	1892	rBV	1437151	2022012	53.82%	4.831%
17	14.322	1920	1927	1938	rBV2	1728990	2528175	67.29%	6.041%
18	14.628	1970	1979	1990	rBV	1498373	2184814	58.15%	5.220%
19	14.828	2007	2013	2035	rBV	738694	1115215	29.68%	2.665%
20	15.039	2045	2049	2056	rVB5	2845	5375	0.14%	0.013%
21	15.622	2141	2148	2163	rVB	2152449	3088138	82.19%	7.379%
22	15.745	2163	2169	2181	rVV	595310	813087	21.64%	1.943%
23	15.863	2185	2189	2193	rVB2	9608	12692	0.34%	0.030%
24	17.169	2407	2411	2415	rVB2	3928	4171	0.11%	0.010%
25	17.386	2441	2448	2458	rBV	1745176	2586223	68.83%	6.179%
26	17.480	2458	2464	2478	rVV2	2381137	3462693	92.16%	8.274%
27	18.363	2609	2614	2617	rBV5	2672	4337	0.12%	0.010%
28	19.345	2777	2781	2786	rBV2	25093	34889	0.93%	0.083%
29	19.416	2789	2793	2799	rVV	26254	36447	0.97%	0.087%
30	19.786	2849	2856	2867	rBV	2672430	3757291	100.00%	8.978%
31	21.486	3142	3145	3150	rBV2	29227	39154	1.04%	0.094%
32	21.580	3156	3161	3167	rBV	1864914	2367850	63.02%	5.658%
33	23.886	3546	3553	3569	rVB2	1379982	2977613	79.25%	7.115%
34	24.051	3574	3581	3590	rVB2	951284	1988326	52.92%	4.751%

Sum of corrected areas: 41852233

Instrument :

BNA_N

ClientSampleId :




SBLK299

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022149.D
Acq On : 17 Oct 2022 13:31
Operator : CG/JU
Sample : PB148299BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK299

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

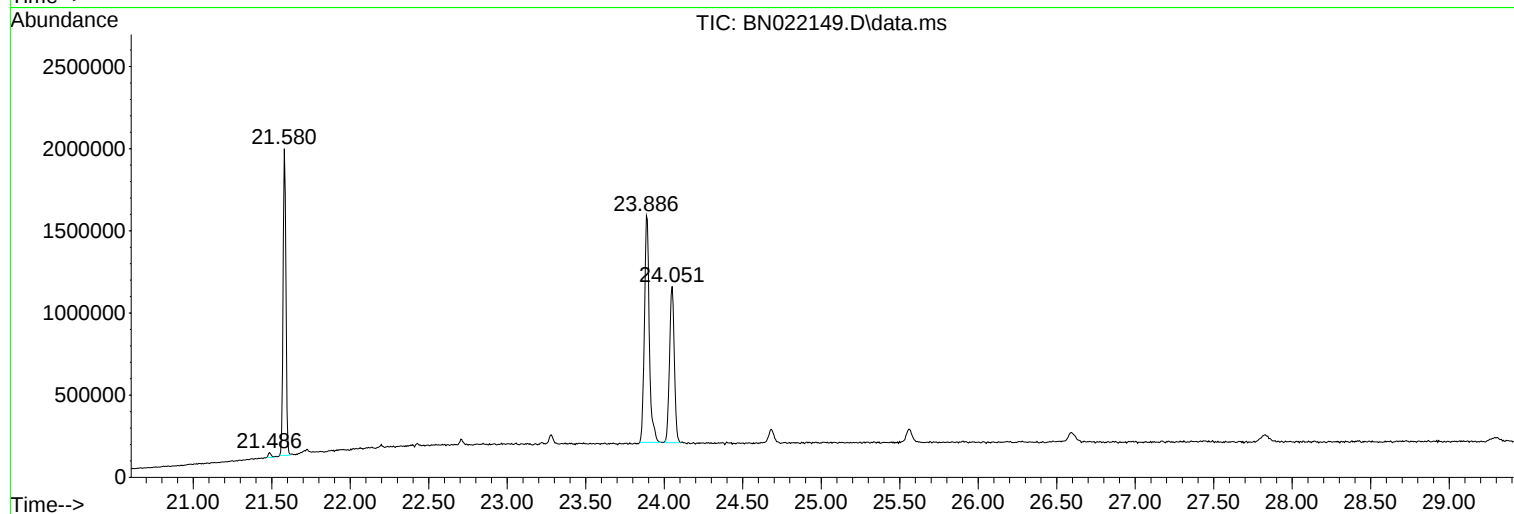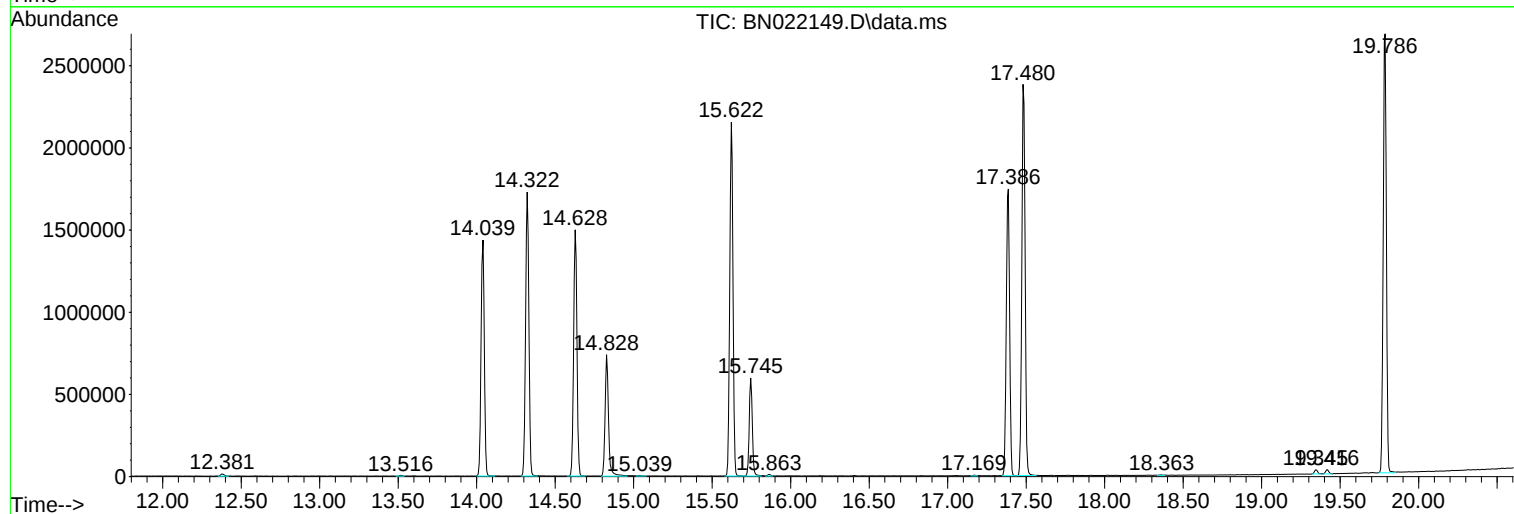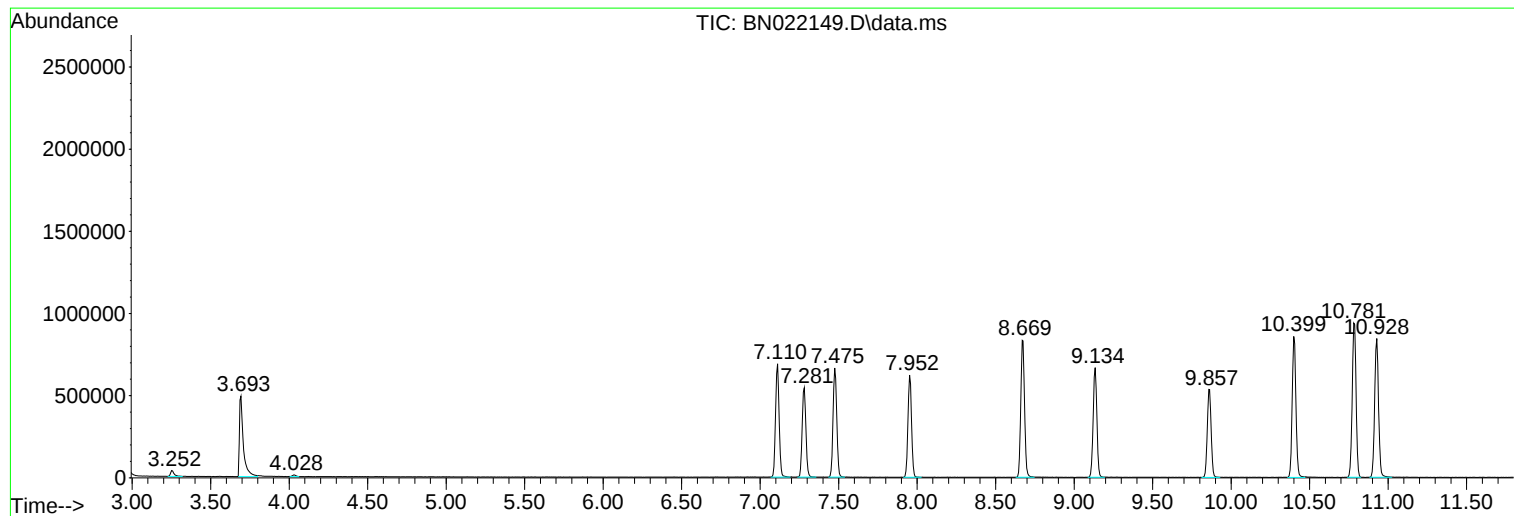

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022149.D
Acq On : 17 Oct 2022 13:31
Operator : CG/JU
Sample : PB148299BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK299

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022149.D
Acq On : 17 Oct 2022 13:31
Operator : CG/JU
Sample : PB148299BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK299

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc