

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022151.D
 Acq On : 17 Oct 2022 14:46
 Operator : CG/JU
 Sample : N5060-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	42	45	58	rVB	29484	52858	1.17%	0.127%
2	3.563	95	98	104	rBV	8763	13633	0.30%	0.033%
3	3.705	118	122	143	rBV	88278	175380	3.88%	0.421%
4	3.934	156	161	168	rBV	14766	27723	0.61%	0.066%
5	4.034	173	178	186	rVB	18666	30723	0.68%	0.074%
6	4.422	241	244	248	rBV5	3252	5003	0.11%	0.012%
7	4.987	336	340	345	rBV2	3360	5088	0.11%	0.012%
8	7.057	687	692	696	rBV2	13135	21308	0.47%	0.051%
9	7.110	696	701	713	rVB	156693	258143	5.71%	0.619%
10	7.281	722	730	745	rBV	594236	942783	20.86%	2.261%
11	7.475	757	763	772	rBV	541617	871667	19.29%	2.090%
12	7.563	775	778	783	rVB5	3777	5387	0.12%	0.013%
13	7.951	838	844	852	rBV	564484	922266	20.41%	2.211%
14	8.675	960	967	978	rBV	447953	737592	16.32%	1.769%
15	9.134	1038	1045	1052	rBV	734854	1198030	26.51%	2.873%
16	9.528	1106	1112	1117	rBV	22423	36376	0.81%	0.087%
17	9.863	1161	1169	1182	rBV	574940	955863	21.15%	2.292%
18	10.404	1253	1261	1275	rBV	817843	1407501	31.15%	3.375%
19	10.569	1285	1289	1298	rBV6	6439	16008	0.35%	0.038%
20	10.787	1318	1326	1333	rBV	863161	1483950	32.84%	3.558%
21	10.928	1342	1350	1365	rBV	584672	1008261	22.31%	2.418%
22	12.034	1534	1538	1544	rVB	12932	20337	0.45%	0.049%
23	12.381	1592	1597	1604	rVB2	15157	23762	0.53%	0.057%
24	12.981	1695	1699	1706	rVB5	2335	4630	0.10%	0.011%
25	13.251	1739	1745	1753	rVB3	8623	13924	0.31%	0.033%
26	13.516	1786	1790	1797	rVB2	8577	13862	0.31%	0.033%
27	13.598	1797	1804	1808	rBV5	2848	5137	0.11%	0.012%
28	14.039	1872	1879	1889	rBV	1739073	2374077	52.54%	5.693%
29	14.322	1920	1927	1938	rVB	1918272	2792872	61.81%	6.697%
30	14.628	1972	1979	1988	rBV	1354015	2003408	44.34%	4.804%
31	14.828	2008	2013	2033	rVB	152580	253518	5.61%	0.608%
32	15.039	2044	2049	2058	rVB6	6521	12657	0.28%	0.030%
33	15.622	2138	2148	2158	rBV	2445008	3565226	78.90%	8.549%
34	15.745	2163	2169	2181	rVV	861259	1141417	25.26%	2.737%
35	15.863	2185	2189	2193	rVV2	10546	14660	0.32%	0.035%
36	16.333	2264	2269	2273	rBV5	3108	5476	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022151.D
 Acq On : 17 Oct 2022 14:46
 Operator : CG/JU
 Sample : N5060-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

37	16.404	2276	2281	2287	rBV7	3216	5129	0.11%	0.012%
38	17.174	2407	2412	2418	rVB3	3312	5440	0.12%	0.013%
39	17.380	2441	2447	2458	rBV	1582601	2337475	51.73%	5.605%
40	17.486	2458	2465	2479	rVV	2768360	4055697	89.76%	9.725%
41	17.663	2490	2495	2499	rBV7	3028	5615	0.12%	0.013%
42	17.769	2509	2513	2521	rVB4	3916	6217	0.14%	0.015%
43	18.051	2557	2561	2566	rVB7	3815	4964	0.11%	0.012%
44	18.269	2592	2598	2605	rBV	66958	99361	2.20%	0.238%
45	18.351	2609	2612	2615	rVB	5123	6615	0.15%	0.016%
46	18.621	2653	2658	2661	rBV3	4980	7784	0.17%	0.019%
47	18.774	2678	2684	2690	rVB3	9459	13827	0.31%	0.033%
48	19.345	2776	2781	2789	rBV2	37931	53169	1.18%	0.127%
49	19.416	2789	2793	2799	rBV	40695	61089	1.35%	0.146%
50	19.551	2812	2816	2824	rBV3	37746	50941	1.13%	0.122%
51	19.786	2849	2856	2865	rBV	3285559	4518515	100.00%	10.835%
52	21.280	3107	3110	3115	rBV2	59582	92128	2.04%	0.221%
53	21.486	3142	3145	3149	rBV3	40532	46289	1.02%	0.111%
54	21.580	3156	3161	3168	rBV	1765030	2286702	50.61%	5.483%
55	23.886	3546	3553	3567	rVB2	1691126	3704182	81.98%	8.882%
56	24.045	3574	3580	3591	rVB2	918350	1923143	42.56%	4.611%




Sum of corrected areas: 41704788

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022151.D
Acq On : 17 Oct 2022 14:46
Operator : CG/JU
Sample : N5060-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

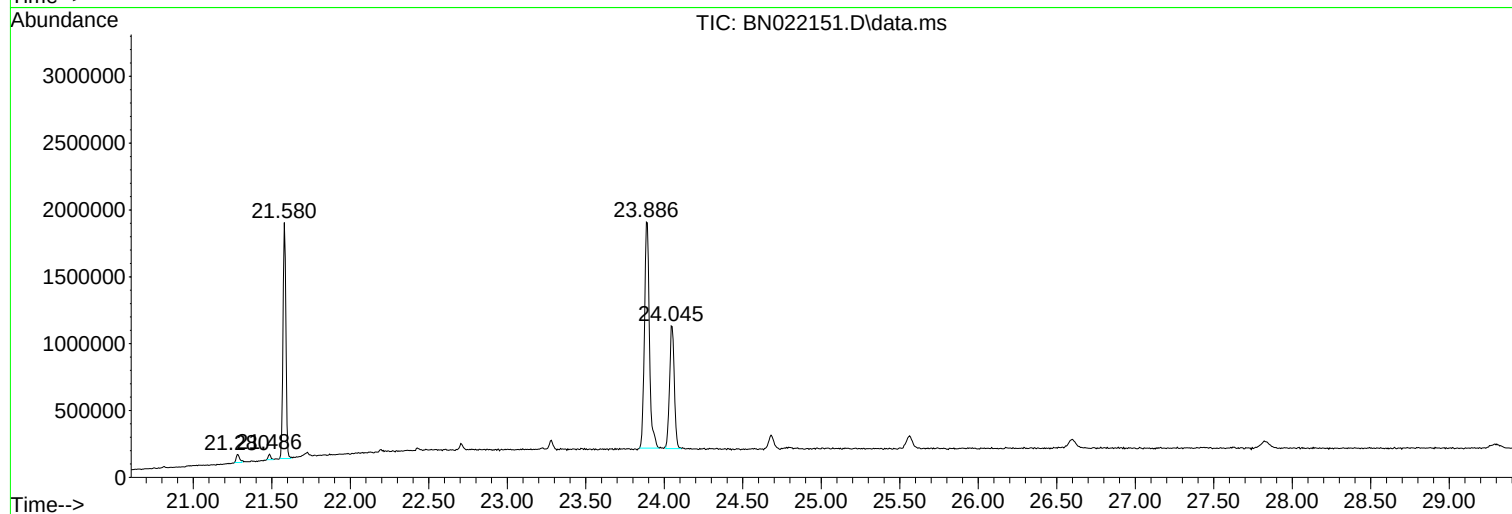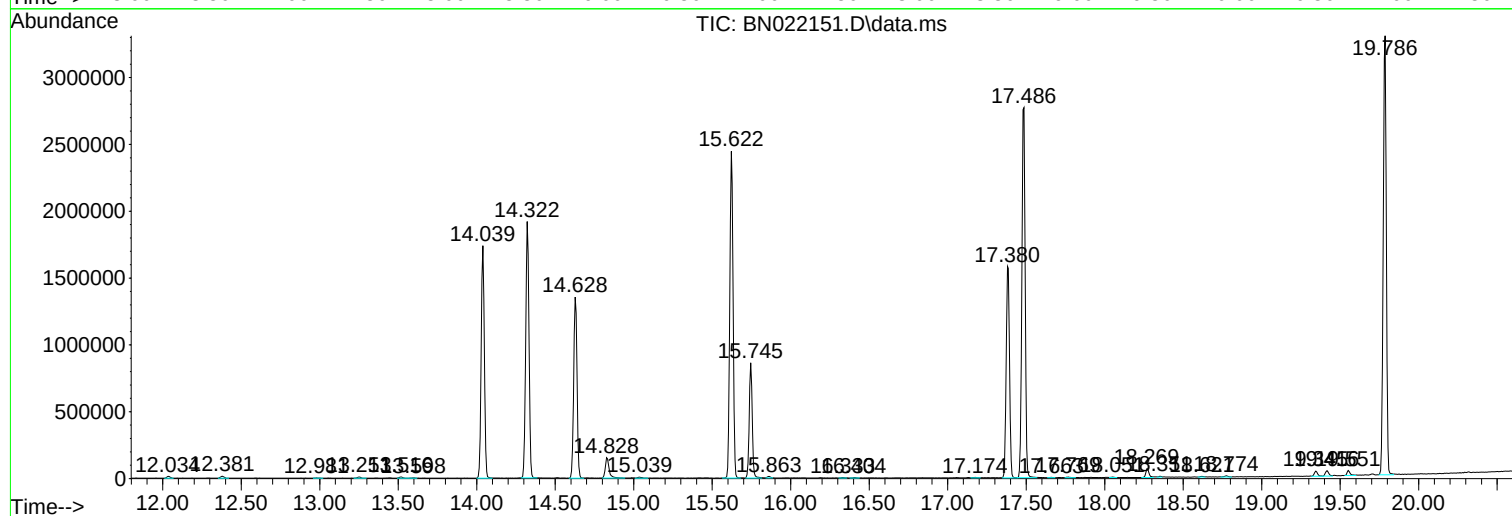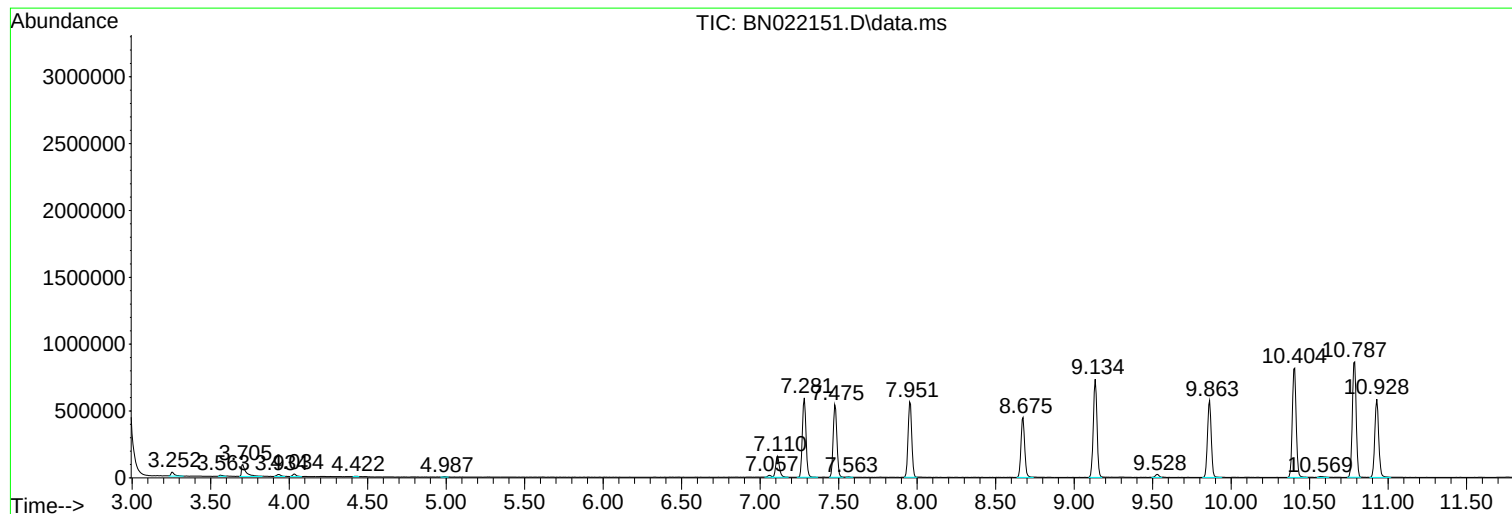

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022151.D
Acq On : 17 Oct 2022 14:46
Operator : CG/JU
Sample : N5060-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022151.D
Acq On : 17 Oct 2022 14:46
Operator : CG/JU
Sample : N5060-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc