

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022157.D
 Acq On : 17 Oct 2022 18:34
 Operator : CG/JU
 Sample : N5060-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022157.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	49	rBV	31482	41543	0.82%	0.079%
2	3.293	49	52	60	rVB	21178	32055	0.63%	0.061%
3	3.570	96	99	103	rBV	5041	6140	0.12%	0.012%
4	3.699	119	121	137	rBV	137123	245789	4.86%	0.470%
5	3.811	137	140	149	rVB	13535	22543	0.45%	0.043%
6	3.934	156	161	170	rVB	19967	38716	0.77%	0.074%
7	4.034	173	178	184	rVB	12147	19419	0.38%	0.037%
8	4.269	215	218	223	rBV	11860	17756	0.35%	0.034%
9	4.322	223	227	232	rVB	9792	13996	0.28%	0.027%
10	4.422	241	244	249	rBV5	4791	6990	0.14%	0.013%
11	4.617	273	277	282	rVB5	3784	5910	0.12%	0.011%
12	4.705	288	292	295	rVB4	5480	7653	0.15%	0.015%
13	4.987	337	340	344	rBV	4020	6560	0.13%	0.013%
14	5.099	354	359	365	rBV4	4983	9741	0.19%	0.019%
15	7.111	694	701	711	rVB	227092	384929	7.61%	0.736%
16	7.281	722	730	742	rBV	791768	1250651	24.73%	2.393%
17	7.475	756	763	771	rBV	745453	1193729	23.61%	2.284%
18	7.952	836	844	852	rBV	707276	1138396	22.51%	2.178%
19	8.022	852	856	858	rVV3	3961	5166	0.10%	0.010%
20	8.675	959	967	976	rBV	596295	969011	19.16%	1.854%
21	8.775	976	984	994	rVB	17505	36850	0.73%	0.070%
22	9.134	1037	1045	1055	rBV	969892	1573451	31.12%	3.010%
23	9.299	1067	1073	1077	rVB4	6079	9238	0.18%	0.018%
24	9.475	1098	1103	1107	rBV2	4714	7839	0.16%	0.015%
25	9.528	1107	1112	1117	rVV2	12940	22676	0.45%	0.043%
26	9.569	1117	1119	1127	rVB3	4911	6249	0.12%	0.012%
27	9.863	1161	1169	1182	rBV	762590	1281919	25.35%	2.452%
28	10.022	1189	1196	1203	rBV2	6351	12042	0.24%	0.023%
29	10.081	1203	1206	1212	rBV7	4027	6894	0.14%	0.013%
30	10.404	1253	1261	1274	rBV	1083647	1866225	36.91%	3.570%
31	10.563	1283	1288	1298	rBV	38219	73347	1.45%	0.140%
32	10.781	1315	1325	1333	rVB	1062578	1821043	36.02%	3.484%
33	10.928	1343	1350	1366	rBV	466916	804759	15.92%	1.540%
34	11.246	1399	1404	1410	rVB7	6878	13836	0.27%	0.026%
35	11.322	1413	1417	1424	rVB9	3430	6506	0.13%	0.012%
36	11.581	1454	1461	1463	rBV6	4789	9275	0.18%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022157.D
 Acq On : 17 Oct 2022 18:34
 Operator : CG/JU
 Sample : N5060-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

37	11.610	1463	1466	1475	rVB4	8266	12982	0.26%	0.025%
38	11.704	1475	1482	1485	rBV5	5145	12181	0.24%	0.023%
39	11.740	1485	1488	1495	rVB7	4799	10421	0.21%	0.020%
40	11.957	1522	1525	1532	rVB7	2984	5555	0.11%	0.011%
41	12.034	1532	1538	1543	rBV2	3937	6569	0.13%	0.013%
42	12.381	1590	1597	1602	rVV	21631	35674	0.71%	0.068%
43	13.251	1739	1745	1749	rVB2	9236	14666	0.29%	0.028%
44	13.440	1773	1777	1781	rBV	8805	11820	0.23%	0.023%
45	13.516	1784	1790	1796	rBV2	18305	29140	0.58%	0.056%
46	13.581	1797	1801	1808	rVB5	11438	20251	0.40%	0.039%
47	13.834	1837	1844	1848	rBV10	5895	14789	0.29%	0.028%
48	14.040	1872	1879	1886	rBV	2086088	2889391	57.14%	5.528%
49	14.187	1900	1904	1909	rBV8	3606	7086	0.14%	0.014%
50	14.263	1914	1917	1920	rVV4	5029	6639	0.13%	0.013%
51	14.322	1920	1927	1938	rVB	2305916	3440392	68.04%	6.582%
52	14.510	1953	1959	1963	rBV4	16409	31441	0.62%	0.060%
53	14.628	1972	1979	1989	rBV	1676406	2451527	48.48%	4.690%
54	14.834	2002	2014	2030	rBV	212797	386625	7.65%	0.740%
55	14.987	2035	2040	2044	rVV2	18214	27803	0.55%	0.053%
56	15.034	2044	2048	2055	rVB5	18409	29460	0.58%	0.056%
57	15.210	2072	2078	2082	rBV	8531	13809	0.27%	0.026%
58	15.287	2084	2091	2094	rBV3	16903	25059	0.50%	0.048%
59	15.369	2101	2105	2110	rBV	39173	51970	1.03%	0.099%
60	15.416	2110	2113	2117	rVV2	6141	8582	0.17%	0.016%
61	15.463	2118	2121	2125	rVB3	6949	8442	0.17%	0.016%
62	15.622	2142	2148	2154	rBV	2997068	4259952	84.25%	8.149%
63	15.745	2163	2169	2181	rBV	1023643	1386654	27.42%	2.653%
64	15.863	2183	2189	2198	rVB5	21744	42754	0.85%	0.082%
65	15.969	2204	2207	2212	rVB7	8529	15348	0.30%	0.029%
66	16.139	2230	2236	2242	rBV	25353	46973	0.93%	0.090%
67	16.269	2255	2258	2259	rBV3	6349	6990	0.14%	0.013%
68	16.328	2264	2268	2271	rVV5	10554	14512	0.29%	0.028%
69	16.398	2277	2280	2290	rVB10	10822	22272	0.44%	0.043%
70	16.586	2310	2312	2318	rVB4	4871	6653	0.13%	0.013%
71	16.651	2318	2323	2327	rBV	17417	27776	0.55%	0.053%
72	16.769	2340	2343	2351	rVB7	7261	11322	0.22%	0.022%
73	16.834	2352	2354	2359	rBV5	4567	6713	0.13%	0.013%
74	17.139	2402	2406	2409	rBV4	16100	24923	0.49%	0.048%
75	17.186	2411	2414	2418	rVB4	23823	32924	0.65%	0.063%
76	17.257	2421	2426	2430	rBV4	11092	21526	0.43%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022157.D
 Acq On : 17 Oct 2022 18:34
 Operator : CG/JU
 Sample : N5060-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

77	17.386	2441	2448	2458	rBV	1993954	3053860	60.40%	5.842%
78	17.481	2458	2464	2475	rVB2	2953867	4453702	88.08%	8.520%
79	17.592	2480	2483	2494	rVB8	20482	43739	0.87%	0.084%
80	17.739	2504	2508	2511	rBV2	43894	62920	1.24%	0.120%
81	18.051	2559	2561	2565	rVB5	13913	13887	0.27%	0.027%
82	18.275	2595	2599	2609	rBV	211056	295440	5.84%	0.565%
83	18.622	2654	2658	2663	rBV4	16786	27151	0.54%	0.052%
84	18.775	2680	2684	2690	rBV2	30681	43154	0.85%	0.083%
85	18.898	2702	2705	2708	rBV3	20944	25214	0.50%	0.048%
86	18.939	2709	2712	2716	rVV	38873	43182	0.85%	0.083%
87	18.980	2716	2719	2722	rVV	22644	24435	0.48%	0.047%
88	19.345	2777	2781	2787	rVB2	48662	71640	1.42%	0.137%
89	19.416	2788	2793	2797	rBV	73383	116791	2.31%	0.223%
90	19.557	2813	2817	2827	rBV	128010	206156	4.08%	0.394%
91	19.786	2849	2856	2869	rBV	3716636	5056315	100.00%	9.673%
92	20.933	3047	3051	3056	rBV2	93829	116834	2.31%	0.224%
93	21.280	3106	3110	3118	rBV	196868	289441	5.72%	0.554%
94	21.580	3156	3161	3168	rBV	2133866	2885329	57.06%	5.520%
95	23.892	3546	3554	3568	rBV2	2022368	4303550	85.11%	8.233%
96	24.051	3574	3581	3595	rVB2	1188848	2466413	48.78%	4.718%
97	24.686	3685	3689	3698	rVB	112074	225011	4.45%	0.430%




Sum of corrected areas: 52272572

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022157.D
Acq On : 17 Oct 2022 18:34
Operator : CG/JU
Sample : N5060-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

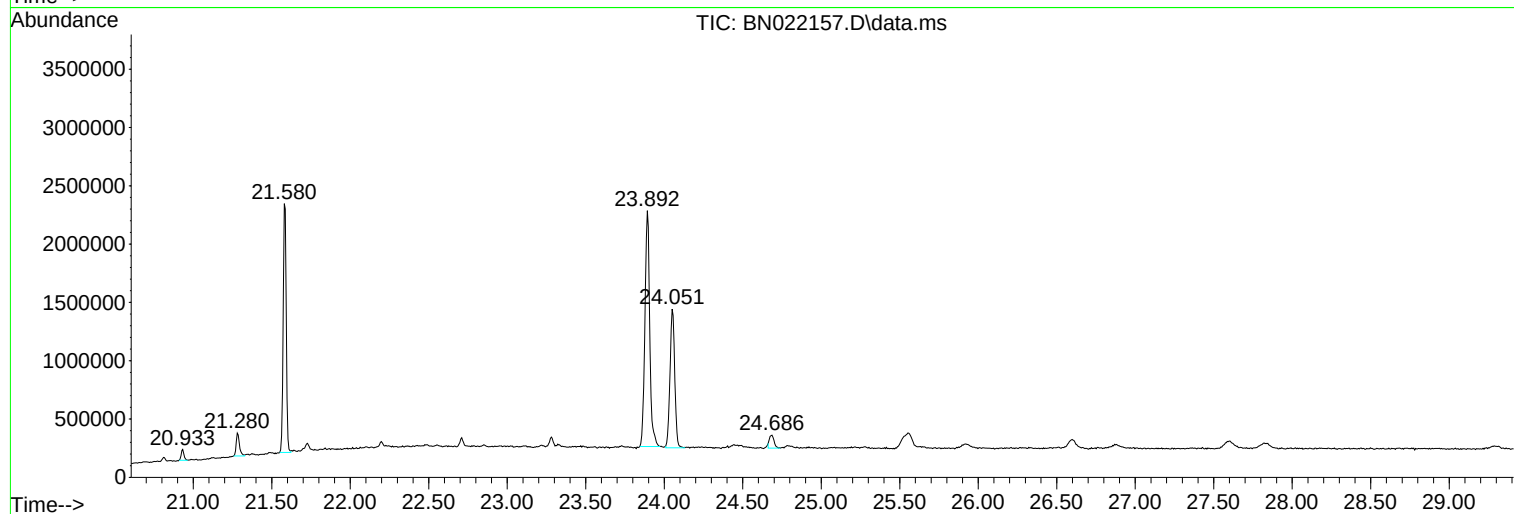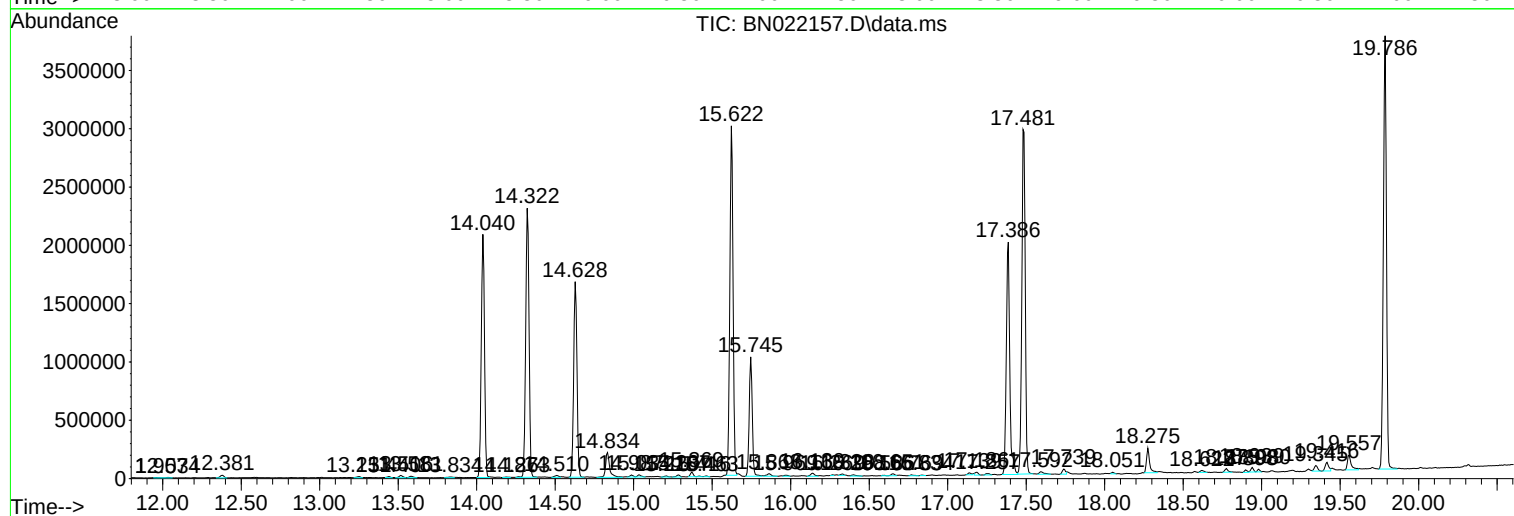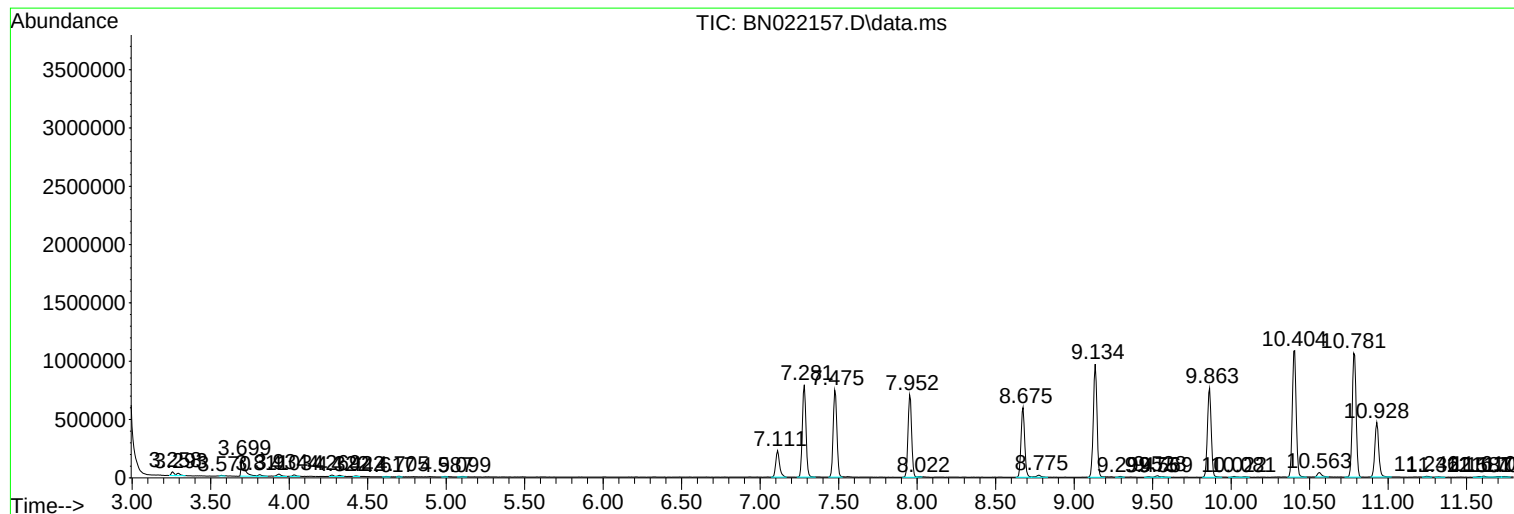

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022157.D
Acq On : 17 Oct 2022 18:34
Operator : CG/JU
Sample : N5060-12
Misc :
ALS Vial : 11 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
C1BD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentadecafluorooctanoic aci... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.280	2.01 ng/ul	289441	Chrysene-d12	21.580	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	94
2	Nonadecyl trifluoroacetate	380	C21H39F3O2	1000351-76-3	91
3	17-Pentatriacontene	491	C35H70	006971-40-0	91
4	Hexadecyl propyl ether	284	C19H40O	1000406-27-9	91
5	Pentafluoropropionic acid, hepta...	402	C20H35F5O2	959218-78-1	91

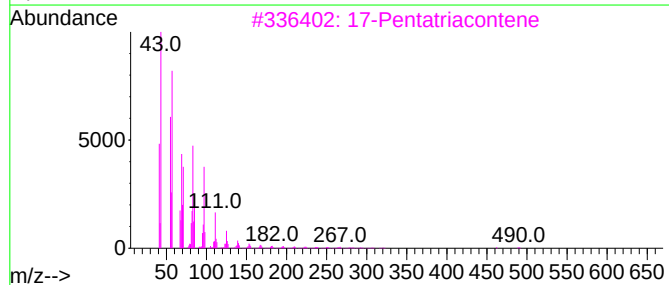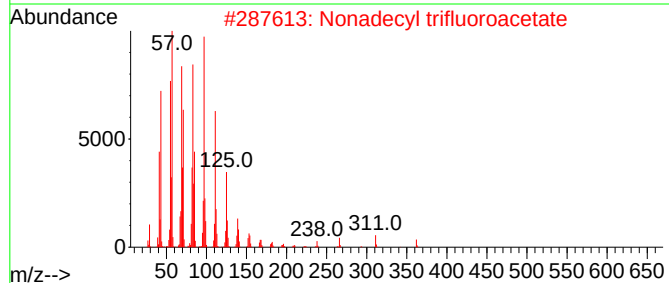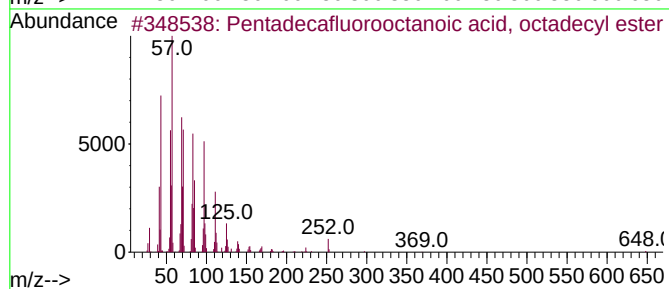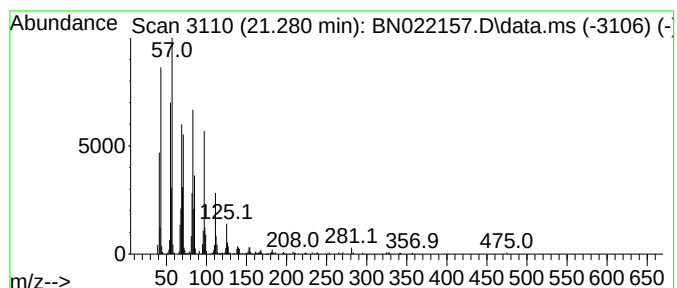

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022157.D
Acq On : 17 Oct 2022 18:34
Operator : CG/JU
Sample : N5060-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentadecafluoro...	21.280	2.0	ng/u1	289441	5	21.580	2885330	20.0