

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022162.D
 Acq On : 17 Oct 2022 21:42
 Operator : CG/JU
 Sample : N5060-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	58	rVB	32938	54968	1.04%	0.115%
2	3.569	96	99	104	rVB	5082	6076	0.11%	0.013%
3	3.699	118	121	137	rBV	163866	287090	5.43%	0.601%
4	3.934	156	161	172	rVB2	18252	36910	0.70%	0.077%
5	4.028	173	177	185	rVB	12094	17798	0.34%	0.037%
6	4.428	241	245	250	rVB7	5457	7936	0.15%	0.017%
7	4.993	337	341	345	rBV3	3751	6041	0.11%	0.013%
8	7.110	694	701	713	rVB	172146	290841	5.50%	0.609%
9	7.281	720	730	743	rBV	641423	1034121	19.57%	2.166%
10	7.475	756	763	772	rBV	597200	956776	18.11%	2.004%
11	7.557	774	777	782	rVB4	4145	6402	0.12%	0.013%
12	7.951	836	844	853	rBV	672490	1062051	20.10%	2.225%
13	8.034	853	858	863	rVB4	6880	14743	0.28%	0.031%
14	8.669	958	966	976	rBV	460012	768319	14.54%	1.610%
15	9.134	1036	1045	1056	rBV	791908	1305371	24.70%	2.735%
16	9.240	1058	1063	1069	rVV4	4508	10632	0.20%	0.022%
17	9.298	1069	1073	1077	rVB4	4204	6906	0.13%	0.014%
18	9.528	1106	1112	1116	rBV	12618	20187	0.38%	0.042%
19	9.857	1161	1168	1180	rBV	614194	1027627	19.45%	2.153%
20	10.398	1253	1260	1272	rBV	944493	1594452	30.17%	3.340%
21	10.563	1282	1288	1295	rBV2	18740	37126	0.70%	0.078%
22	10.781	1317	1325	1335	rBV	1013671	1705651	32.28%	3.573%
23	10.928	1342	1350	1363	rBV	695528	1239698	23.46%	2.597%
24	11.581	1457	1461	1465	rBV7	3152	6333	0.12%	0.013%
25	11.698	1475	1481	1487	rBV3	6238	13734	0.26%	0.029%
26	11.763	1487	1492	1502	rVB3	11204	23913	0.45%	0.050%
27	12.034	1531	1538	1547	rVB3	10669	16965	0.32%	0.036%
28	12.375	1589	1596	1605	rVB	16476	30166	0.57%	0.063%
29	13.251	1737	1745	1750	rBV3	4116	10854	0.21%	0.023%
30	13.439	1772	1777	1783	rVB5	5566	8448	0.16%	0.018%
31	13.516	1783	1790	1797	rVV4	12582	22747	0.43%	0.048%
32	13.598	1797	1804	1812	rVB5	3321	6773	0.13%	0.014%
33	13.798	1833	1838	1843	rBV5	2349	5349	0.10%	0.011%
34	14.039	1871	1879	1891	rBV	1933489	2623503	49.65%	5.496%
35	14.269	1913	1918	1920	rBV5	4589	6144	0.12%	0.013%
36	14.322	1920	1927	1939	rVB	2098249	3063051	57.96%	6.417%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022162.D
 Acq On : 17 Oct 2022 21:42
 Operator : CG/JU
 Sample : N5060-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BC3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

37	14.510	1955	1959	1965	rVB3	4787	6698	0.13%	0.014%
38	14.628	1969	1979	1994	rVV	1629893	2346972	44.41%	4.917%
39	14.833	2008	2014	2025	rBV	174282	280203	5.30%	0.587%
40	15.033	2043	2048	2056	rVB5	11632	23607	0.45%	0.049%
41	15.416	2110	2113	2118	rBV3	4544	5916	0.11%	0.012%
42	15.622	2141	2148	2159	rVV	2804274	3918936	74.16%	8.210%
43	15.745	2162	2169	2184	rBV	928853	1255577	23.76%	2.630%
44	15.863	2184	2189	2196	rVB2	14770	23550	0.45%	0.049%
45	16.086	2223	2227	2231	rVB5	6025	8991	0.17%	0.019%
46	16.327	2264	2268	2271	rBV5	4599	7348	0.14%	0.015%
47	16.404	2276	2281	2284	rBV4	6921	11828	0.22%	0.025%
48	16.510	2293	2299	2304	rBV3	21216	34101	0.65%	0.071%
49	16.698	2327	2331	2339	rVB7	10559	19977	0.38%	0.042%
50	17.169	2408	2411	2419	rVB4	4983	9390	0.18%	0.020%
51	17.380	2441	2447	2458	rBV	1895209	2768770	52.39%	5.801%
52	17.486	2458	2465	2478	rBV2	3031207	4448248	84.18%	9.319%
53	17.916	2534	2538	2542	rBV7	2953	5724	0.11%	0.012%
54	18.051	2558	2561	2565	rVB6	4779	6303	0.12%	0.013%
55	18.274	2594	2599	2604	rBV	72890	102291	1.94%	0.214%
56	18.351	2610	2612	2617	rVB2	6033	6884	0.13%	0.014%
57	18.627	2654	2659	2664	rBV5	6213	11446	0.22%	0.024%
58	18.774	2680	2684	2690	rBV2	22824	30517	0.58%	0.064%
59	19.186	2751	2754	2761	rVB10	4988	9627	0.18%	0.020%
60	19.345	2776	2781	2787	rBV	42192	59033	1.12%	0.124%
61	19.416	2788	2793	2797	rBV	49628	75804	1.43%	0.159%
62	19.551	2812	2816	2822	rBV2	41164	57588	1.09%	0.121%
63	19.704	2838	2842	2845	rBV2	13035	18960	0.36%	0.040%
64	19.786	2849	2856	2865	rVV	3750620	5284489	100.00%	11.071%
65	21.280	3106	3110	3119	rBV2	130087	208630	3.95%	0.437%
66	21.580	3156	3161	3167	rBV2	2023215	2662159	50.38%	5.577%
67	23.886	3546	3553	3569	rVB2	2068699	4378286	82.85%	9.173%
68	24.051	3573	3581	3592	rVB	1139947	2308915	43.69%	4.837%




Sum of corrected areas: 47732470

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022162.D
Acq On : 17 Oct 2022 21:42
Operator : CG/JU
Sample : N5060-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

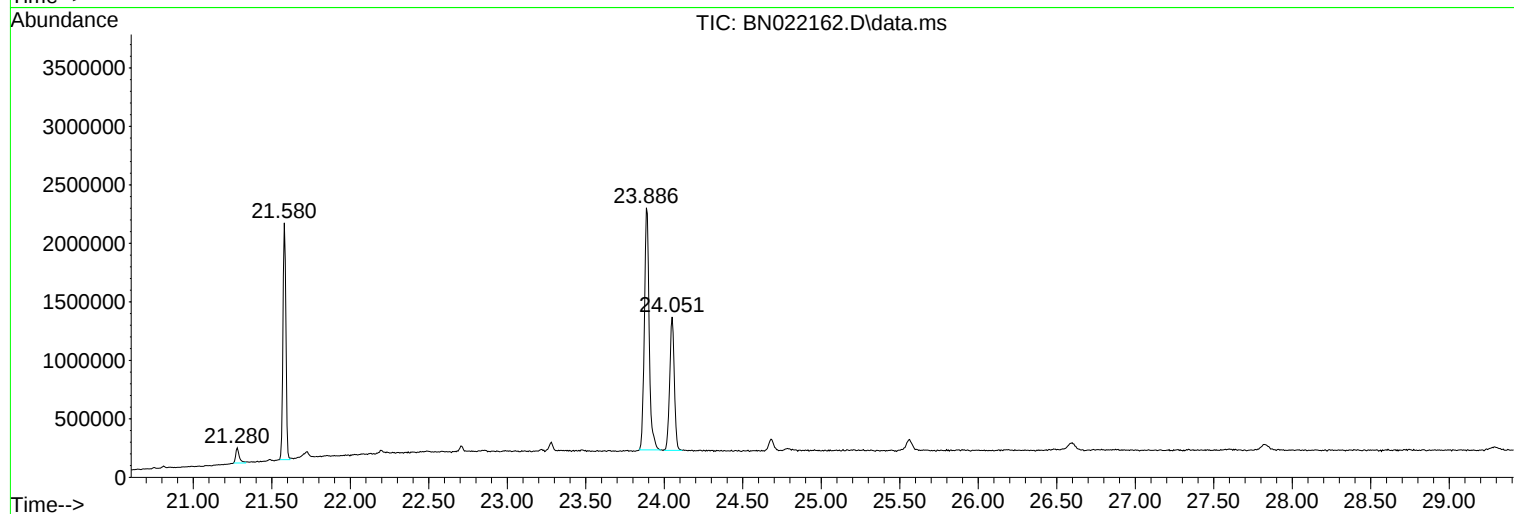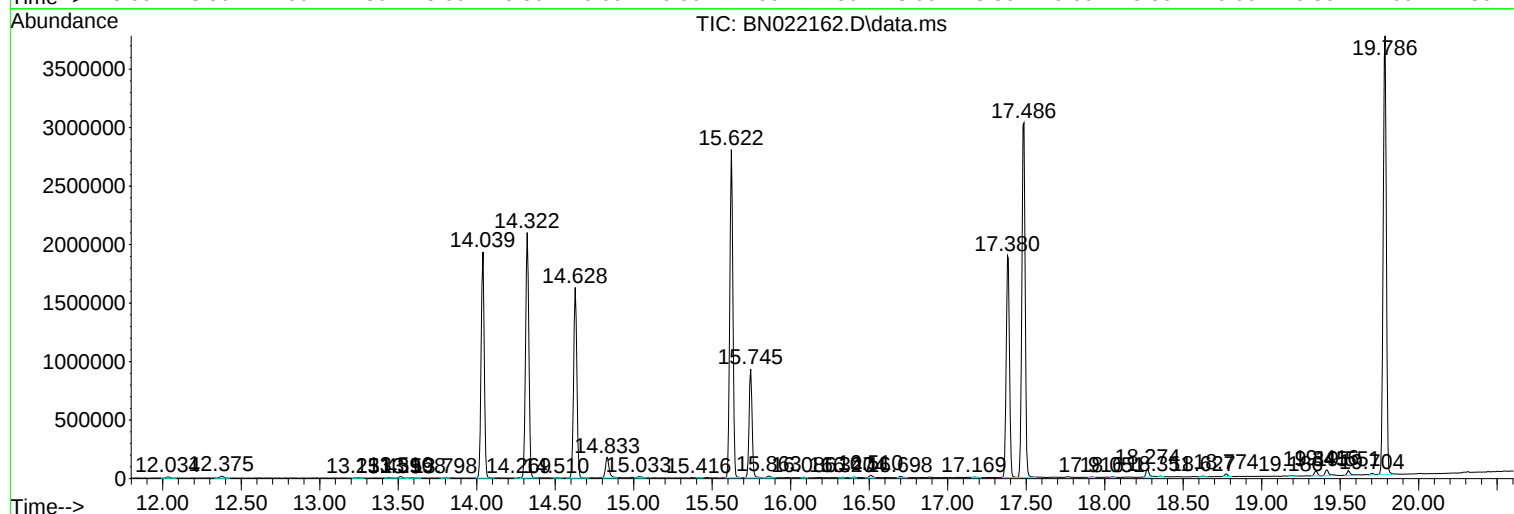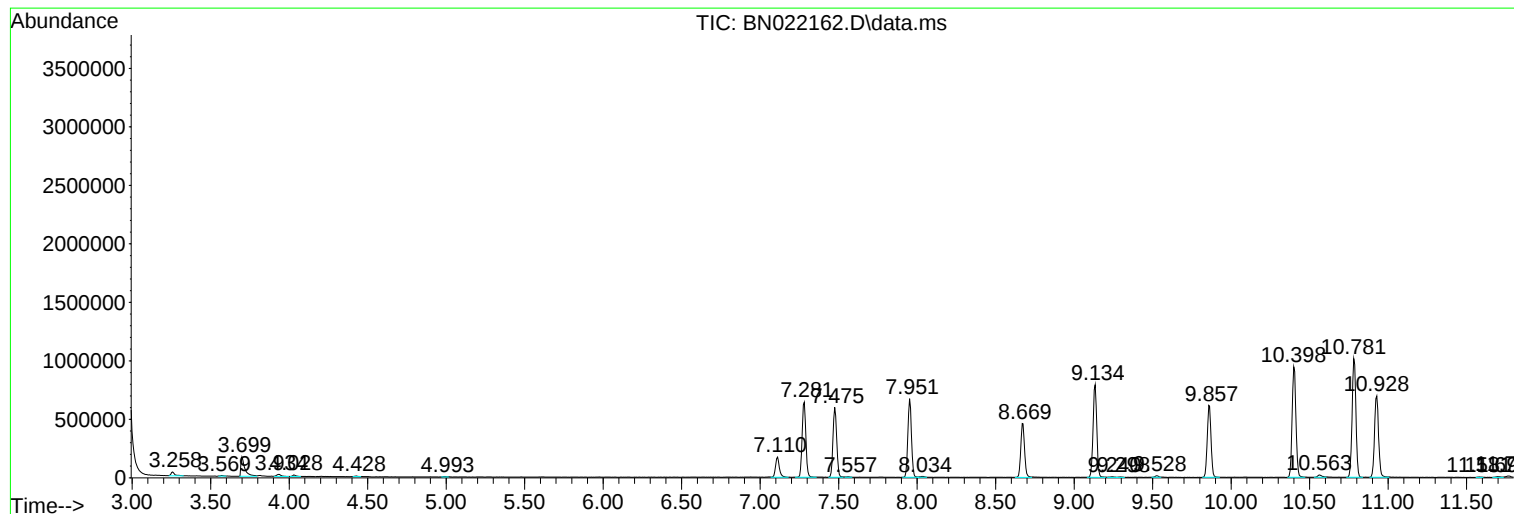

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022162.D
Acq On : 17 Oct 2022 21:42
Operator : CG/JU
Sample : N5060-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022162.D
Acq On : 17 Oct 2022 21:42
Operator : CG/JU
Sample : N5060-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
