

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022165.D
 Acq On : 18 Oct 2022 00:49
 Operator : CG/JU
 Sample : PB148277BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	56	rVB	48234	75124	1.54%	0.141%
2	3.693	117	120	146	rBV	624877	1104522	22.59%	2.080%
3	4.028	173	177	185	rVB	11578	17373	0.36%	0.033%
4	7.111	693	701	716	rBV	893372	1464993	29.97%	2.759%
5	7.275	721	729	738	rBV	736147	1160010	23.73%	2.185%
6	7.475	755	763	776	rBV	873601	1404205	28.72%	2.645%
7	7.952	837	844	856	rVB	651566	1029226	21.05%	1.939%
8	8.669	959	966	977	rBV	1158938	1853347	37.91%	3.491%
9	9.128	1037	1044	1055	rBV	888999	1456948	29.80%	2.744%
10	9.857	1161	1168	1180	rBV	755745	1242876	25.42%	2.341%
11	10.399	1252	1260	1271	rBV	1157620	1897021	38.80%	3.573%
12	10.781	1316	1325	1333	rBV	1023441	1696707	34.71%	3.196%
13	10.922	1341	1349	1365	rBV	1185685	2025690	41.43%	3.815%
14	12.375	1591	1596	1604	rBV2	19852	33508	0.69%	0.063%
15	13.510	1785	1789	1796	rBV6	2807	5321	0.11%	0.010%
16	14.040	1872	1879	1891	rBV	1940526	2747692	56.20%	5.175%
17	14.322	1919	1927	1935	rBV2	2248680	3410360	69.76%	6.424%
18	14.628	1971	1979	1989	rBV	1594993	2358597	48.24%	4.442%
19	14.828	2005	2013	2028	rBV	1037489	1525653	31.21%	2.874%
20	15.045	2043	2050	2054	rVB8	3848	6968	0.14%	0.013%
21	15.622	2141	2148	2160	rVB	2976201	4162490	85.14%	7.840%
22	15.745	2163	2169	2184	rBV	743273	1027508	21.02%	1.935%
23	15.863	2184	2189	2194	rVB	12660	19258	0.39%	0.036%
24	17.169	2407	2411	2418	rVB	3814	5023	0.10%	0.009%
25	17.381	2441	2447	2457	rBV	1993616	2787658	57.02%	5.251%
26	17.481	2457	2464	2478	rBV2	3161412	4504135	92.13%	8.484%
27	17.651	2489	2493	2499	rVB6	3917	5925	0.12%	0.011%
28	17.763	2509	2512	2517	rVB2	3974	5190	0.11%	0.010%
29	19.345	2776	2781	2788	rBV2	39002	54638	1.12%	0.103%
30	19.416	2788	2793	2800	rBV	40164	58317	1.19%	0.110%
31	19.698	2839	2841	2845	rVB5	5206	6194	0.13%	0.012%
32	19.780	2849	2855	2865	rVV	3607633	4888887	100.00%	9.208%
33	21.580	3155	3161	3168	rBV	1962922	2682499	54.87%	5.053%
34	23.886	3545	3553	3566	rBV	1931097	4057944	83.00%	7.643%
35	24.045	3573	3580	3591	rVB2	1078615	2309972	47.25%	4.351%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022165.D
Acq On : 18 Oct 2022 00:49
Operator : CG/JU
Sample : PB148277BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK277

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Title : SVOA CALIBRATION




Sum of corrected areas: 53091779

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022165.D
Acq On : 18 Oct 2022 00:49
Operator : CG/JU
Sample : PB148277BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK277

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

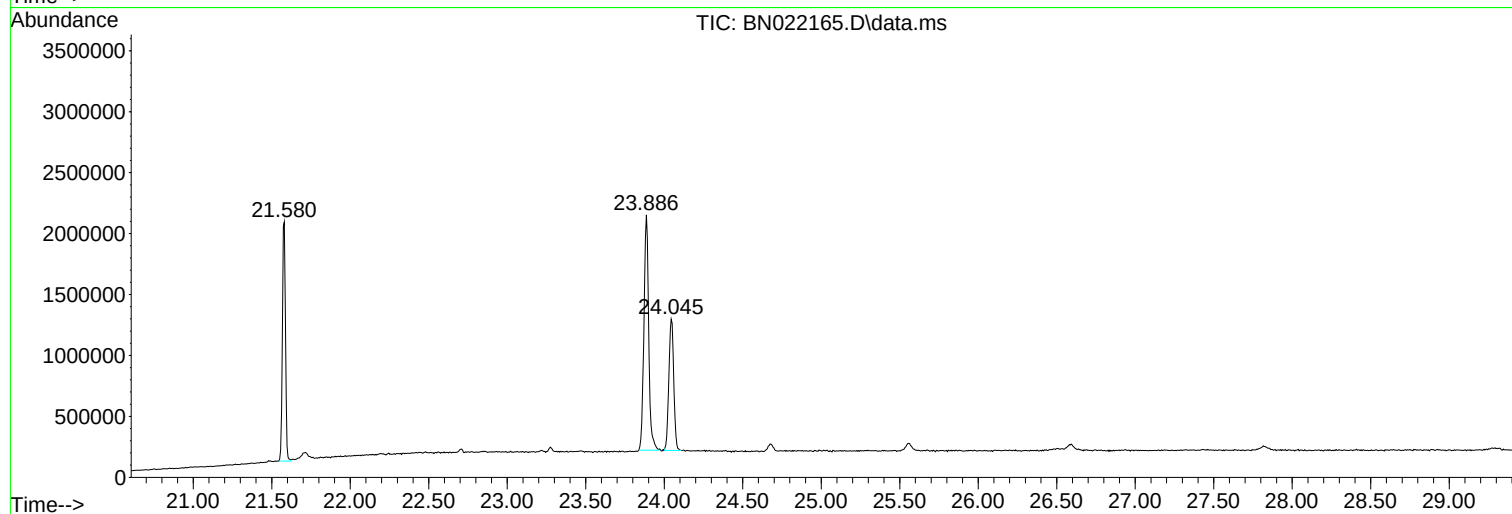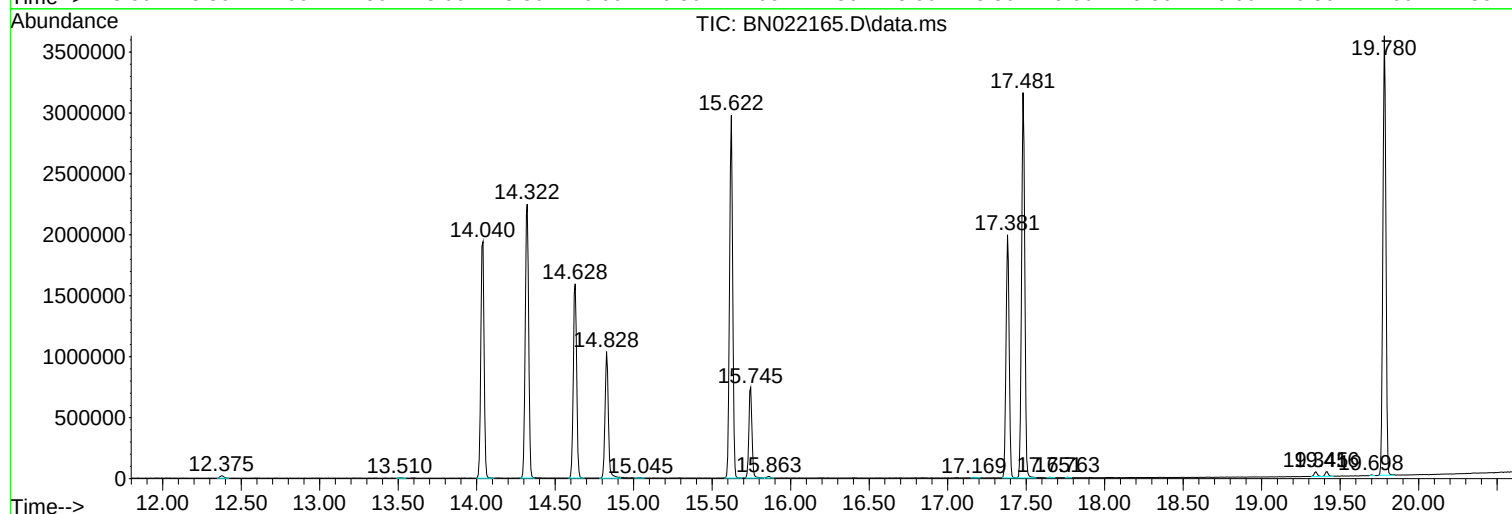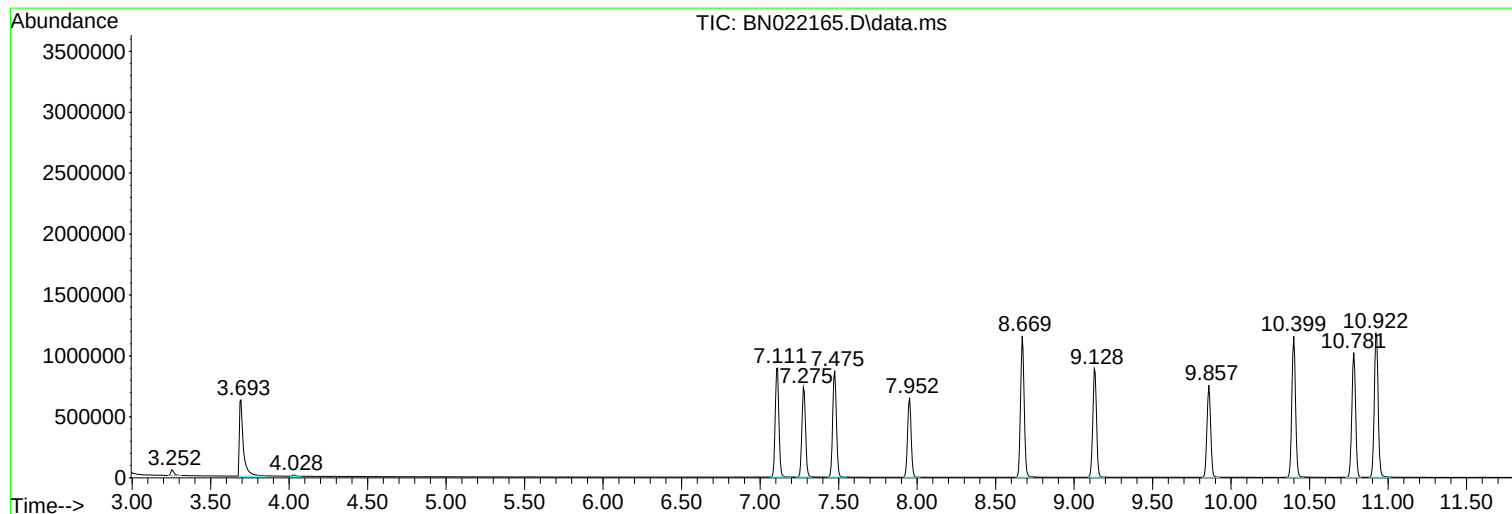

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022165.D
Acq On : 18 Oct 2022 00:49
Operator : CG/JU
Sample : PB148277BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK277

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022165.D
Acq On : 18 Oct 2022 00:49
Operator : CG/JU
Sample : PB148277BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK277

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
