

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022166.D
 Acq On : 18 Oct 2022 01:26
 Operator : CG/JU
 Sample : PB148279BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK279

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022166.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	55	rVB	40442	62455	1.51%	0.139%
2	3.687	116	119	145	rBV	548687	961254	23.18%	2.143%
3	4.028	173	177	186	rVB	9115	14500	0.35%	0.032%
4	7.105	693	700	714	rBV	792341	1260551	30.40%	2.810%
5	7.275	722	729	743	rVB	632427	1005725	24.26%	2.242%
6	7.475	755	763	774	rBV	750547	1209204	29.16%	2.695%
7	7.952	836	844	852	rBV	536634	855696	20.64%	1.907%
8	8.669	959	966	980	rBV	1015287	1613364	38.91%	3.596%
9	9.128	1037	1044	1060	rBV	755111	1255271	30.28%	2.798%
10	9.857	1160	1168	1178	rBV	648050	1061405	25.60%	2.366%
11	10.399	1252	1260	1277	rBV	989776	1647725	39.74%	3.673%
12	10.781	1317	1325	1333	rBV	846370	1408549	33.97%	3.140%
13	10.922	1340	1349	1369	rBV	1028289	1768297	42.65%	3.941%
14	12.375	1590	1596	1604	rVB2	16392	27186	0.66%	0.061%
15	13.593	1796	1803	1808	rBV4	2438	4656	0.11%	0.010%
16	14.040	1872	1879	1889	rBV	1678744	2440748	58.87%	5.440%
17	14.322	1920	1927	1936	rBV	2002429	2966427	71.55%	6.612%
18	14.628	1972	1979	1987	rBV	1354499	1987157	47.93%	4.429%
19	14.828	2007	2013	2032	rBV	879060	1277247	30.81%	2.847%
20	15.045	2044	2050	2054	rVB6	3496	5992	0.14%	0.013%
21	15.622	2138	2148	2160	rBV	2638342	3667748	88.46%	8.175%
22	15.745	2163	2169	2183	rVV	578317	797982	19.25%	1.779%
23	15.863	2184	2189	2194	rVB	11159	16903	0.41%	0.038%
24	16.192	2238	2245	2253	rVB8	2280	5361	0.13%	0.012%
25	17.169	2406	2411	2414	rBV4	3169	5023	0.12%	0.011%
26	17.381	2441	2447	2457	rBV	1654285	2311842	55.76%	5.153%
27	17.481	2457	2464	2478	rBV	2930938	3978873	95.96%	8.869%
28	19.345	2776	2781	2785	rBV2	30287	42795	1.03%	0.095%
29	19.416	2788	2793	2799	rBV	32584	47541	1.15%	0.106%
30	19.780	2849	2855	2869	rBV	3059171	4146210	100.00%	9.242%
31	21.580	3155	3161	3167	rBV	1538624	2057159	49.62%	4.585%
32	23.886	3545	3553	3570	rVB2	1591183	3235448	78.03%	7.212%
33	24.045	3573	3580	3591	rVB2	821841	1717908	41.43%	3.829%


Sum of corrected areas: 44864202

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022166.D
Acq On : 18 Oct 2022 01:26
Operator : CG/JU
Sample : PB148279BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK279

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

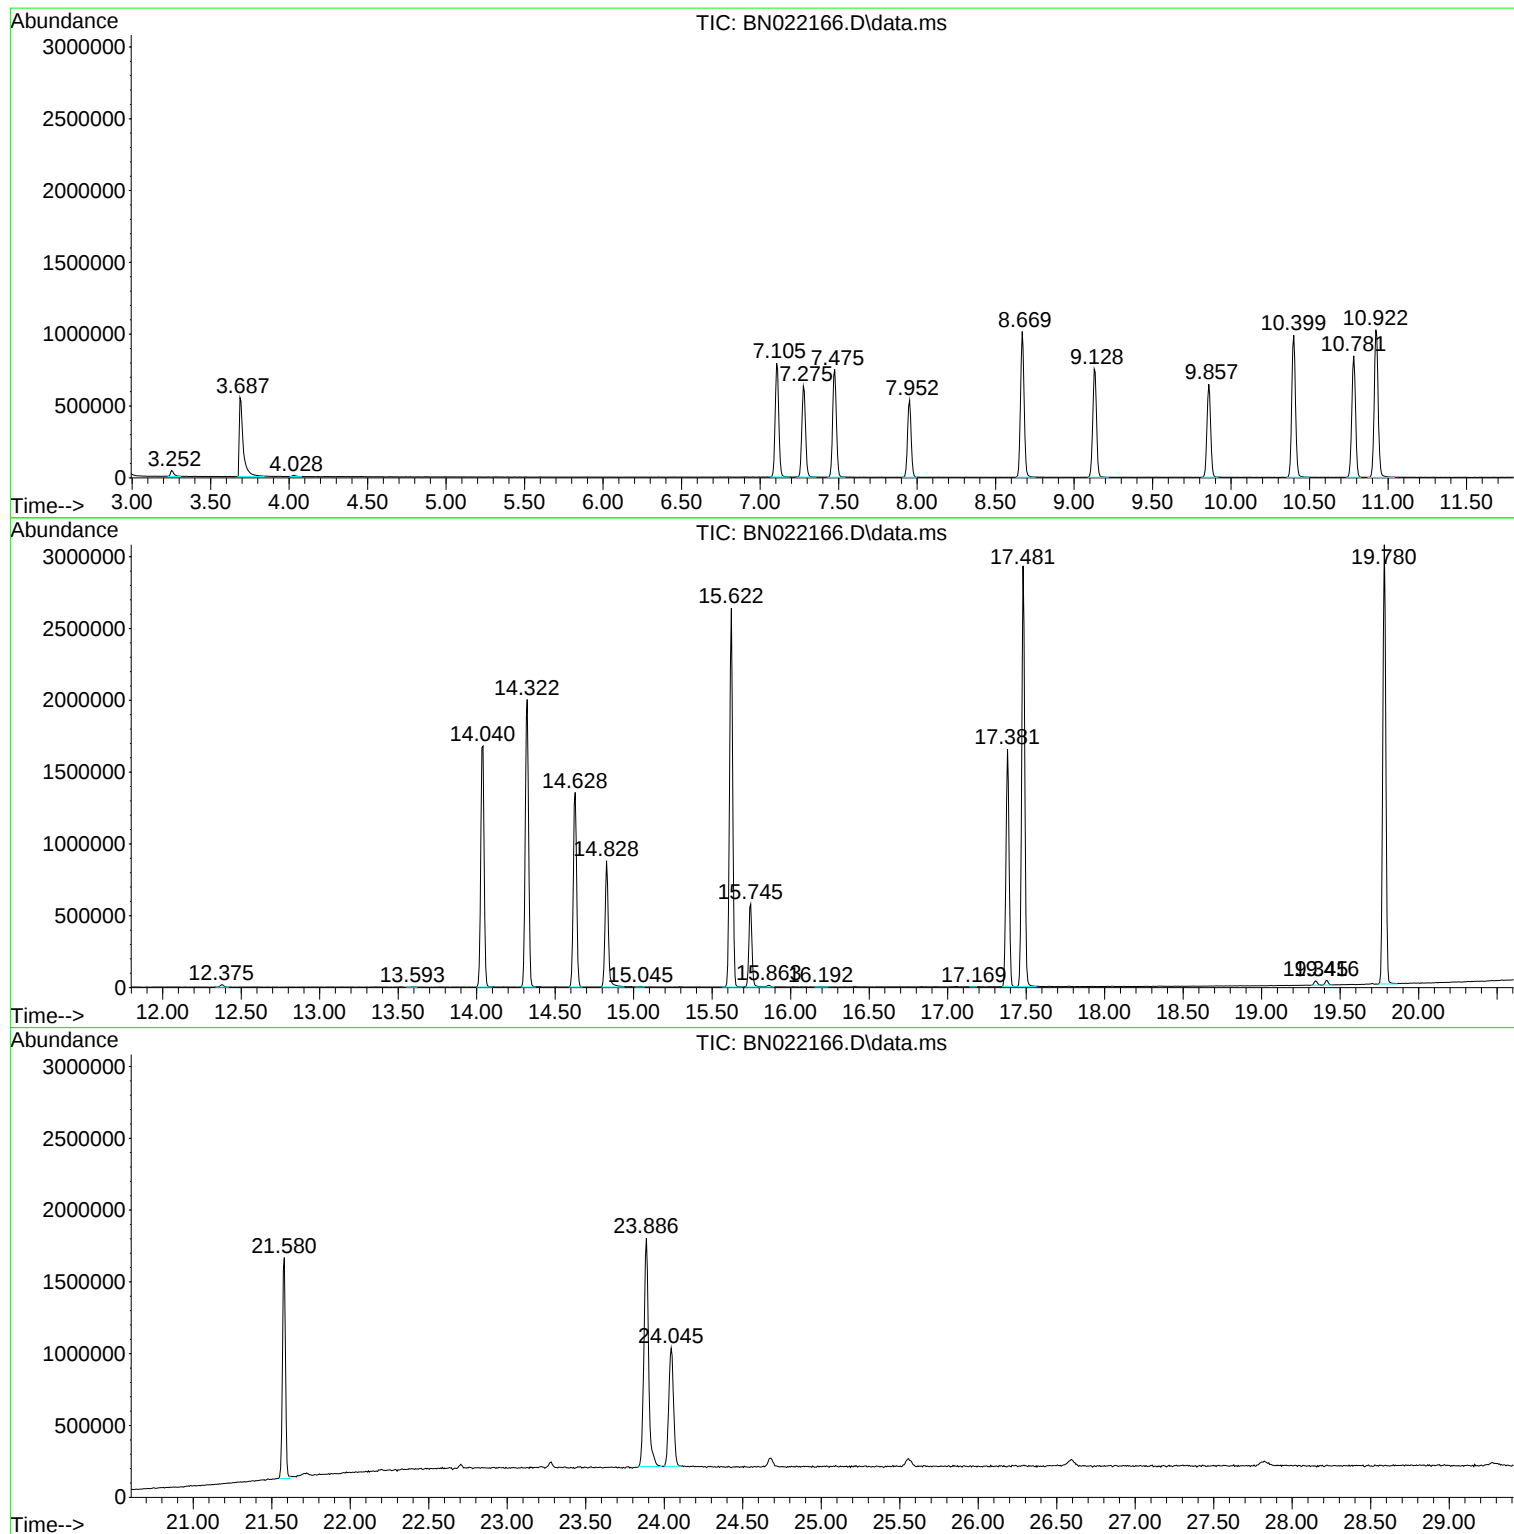

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022166.D
Acq On : 18 Oct 2022 01:26
Operator : CG/JU
Sample : PB148279BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK279

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022166.D
Acq On : 18 Oct 2022 01:26
Operator : CG/JU
Sample : PB148279BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK279

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc