

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
 Data File : BN022174.D
 Acq On : 18 Oct 2022 13:05
 Operator : CG/JU
 Sample : PB148363BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK363

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022174.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	56	rVB	42453	64568	1.49%	0.141%
2	3.693	117	120	143	rBV	390171	689384	15.93%	1.508%
3	4.028	173	177	183	rBV	11130	16128	0.37%	0.035%
4	7.104	693	700	711	rBV	783670	1277482	29.52%	2.794%
5	7.275	723	729	739	rBV	649722	1029795	23.80%	2.253%
6	7.475	756	763	778	rBV	778028	1243200	28.73%	2.719%
7	7.951	836	844	854	rBV	592383	949290	21.94%	2.076%
8	8.669	959	966	977	rBV	1013835	1636886	37.83%	3.581%
9	9.128	1036	1044	1058	rBV	779319	1296082	29.95%	2.835%
10	9.857	1159	1168	1180	rBV	667214	1088390	25.15%	2.381%
11	10.398	1253	1260	1277	rBV	1013796	1679647	38.82%	3.674%
12	10.781	1317	1325	1334	rBV	926303	1550366	35.83%	3.391%
13	10.928	1341	1350	1367	rBV	536291	960110	22.19%	2.100%
14	12.375	1591	1596	1604	rVB	15214	26439	0.61%	0.058%
15	13.516	1785	1790	1795	rBV2	5685	8553	0.20%	0.019%
16	14.039	1871	1879	1890	rBV	1719944	2453280	56.70%	5.366%
17	14.322	1920	1927	1943	rBV2	2030807	3039676	70.25%	6.649%
18	14.628	1972	1979	1989	rBV	1485536	2182987	50.45%	4.775%
19	14.828	2006	2013	2028	rBV	884125	1298106	30.00%	2.839%
20	15.039	2045	2049	2053	rVB6	3070	4492	0.10%	0.010%
21	15.622	2141	2148	2157	rVB	2642126	3729487	86.19%	8.158%
22	15.745	2161	2169	2180	rBV	702206	970358	22.43%	2.123%
23	15.863	2185	2189	2195	rVB	10928	15962	0.37%	0.035%
24	17.163	2407	2410	2420	rVB3	2811	5544	0.13%	0.012%
25	17.380	2441	2447	2457	rBV	1827516	2576287	59.54%	5.635%
26	17.480	2457	2464	2479	rBV2	2842625	4060256	93.84%	8.881%
27	18.569	2646	2649	2654	rVB3	6071	6866	0.16%	0.015%
28	19.063	2729	2733	2736	rBV4	4539	6414	0.15%	0.014%
29	19.345	2777	2781	2787	rBV2	33474	44650	1.03%	0.098%
30	19.416	2789	2793	2797	rVV	29985	38501	0.89%	0.084%
31	19.780	2849	2855	2866	rBV	3105127	4326826	100.00%	9.465%
32	21.086	3074	3077	3080	rBV4	17804	19988	0.46%	0.044%
33	21.151	3086	3088	3093	rBV4	19472	21408	0.49%	0.047%
34	21.580	3156	3161	3167	rBV	1743031	2212014	51.12%	4.839%
35	23.886	3546	3553	3567	rVB2	1624649	3320684	76.75%	7.264%
36	24.051	3574	3581	3589	rVB2	930921	1866210	43.13%	4.082%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022174.D
Acq On : 18 Oct 2022 13:05
Operator : CG/JU
Sample : PB148363BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK363

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Title : SVOA CALIBRATION




Sum of corrected areas: 45716316

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022174.D
Acq On : 18 Oct 2022 13:05
Operator : CG/JU
Sample : PB148363BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK363

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

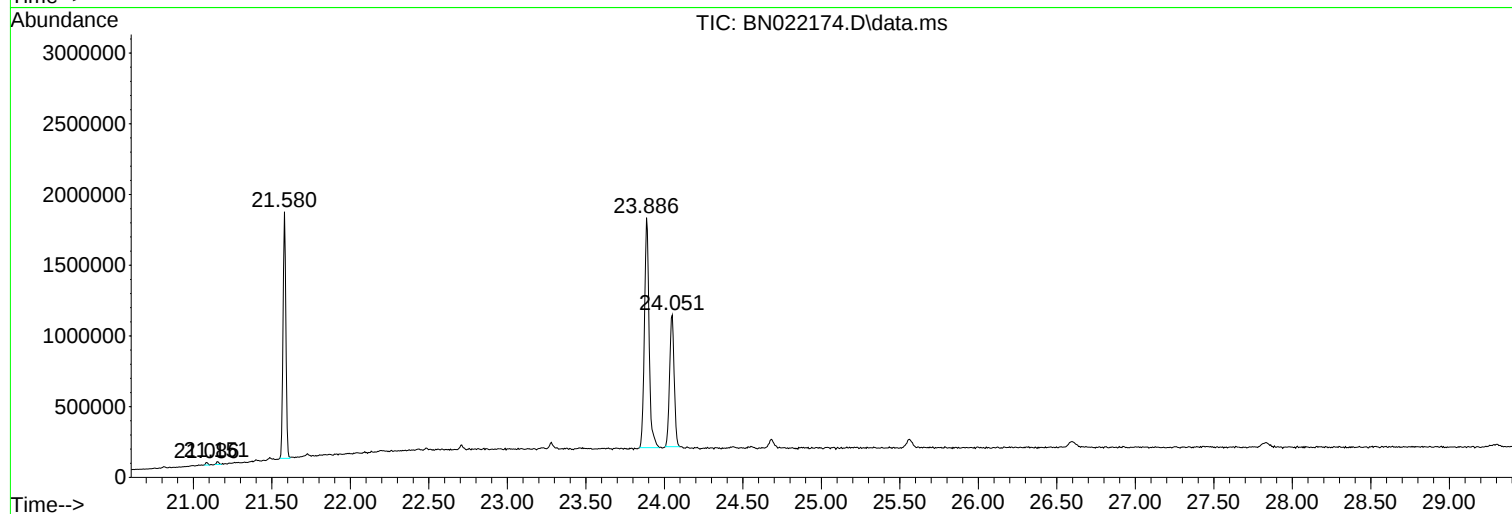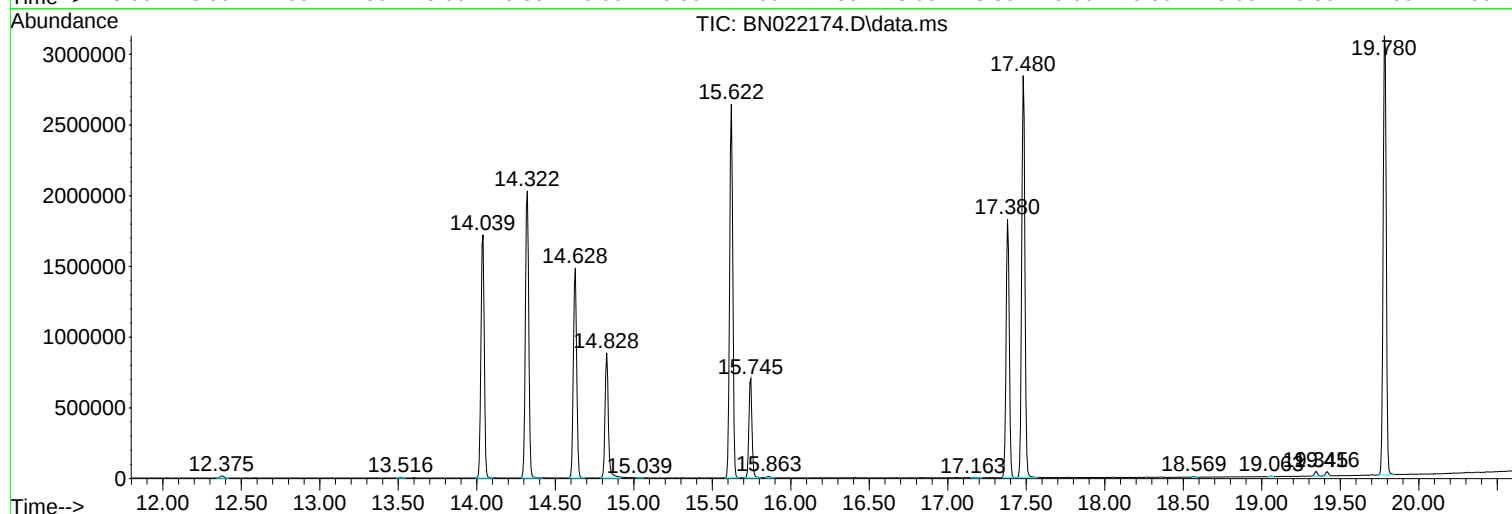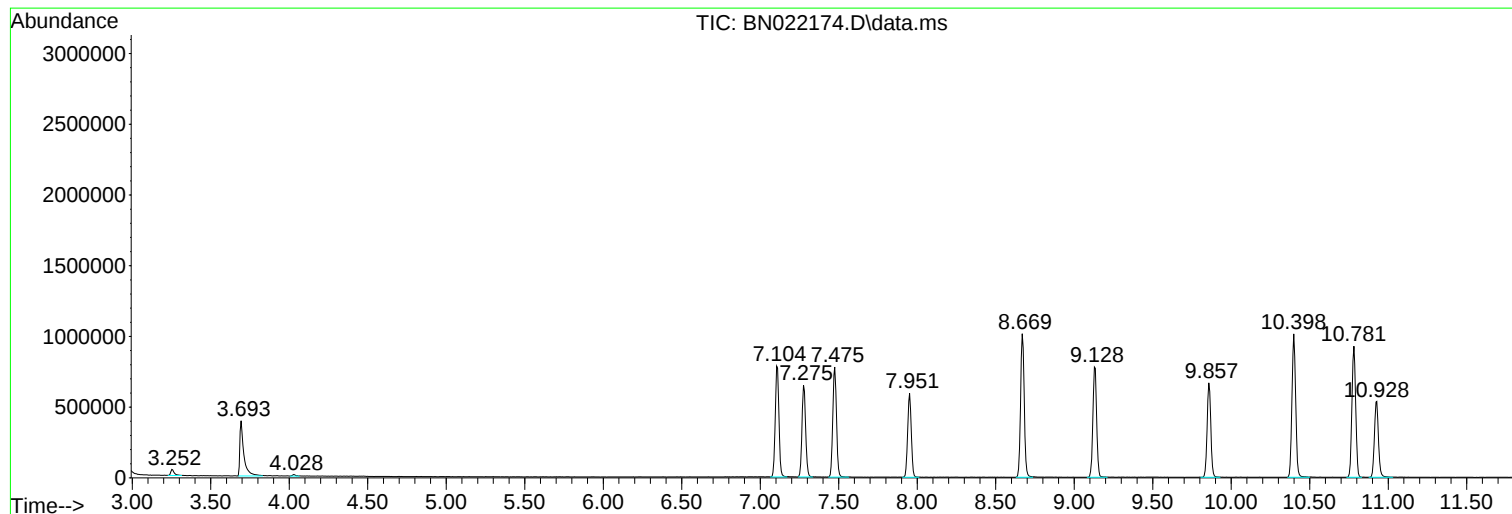

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022174.D
Acq On : 18 Oct 2022 13:05
Operator : CG/JU
Sample : PB148363BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK363

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101822\
Data File : BN022174.D
Acq On : 18 Oct 2022 13:05
Operator : CG/JU
Sample : PB148363BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK363

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc