
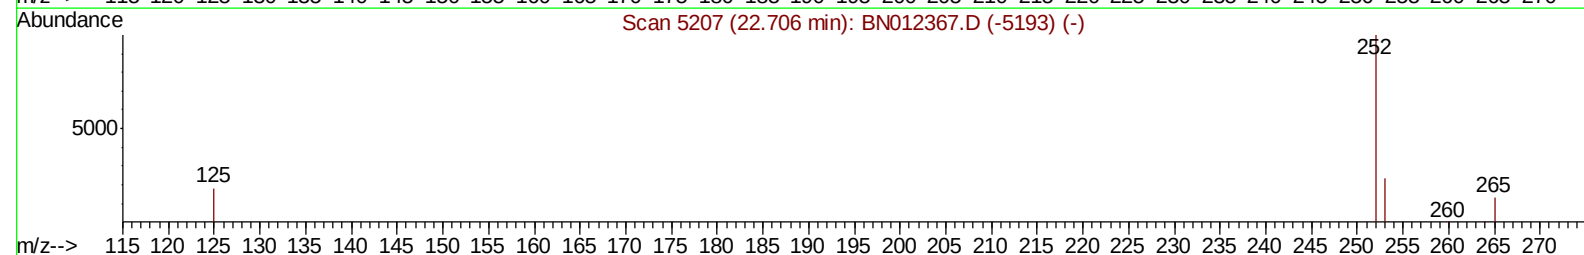
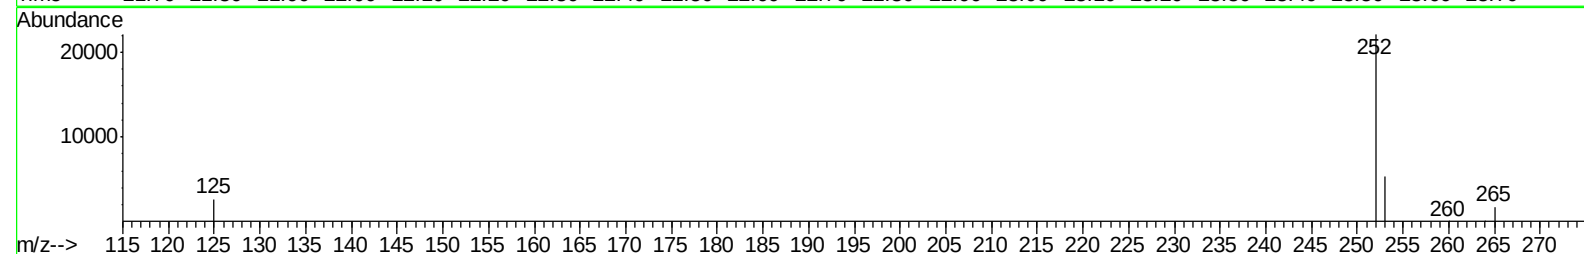


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\  
Data File : BN012370.D  
Acq On : 20 Oct 2020 03:00  
Operator : CG/JU  
Sample : L4308-03DL 5X  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Oct 20 08:25:40 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 20 08:18:15 2020  
Response via : Initial Calibration

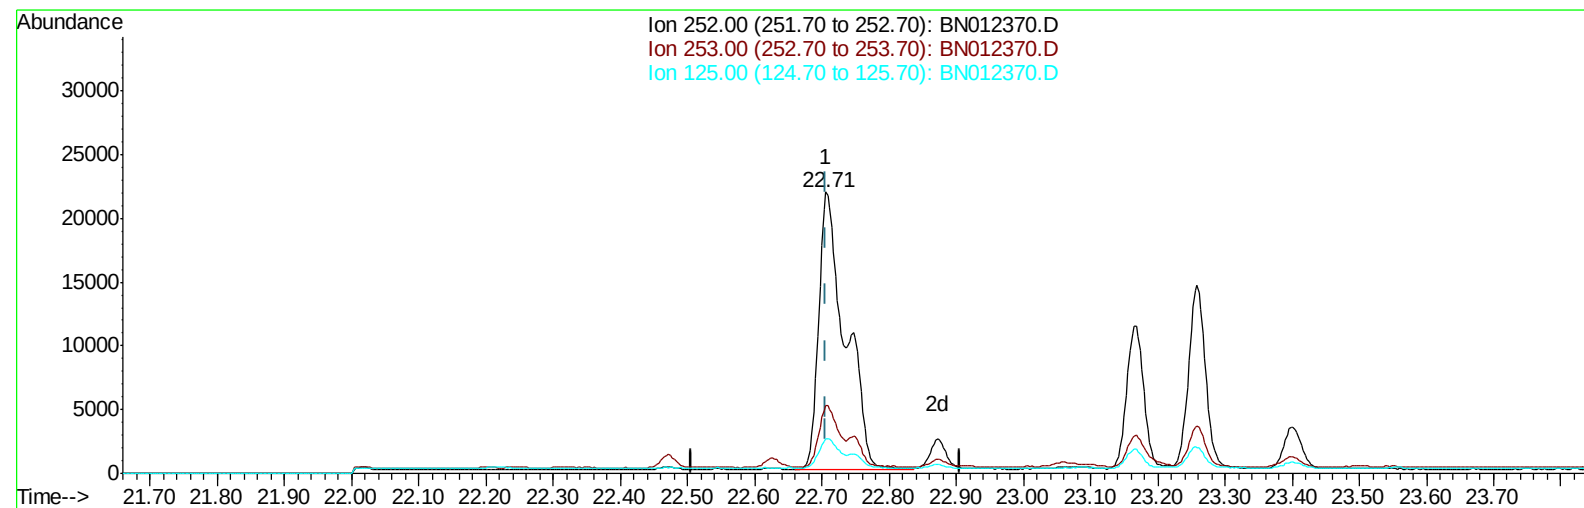

TIC: BN012370.D

(21) Benzo(b)fluoranthene

22.706min (+0.000) 2.48ng/ul

response 59719

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 28.20 | 23.94 |
| 125.00 | 18.90 | 12.30 |
| 0.00   | 0.00  | 0.00  |