
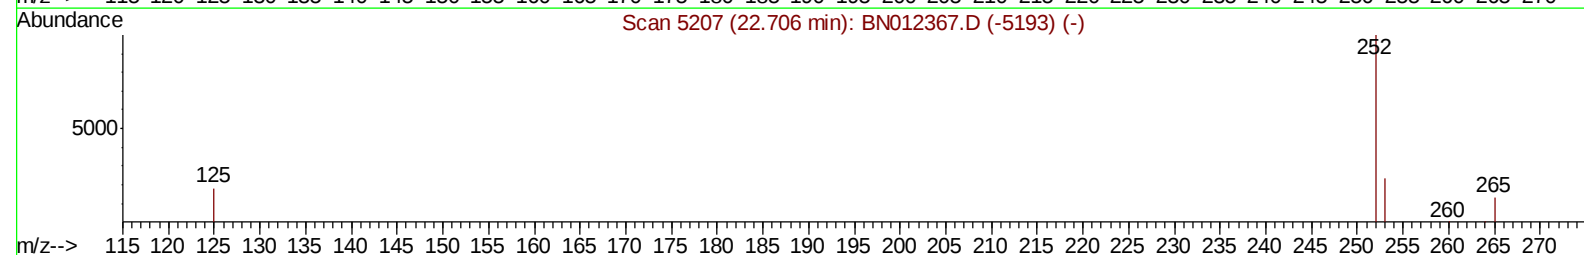
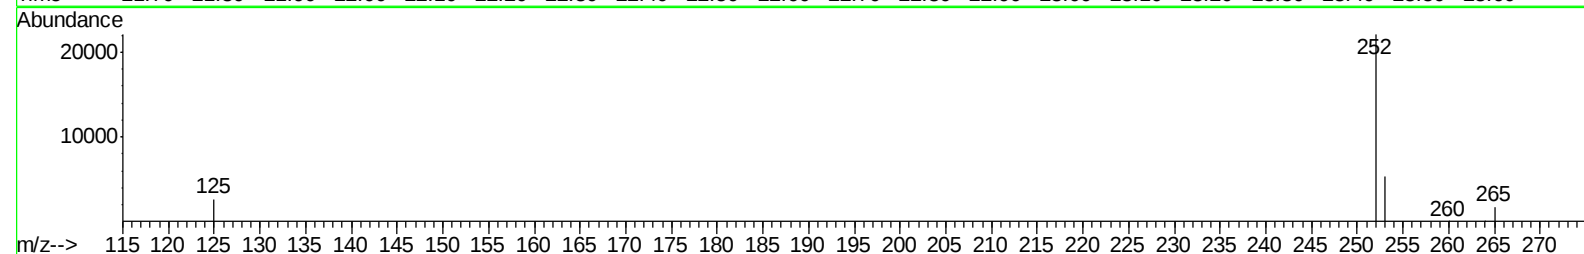


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
Data File : BN012370.D
Acq On : 20 Oct 2020 03:00
Operator : CG/JU
Sample : L4308-03DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Oct 20 08:25:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 20 08:18:15 2020
Response via : Initial Calibration

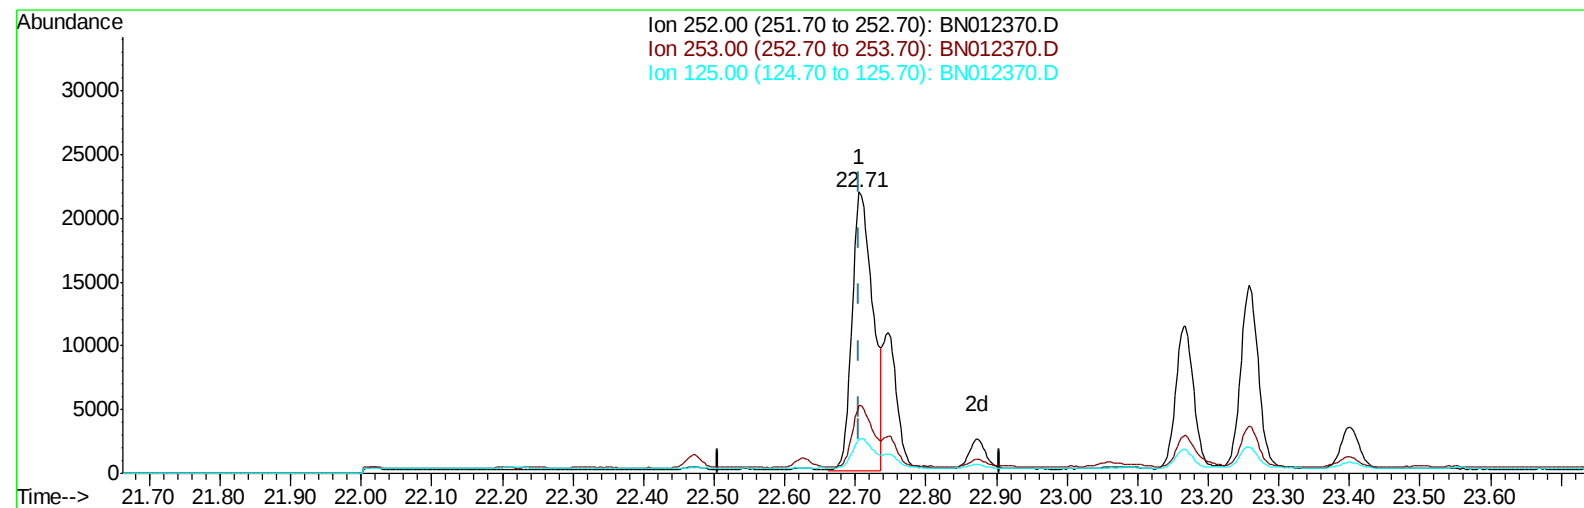

TIC: BN012370.D

(21) Benzo(b)fluoranthene

22.706min (+0.000) 1.84ng/ul m

response 44284

Ion	Exp%	Act%
252.00	100	100
253.00	28.20	23.94
125.00	18.90	12.30
0.00	0.00	0.00