
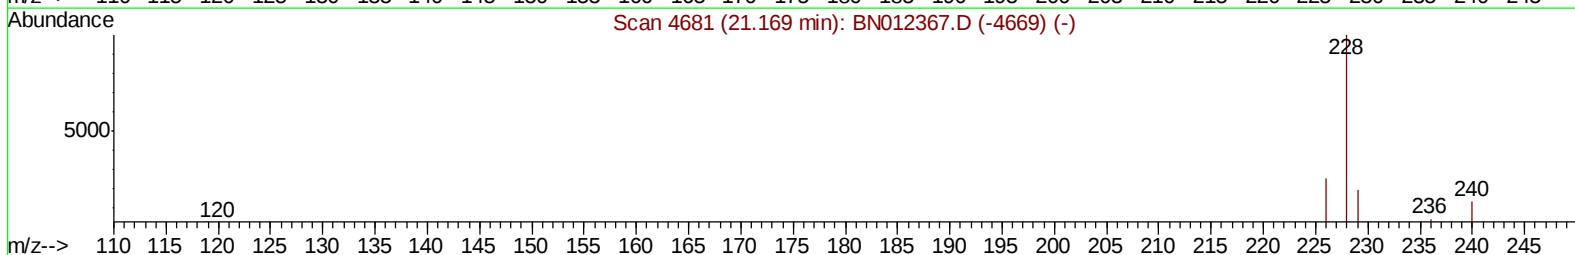
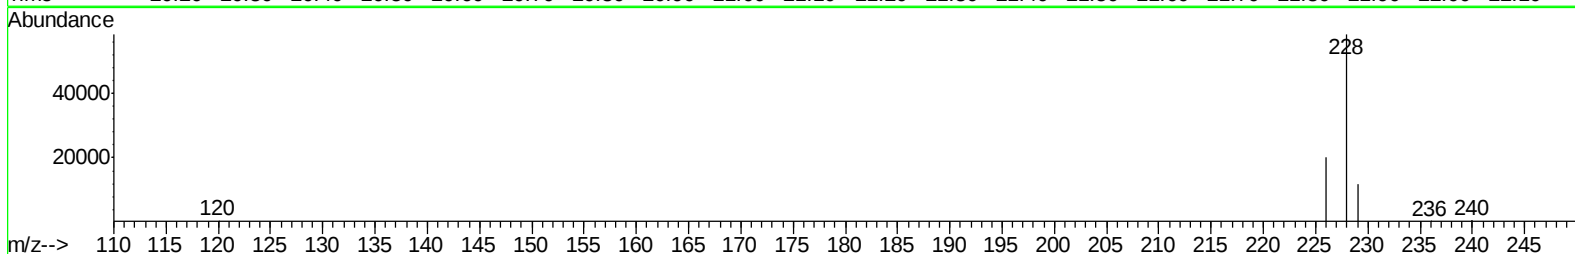


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
Data File : BN012371.D
Acq On : 20 Oct 2020 03:37
Operator : CG/JU
Sample : L4326-01DL 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Oct 20 08:25:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 20 08:18:15 2020
Response via : Initial Calibration

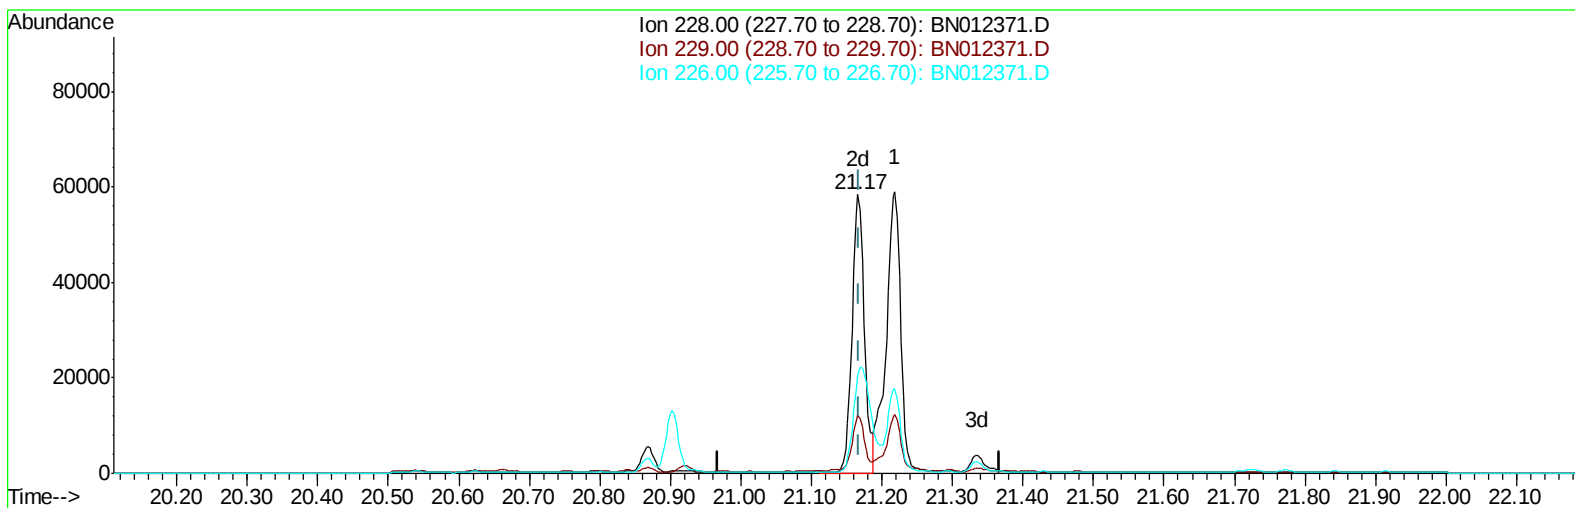

TIC: BN012371.D

(18) Benzo(a)anthracene

21.166min (-0.003) 3.68ng/ul m

response 71279

Ion	Exp%	Act%
228.00	100	100
229.00	20.30	20.56
226.00	26.50	34.79#
0.00	0.00	0.00