
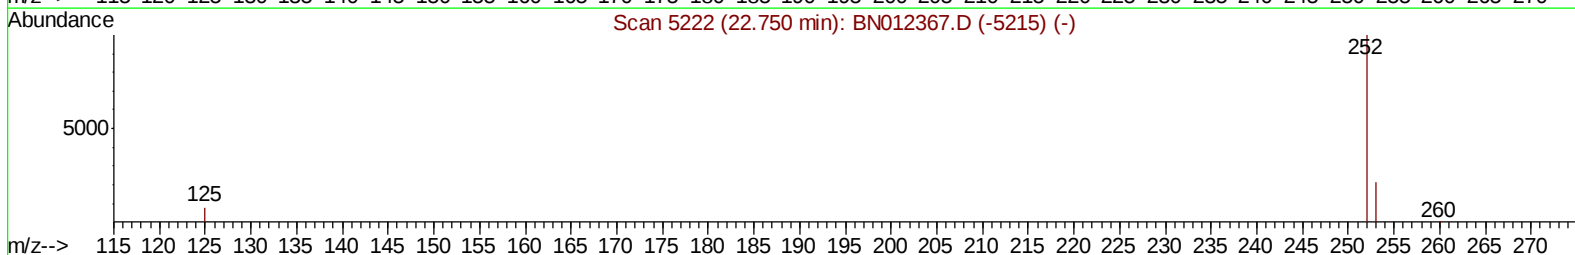
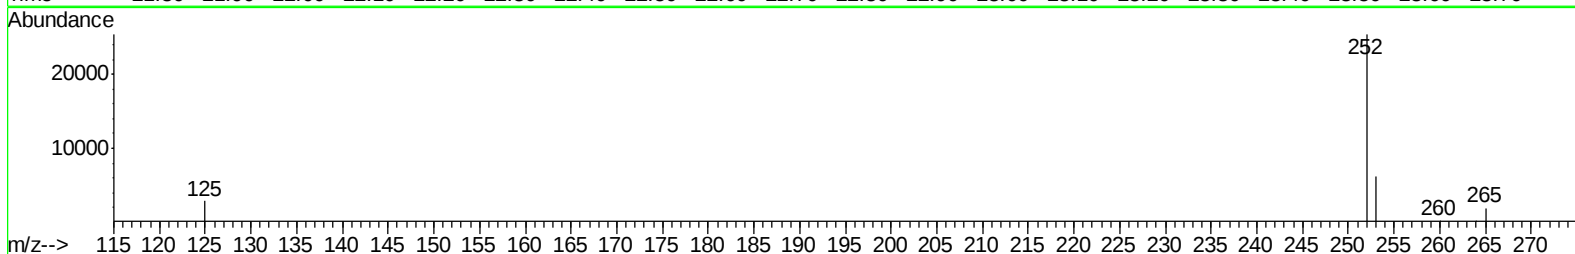


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012371.D
 Acq On : 20 Oct 2020 03:37
 Operator : CG/JU
 Sample : L4326-01DL 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Quant Time: Oct 20 08:25:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 08:18:15 2020
 Response via : Initial Calibration

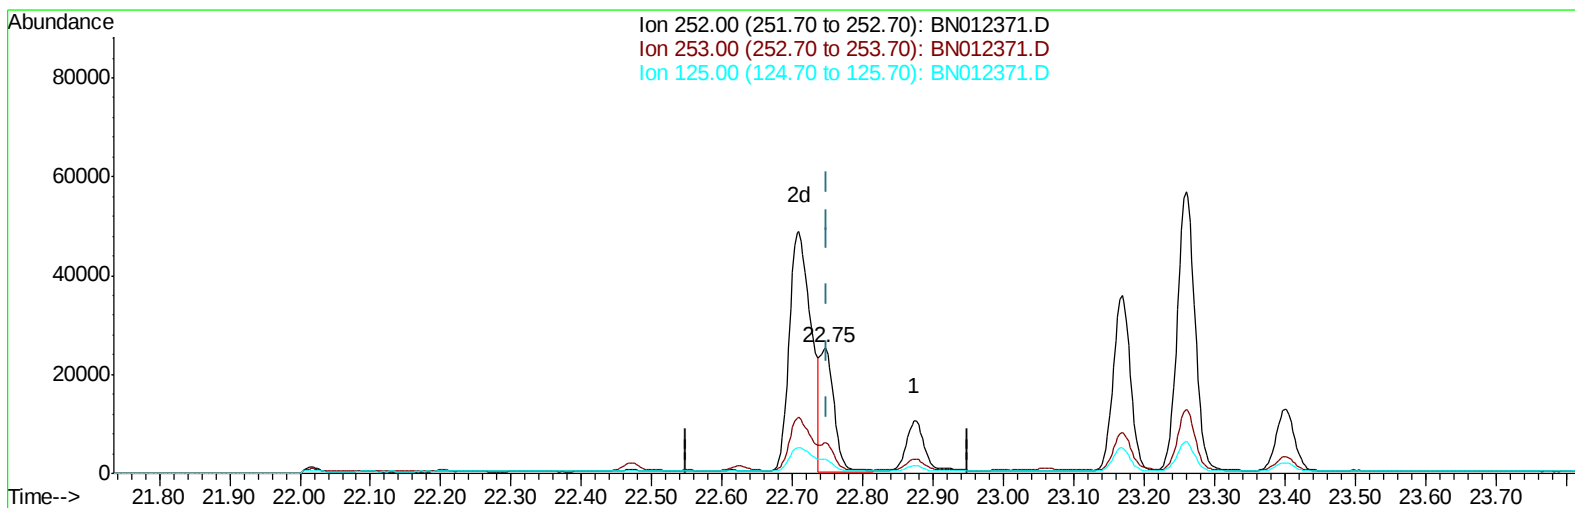

TIC: BN012371.D

(22) Benzo(k)fluoranthene

22.747min (-0.003) 1.53ng/ul m

response 36459

Ion	Exp%	Act%
252.00	100	100
253.00	27.80	24.08
125.00	13.70	11.10
0.00	0.00	0.00