
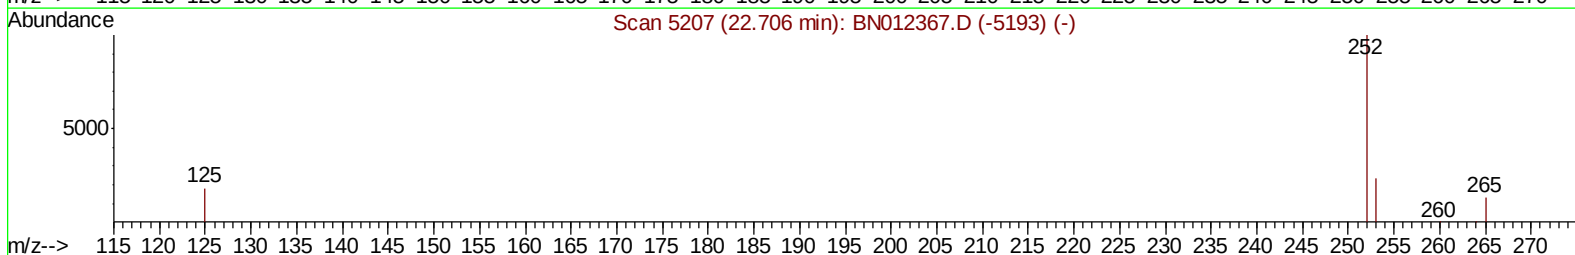
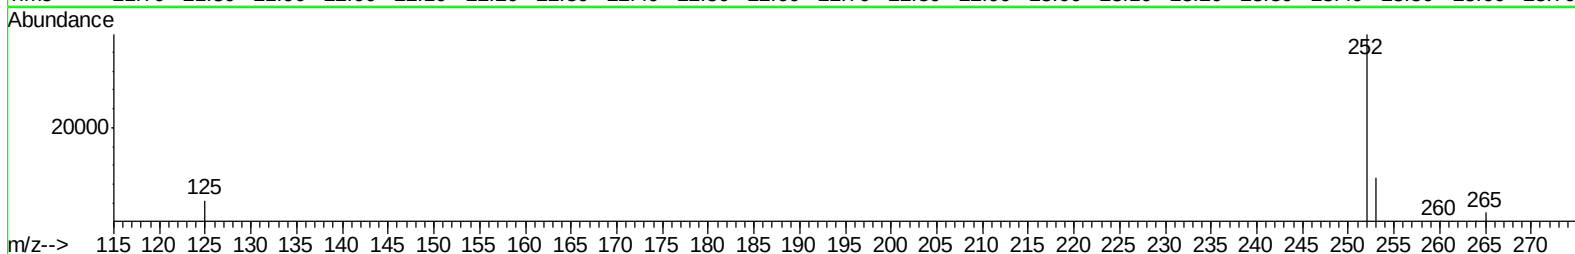


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
Data File : BN012372.D
Acq On : 20 Oct 2020 04:13
Operator : CG/JU
Sample : L4308-02DL 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Oct 20 08:25:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 20 08:18:15 2020
Response via : Initial Calibration

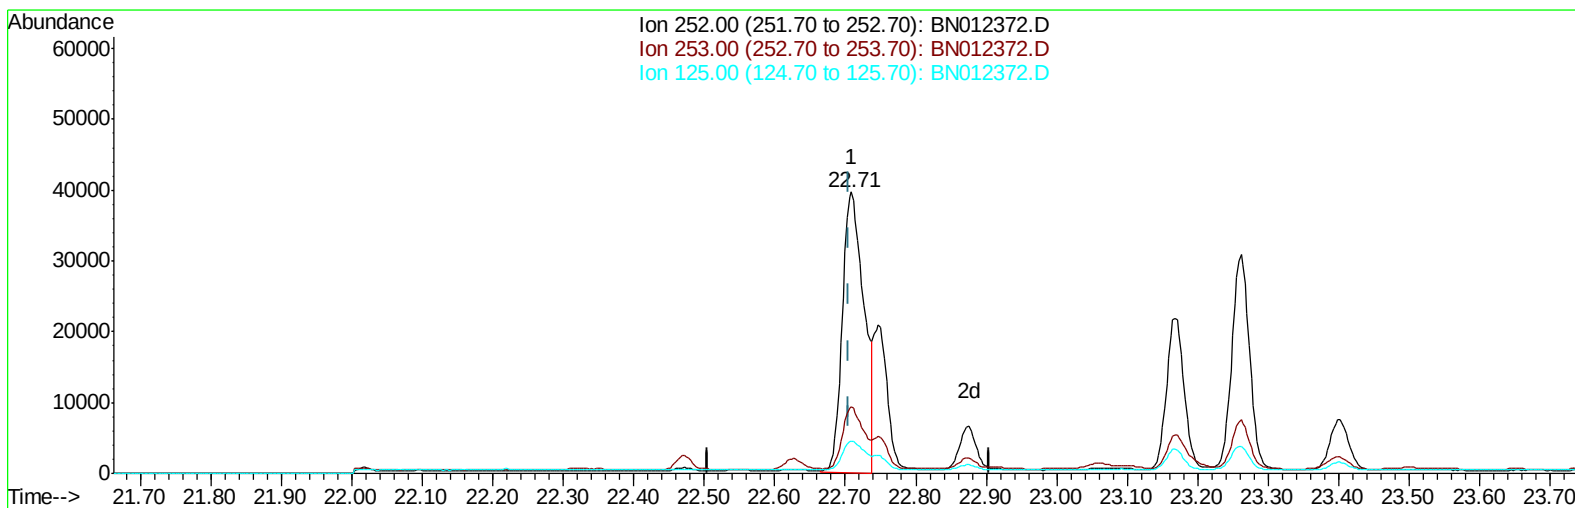

TIC: BN012372.D

(21) Benzo(b)fluoranthene

22.709min (+0.003) 3.55ng/ul m

response 84945

Ion	Exp%	Act%
252.00	100	100
253.00	28.20	23.68
125.00	18.90	11.49
0.00	0.00	0.00