
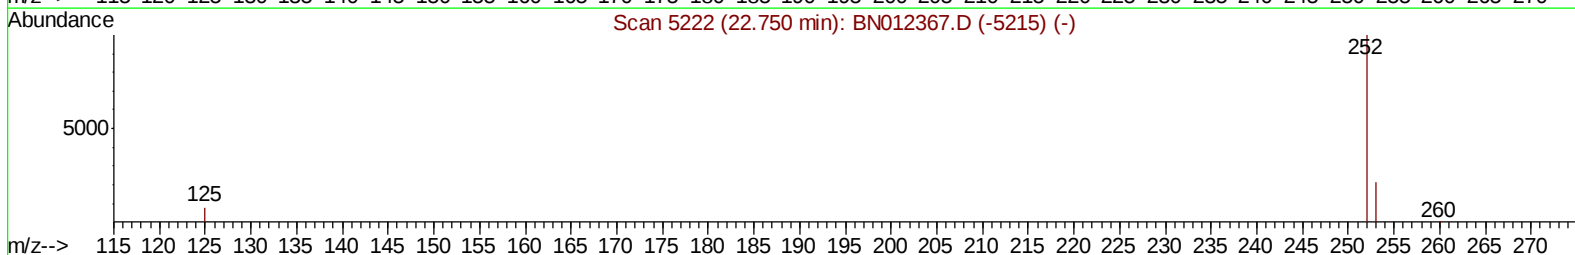
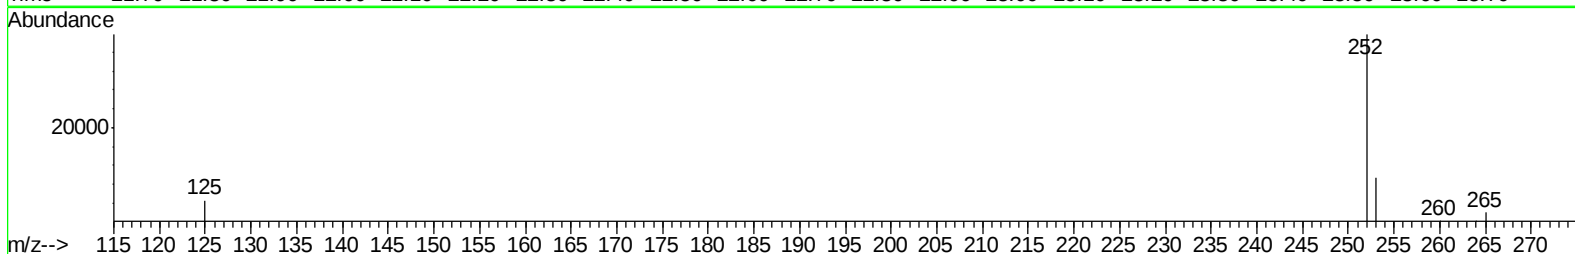


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012372.D
 Acq On : 20 Oct 2020 04:13
 Operator : CG/JU
 Sample : L4308-02DL 5X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Quant Time: Oct 20 08:25:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 08:18:15 2020
 Response via : Initial Calibration

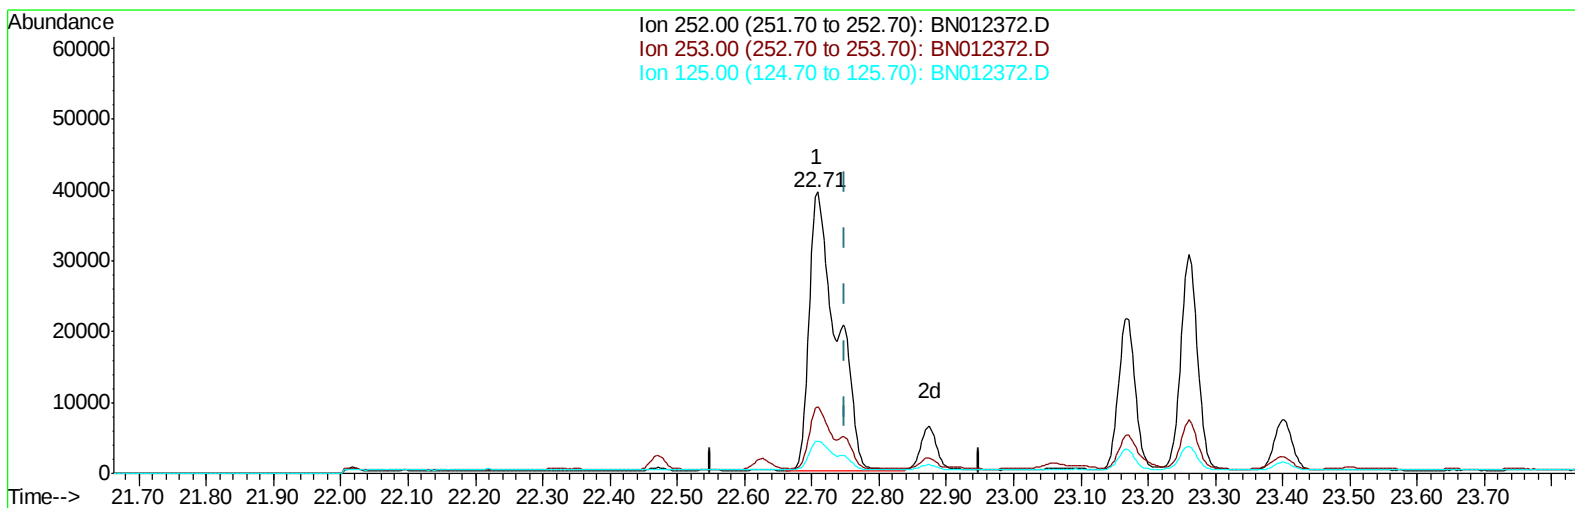

TIC: BN012372.D

(22) Benzo(k)fluoranthene
 22.709min (-0.041) 4.20ng/ul
 response 111377

Ion	Exp%	Act%
252.00	100	100
253.00	27.80	23.68
125.00	13.70	11.49
0.00	0.00	0.00