

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012357.D
 Acq On : 19 Oct 2020 18:34
 Operator : CG/JU
 Sample : L4286-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AQ7

Quant Time: Oct 20 07:31:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 07:24:17 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	1220	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	5307	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	3156	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.99
16) Chrysene-d12	21.19	240	5532	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	5655	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	2865	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	6817	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.39	202	1372	0.055	ng/ul#	1
23) Benzo(a)pyrene	23.23	252	2496	0.112	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
Data File : BN012357.D
Acq On : 19 Oct 2020 18:34
Operator : CG/JU
Sample : L4286-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AQ7

Quant Time: Oct 20 07:31:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 20 07:24:17 2020
Response via : Initial Calibration

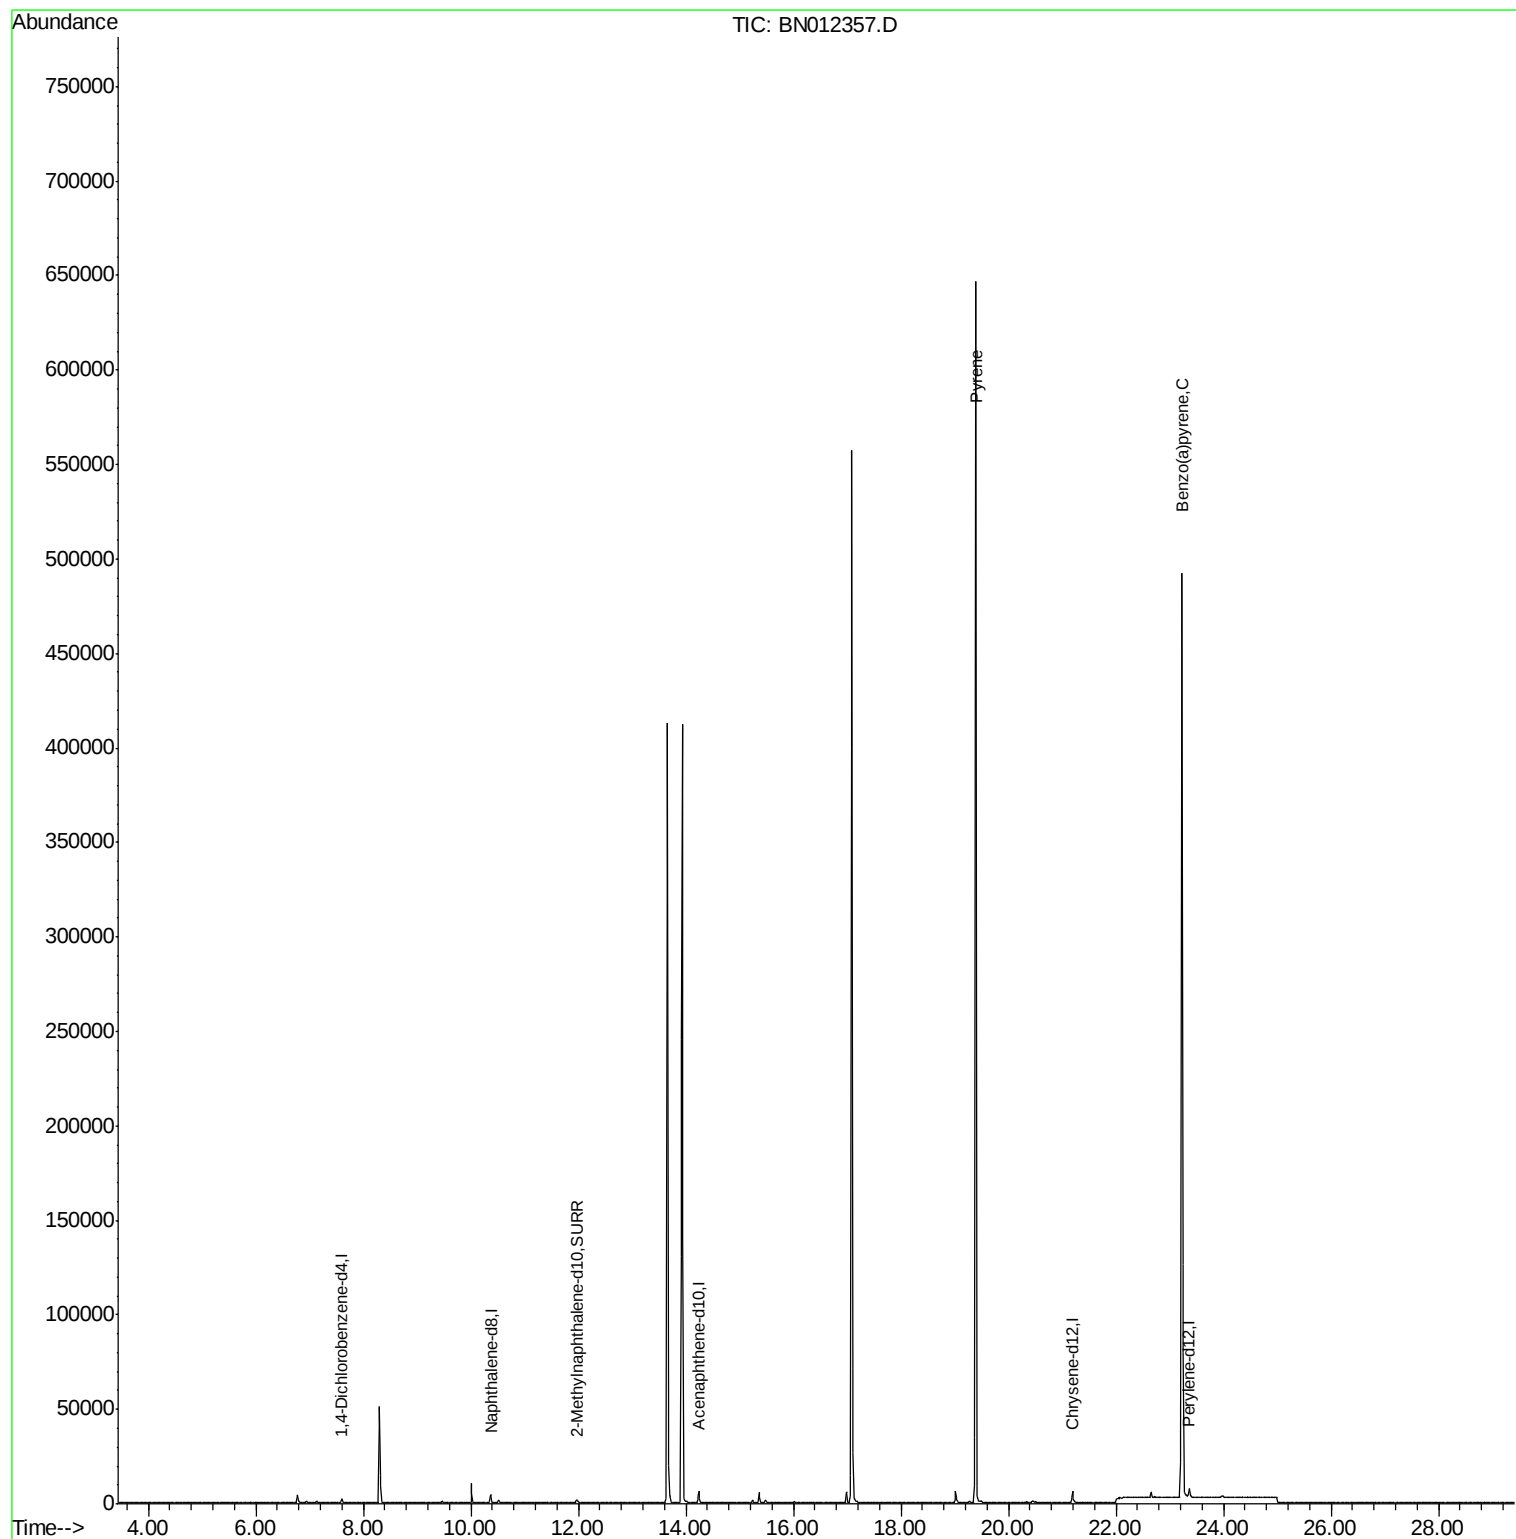


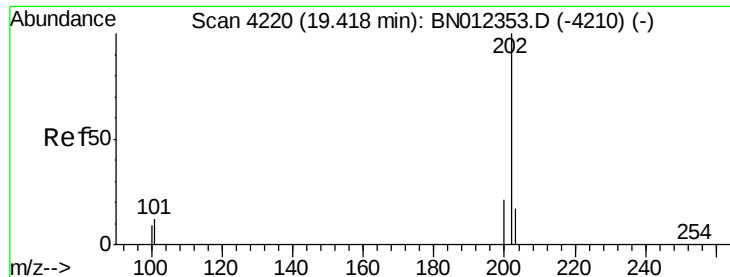




#17
Pvrene
Concen: 0.055 ng/ul
RT: 19.39 min Scan# 4214
Delta R.T. -0.03 min
Lab File: BN012357.D
Acq: 19 Oct 2020 18:34

Instrument :
BNA_N
ClientSampleId :
C0AQ7

Tot Ion:202 Resp: 1372
Ion Ratio Lower Upper
202 100
101 167.8 9.6 14.4#
100 1083.0 7.8 11.8#

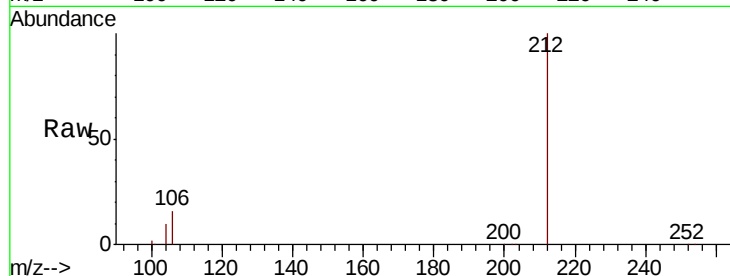


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

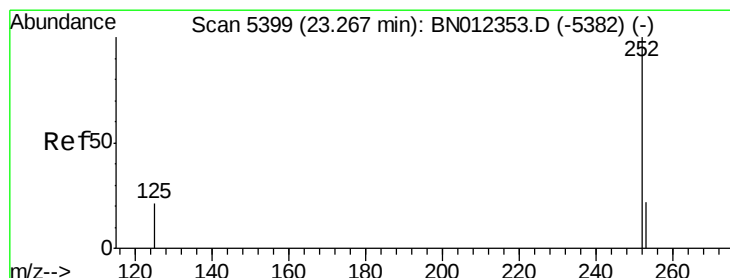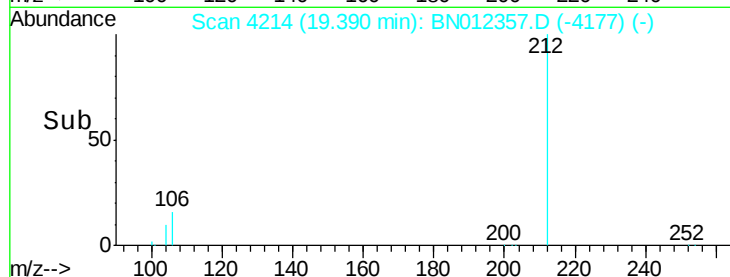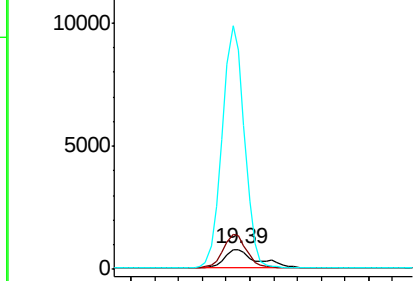

#23
Benzo(a)pyrene
Concen: 0.112 ng/ul
RT: 23.23 min Scan# 5385
Delta R.T. -0.04 min
Lab File: BN012357.D
Acq: 19 Oct 2020 18:34

Tgt Ion:252 Resp: 2496
Ion Ratio Lower Upper
252 100
253 51.0 23.8 35.6#
125 45.1 19.3 28.9#

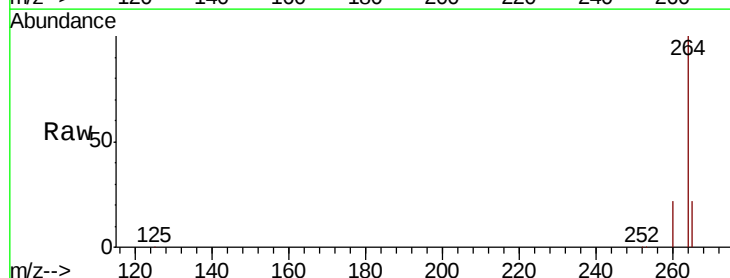

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

