


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN101920\
Data File : BN012344.D
Acq On : 19 Oct 2020 10:40
Operator : CG/JU
Sample : PB132223BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK23

Manual Integrations
APPROVED

Sohil
10/20/2020 9:35:32 AM

Quant Time: Oct 19 11:55:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 19 11:52:04 2020
Response via : Initial Calibration

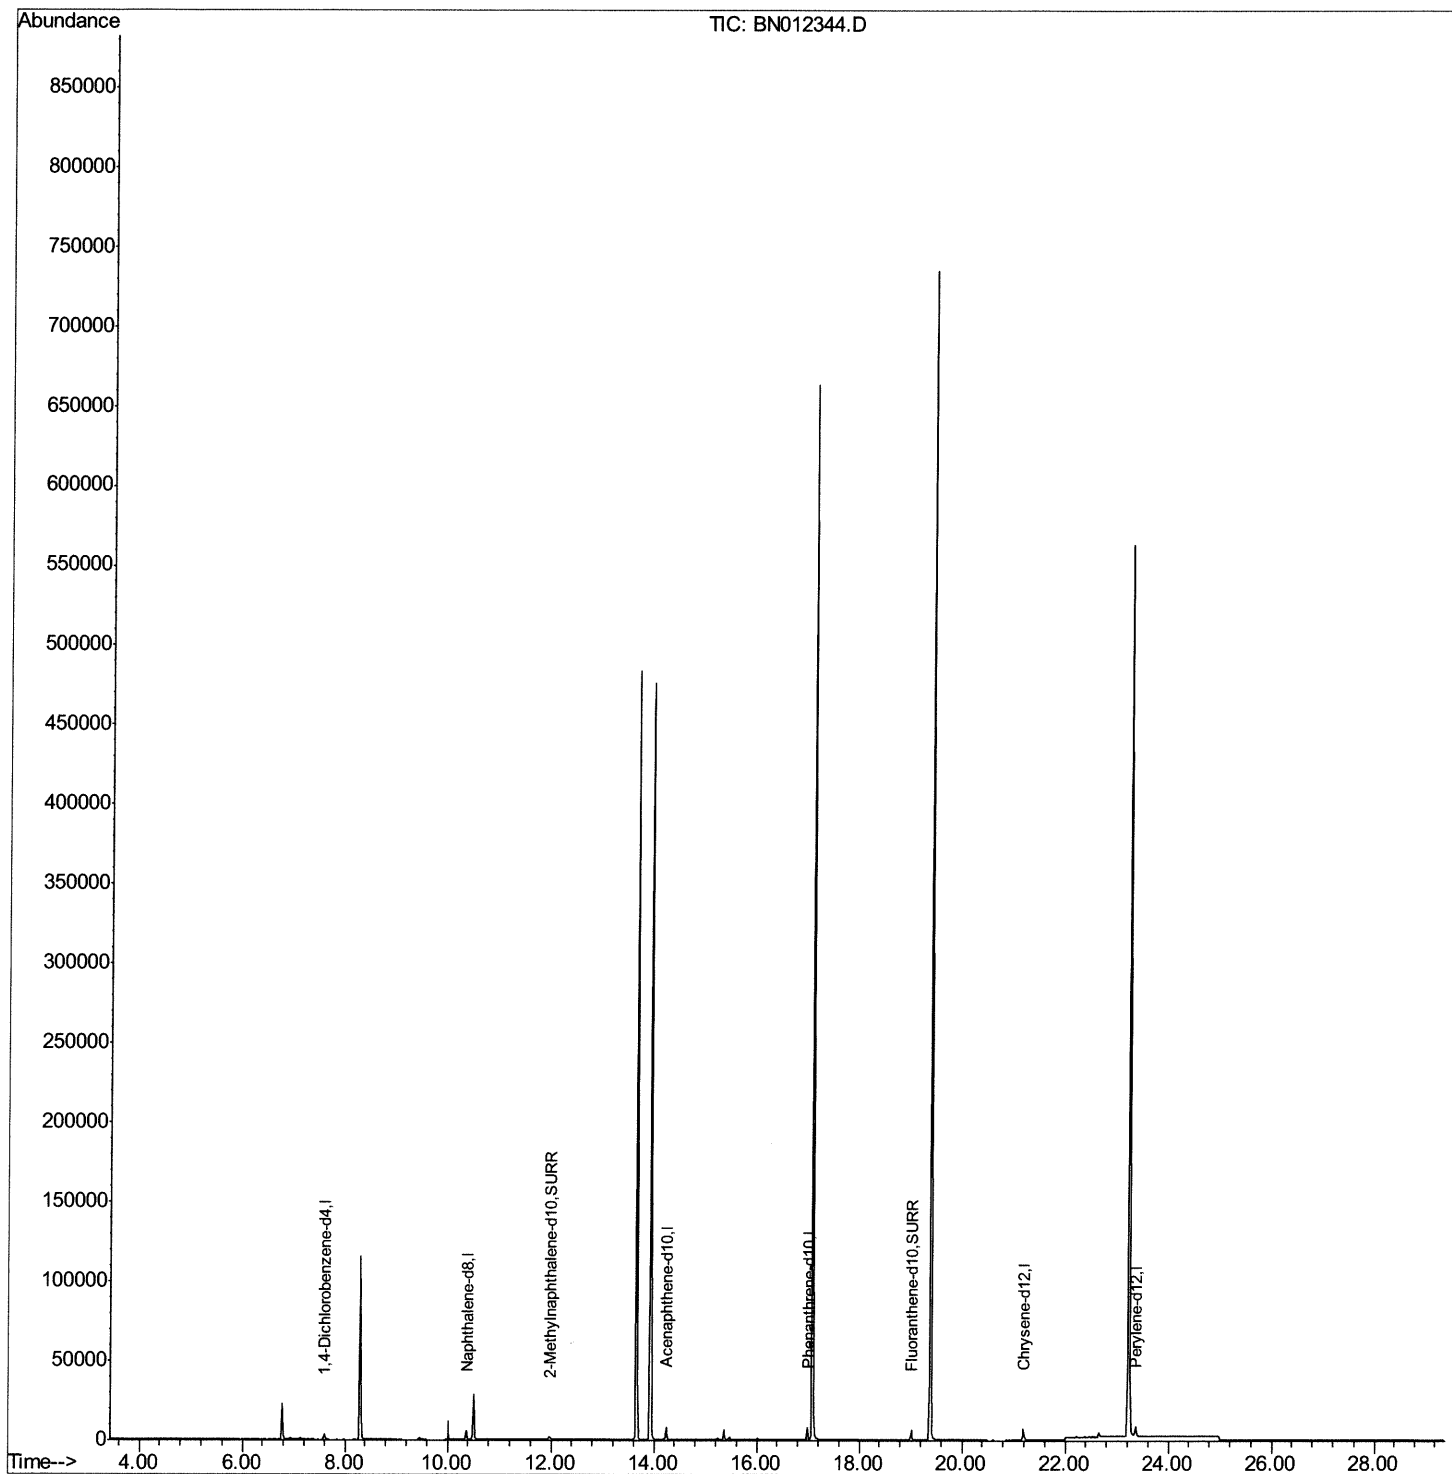

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN101920\
 Data File : BN012344.D
 Acq On : 19 Oct 2020 10:40
 Operator : CG/JU
 Sample : PB132223BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 SBLK23

Manual Integrations
APPROVED

Sohil
 10/20/2020 9:35:32 AM

Quant Time: Oct 19 11:53:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 19 11:52:04 2020
 Response via : Initial Calibration

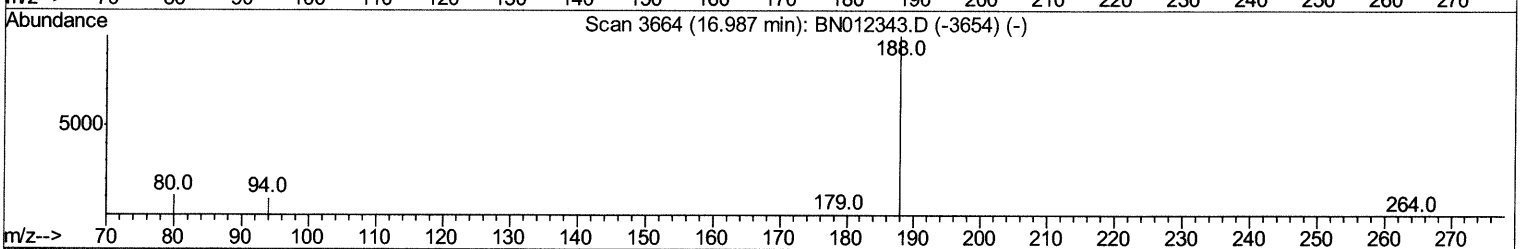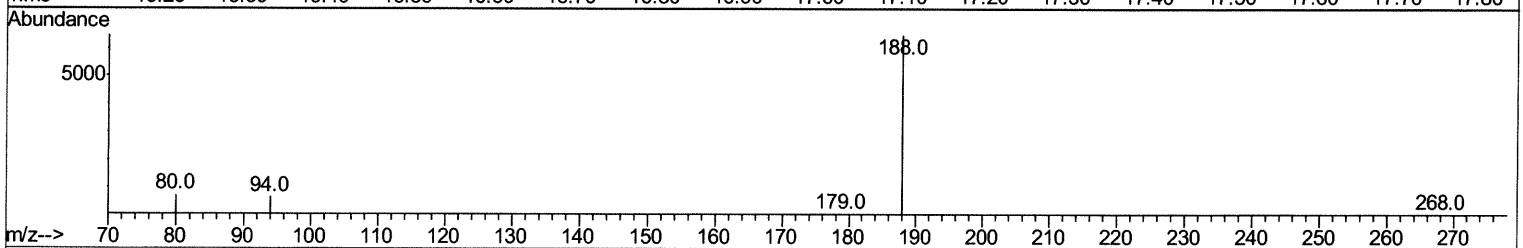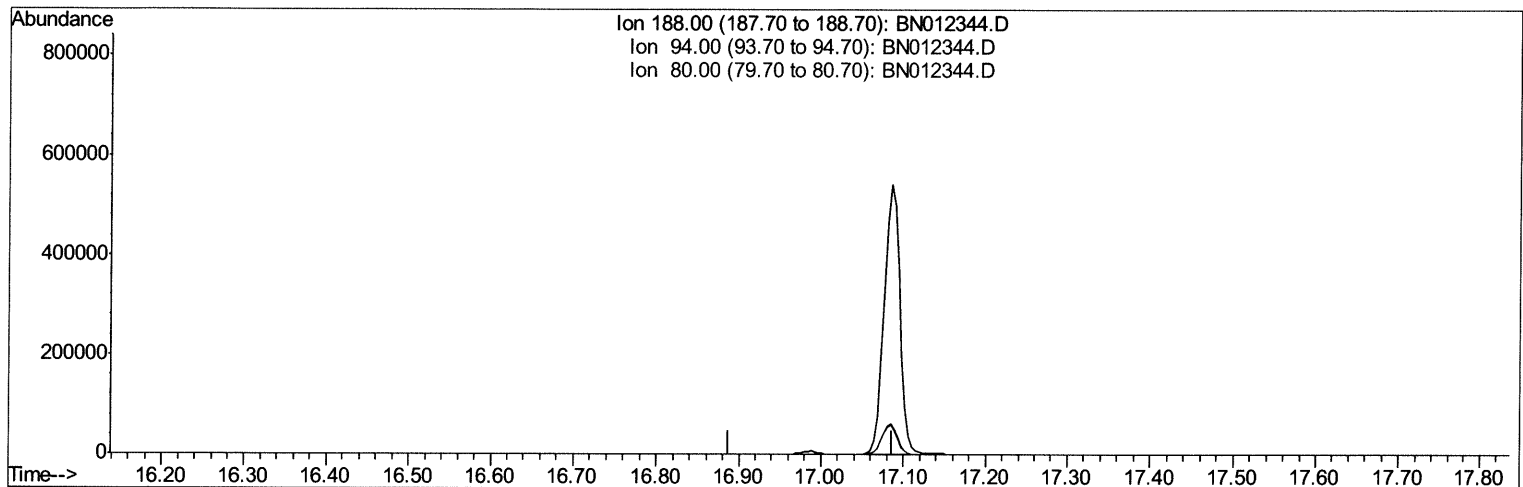

TIC: BN012344.D

(10) Phenanthrene-d10 (I)
 16.987min (-16.987) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.20	0.00#
80.00	12.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN101920\
 Data File : BN012344.D
 Acq On : 19 Oct 2020 10:40
 Operator : CG/JU
 Sample : PB132223BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK23

Manual Integrations
 APPROVED

Sohil
 10/20/2020 9:35:32 AM

Quant Time: Oct 19 11:53:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 19 11:52:04 2020
 Response via : Initial Calibration

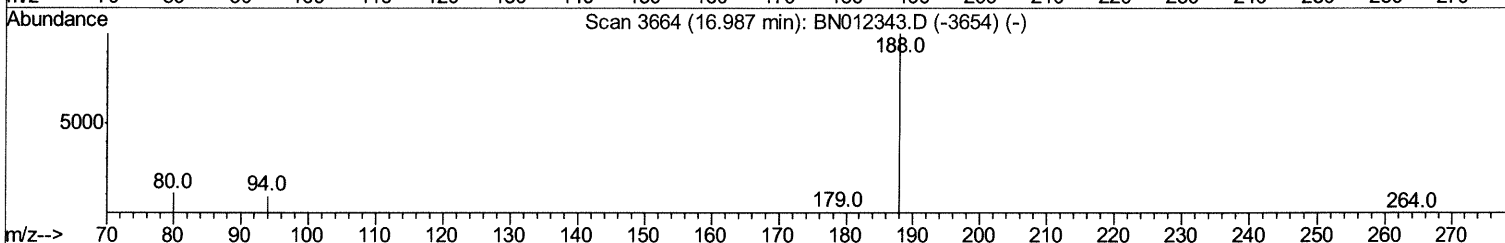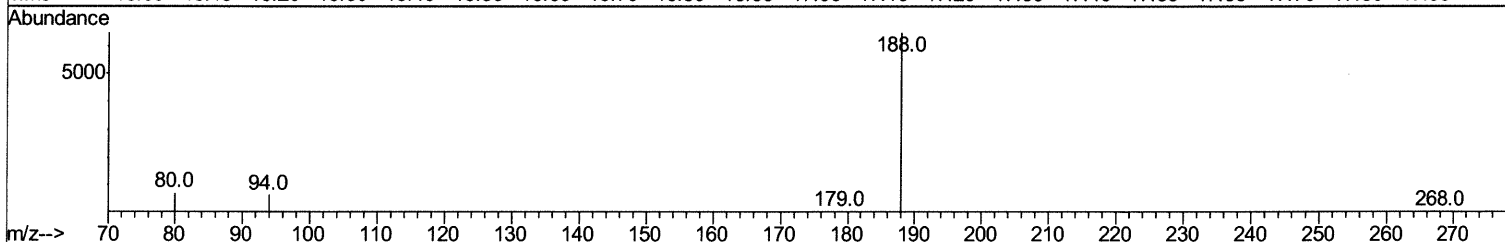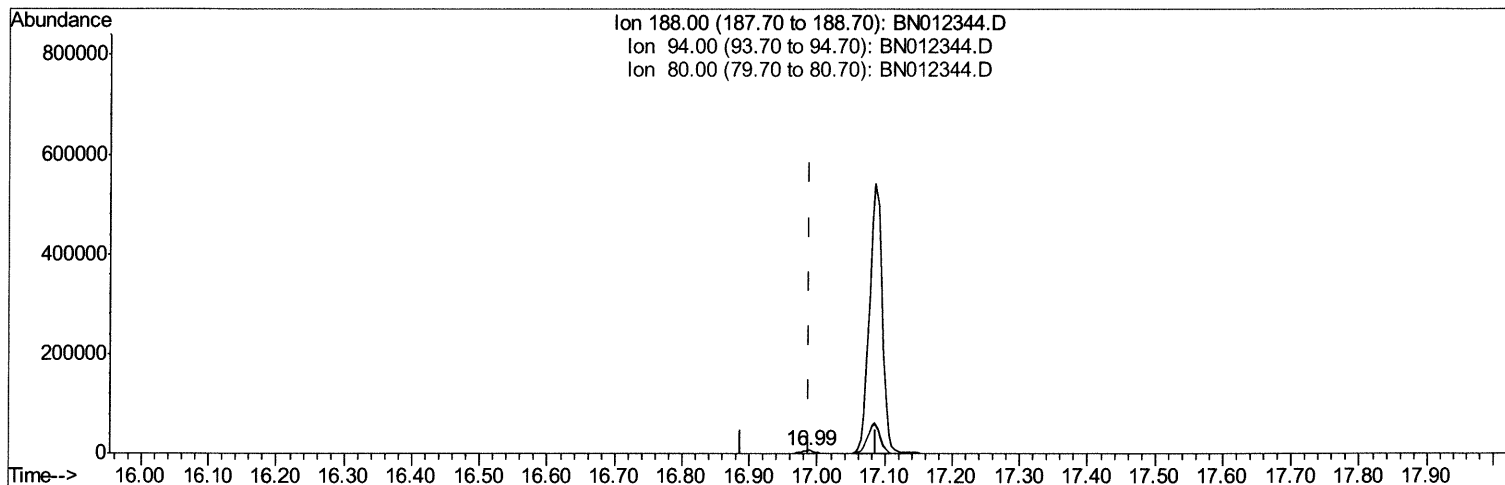

TIC: BN012344.D

(10) Phenanthrene-d10 (I)

16.988min (+0.000) 0.40ng/ul m 10/20/20 JU

response 9060

Ion	Exp%	Act%
188.00	100	100
94.00	10.20	10.02
80.00	12.00	11.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN101920\
 Data File : BN012344.D
 Acq On : 19 Oct 2020 10:40
 Operator : CG/JU
 Sample : PB132223BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK23

Manual Integrations
 APPROVED

Sohil
 10/20/2020 9:35:32 AM

Quant Time: Oct 19 11:55:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 19 11:52:04 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	1706	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	7322	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	4388	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.99	188	9060m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.19	240	7521	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	8002	0.40	ng/ul	0.00

10/20/20 34

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.97	152	3268	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	7083	0.29	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed