


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
Data File : BN012357.D
Acq On : 19 Oct 2020 18:34
Operator : CG/JU
Sample : L4286-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AQ7

Manual Integrations
APPROVED

Sohil
10/20/2020 9:36:02 AM

Quant Time: Oct 20 07:59:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 20 07:24:17 2020
Response via : Initial Calibration

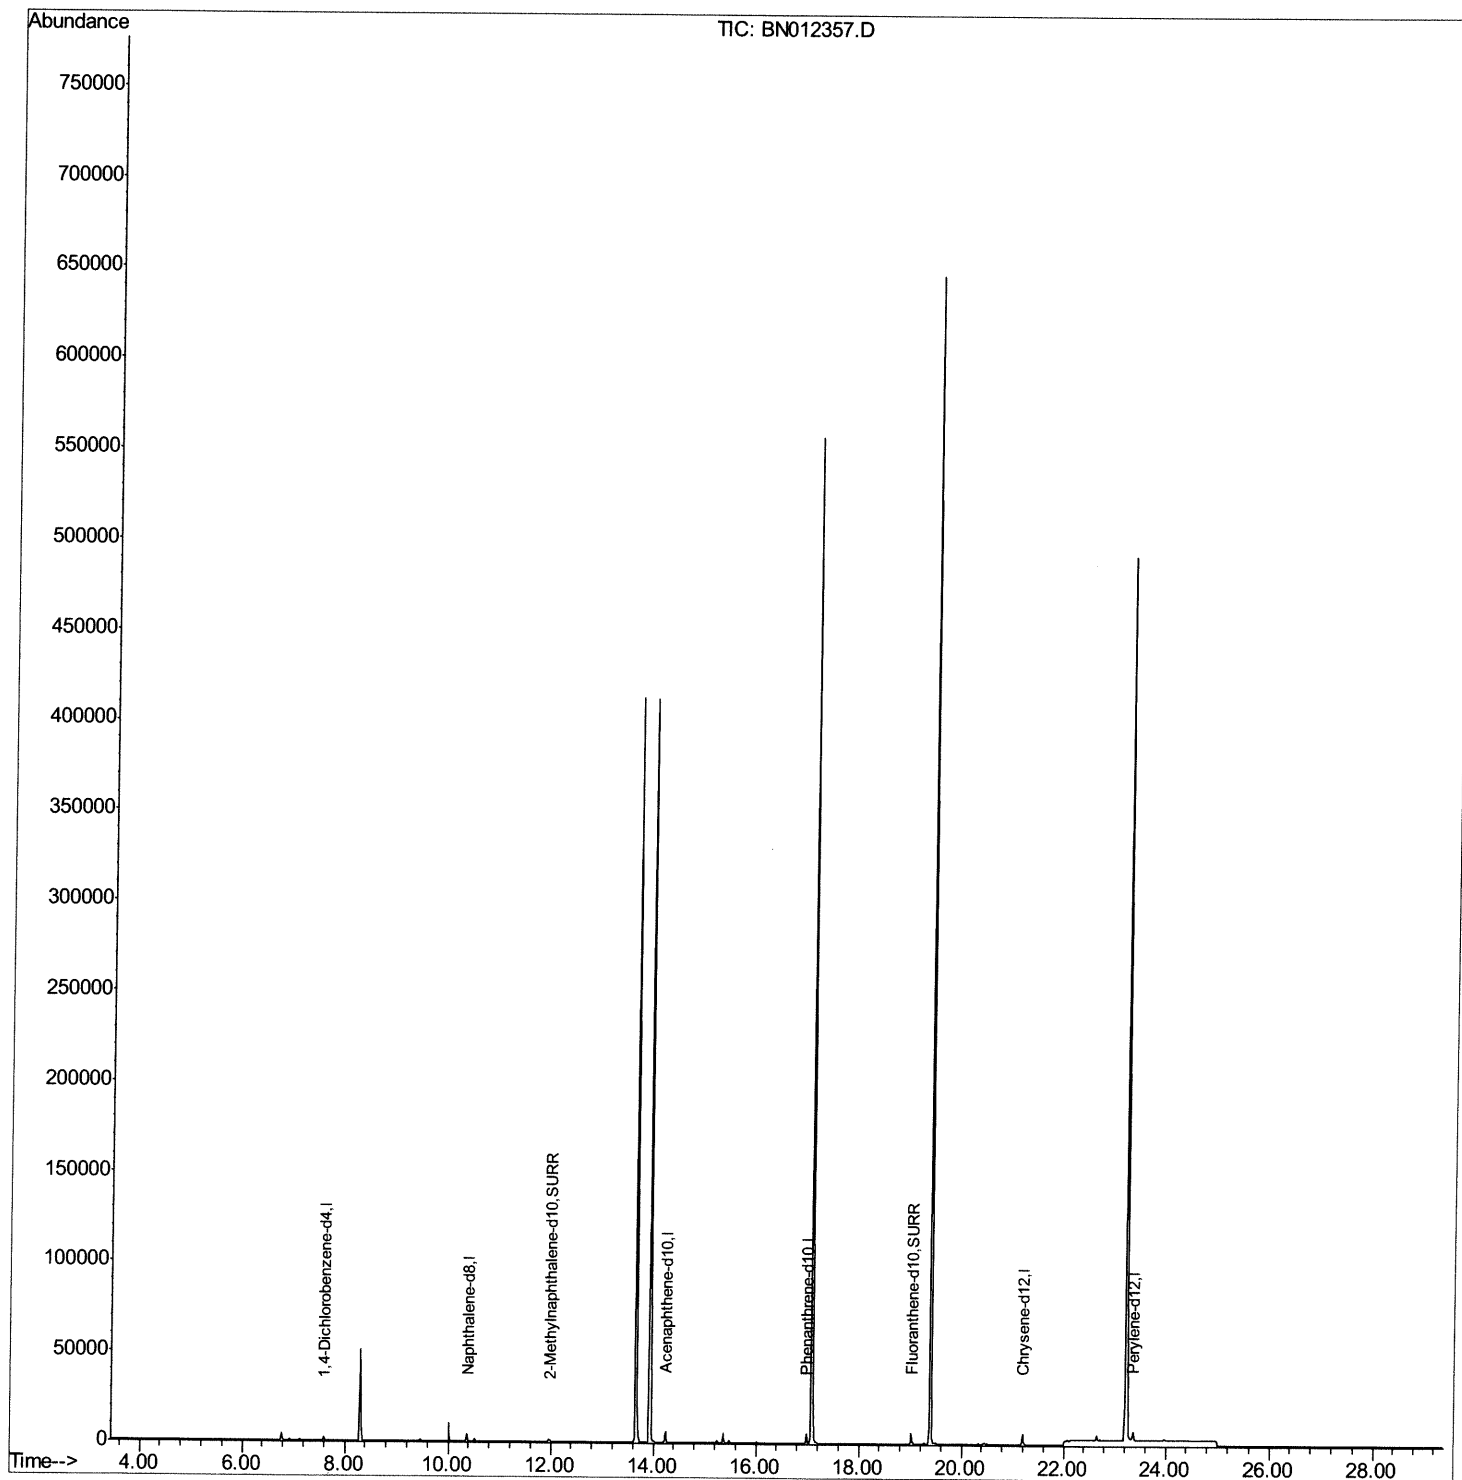

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012357.D
 Acq On : 19 Oct 2020 18:34
 Operator : CG/JU
 Sample : L4286-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AQ7

Manual Integrations
 APPROVED

Sohil
 10/20/2020 9:36:02 AM

Quant Time: Oct 20 07:31:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 07:24:17 2020
 Response via : Initial Calibration

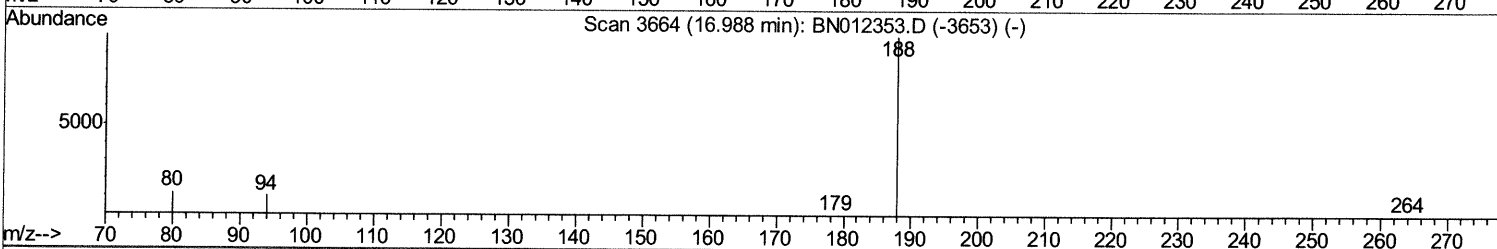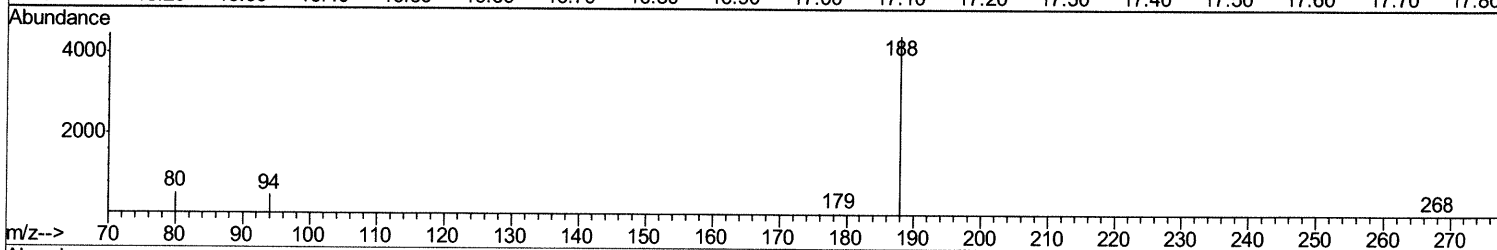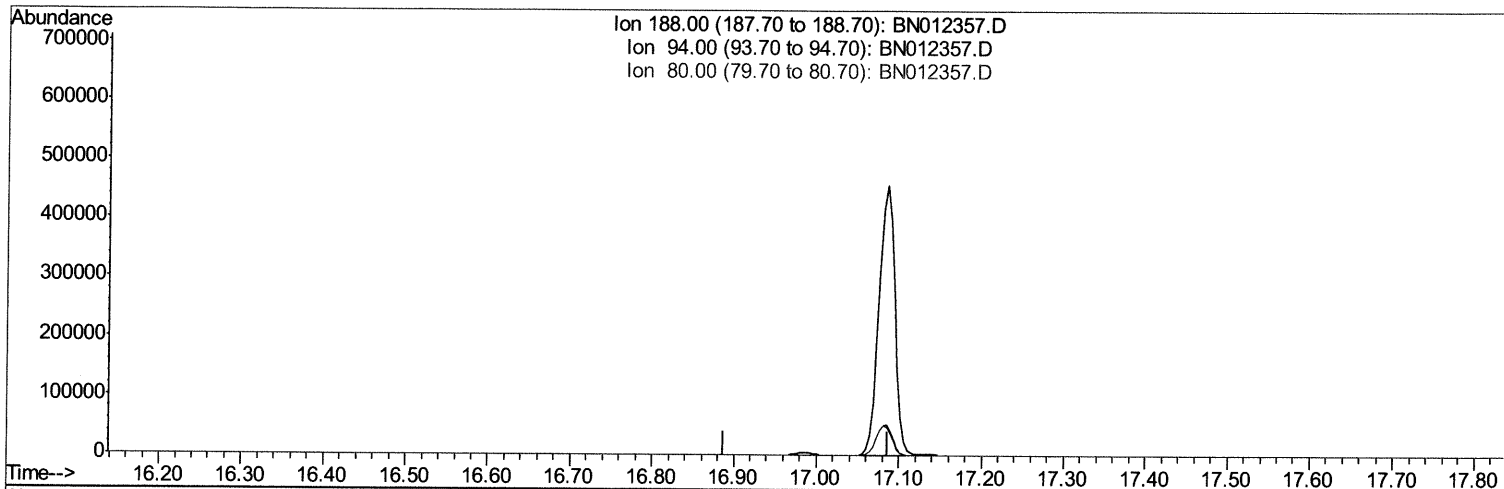

TIC: BN012357.D

(10) Phenanthrene-d10 (I)

16.988min (-16.988) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.20	0.00#
80.00	12.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012357.D
 Acq On : 19 Oct 2020 18:34
 Operator : CG/JU
 Sample : L4286-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AQ7

Manual Integrations
 APPROVED

Sohil
 10/20/2020 9:36:02 AM

Quant Time: Oct 20 07:31:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 07:24:17 2020
 Response via : Initial Calibration

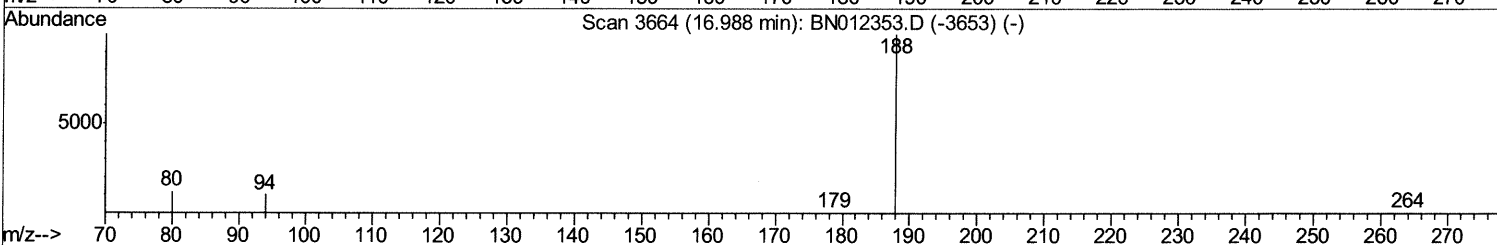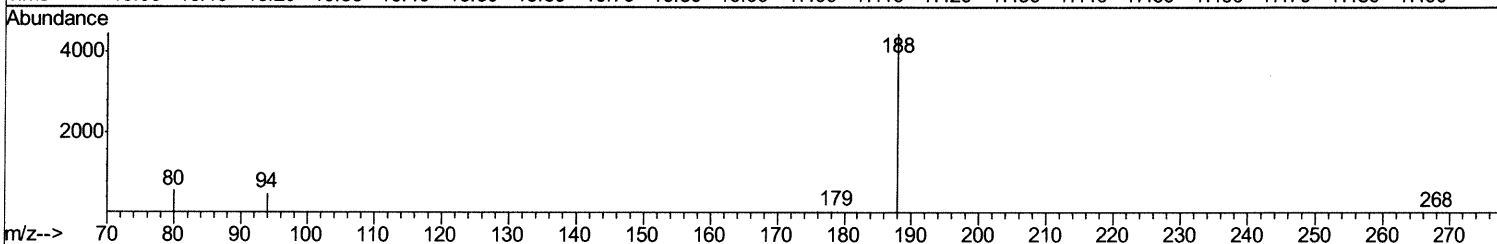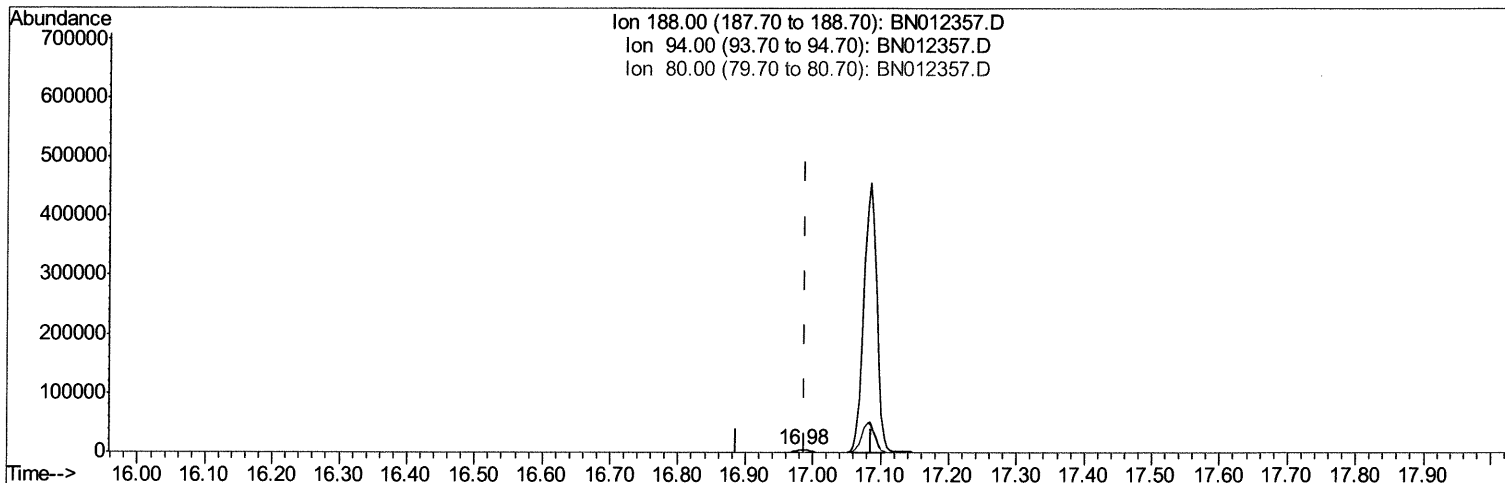

TIC: BN012357.D

(10) Phenanthrene-d10 (I)

16.983min (-0.004) 0.40ng/ul m 10/20/2020

response 6330

Ion	Exp%	Act%
188.00	100	100
94.00	10.20	11.26
80.00	12.00	12.96
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012357.D
 Acq On : 19 Oct 2020 18:34
 Operator : CG/JU
 Sample : L4286-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AQ7

Manual Integrations
 APPROVED

Sohil
 10/20/2020 9:36:02 AM

Quant Time: Oct 20 07:59:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 07:24:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	1220	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	5307	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	3156	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	6330m	0.40	ng/ul	0.00
16) Chrysene-d12	21.19	240	5532	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	5655	0.40	ng/ul	0.00

10/20/2020 SV

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.97	152	2865	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	6817	0.39	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed