

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012361.D
 Acq On : 19 Oct 2020 20:58
 Operator : CG/JU
 Sample : L4424-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F4W01

Manual Integrations
 APPROVED

Sohil
 10/20/2020 9:36:11 AM

Quant Time: Oct 20 08:11:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 07:24:17 2020
 Response via : Initial Calibration

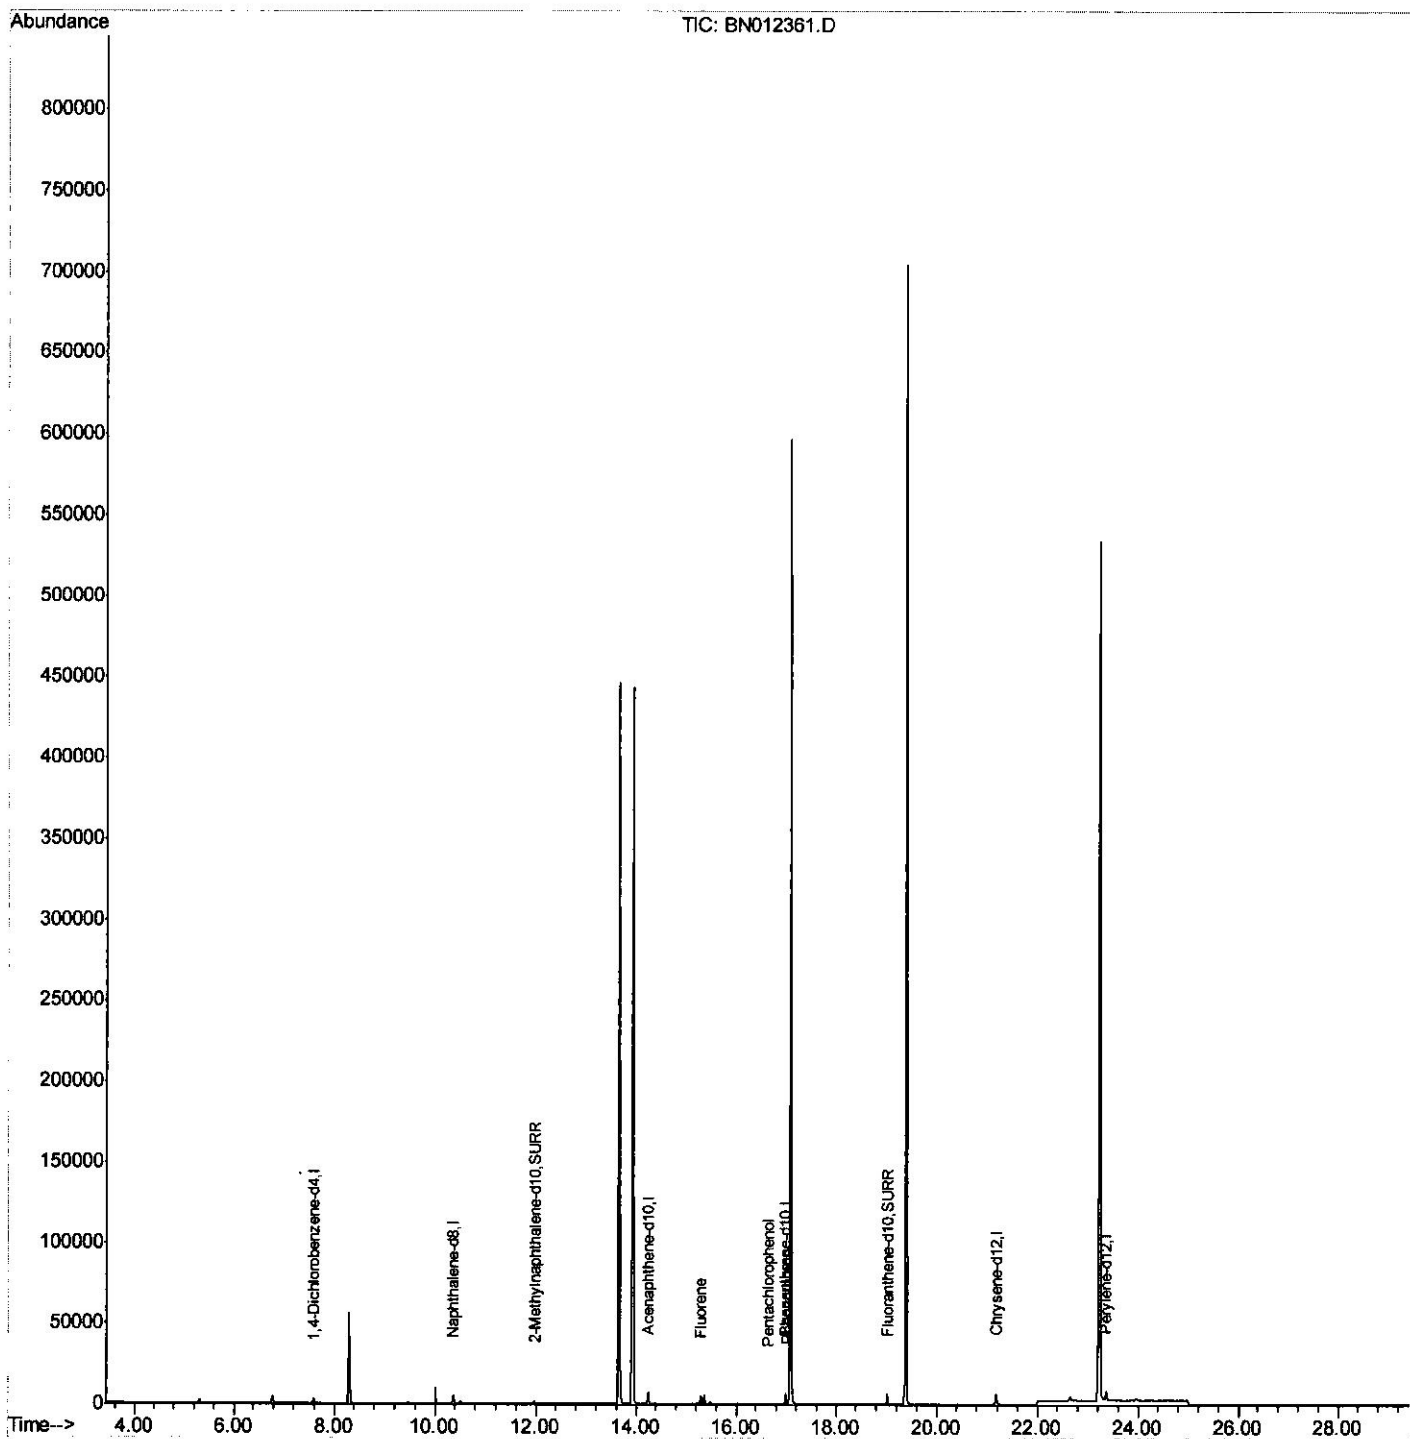

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012361.D
 Acq On : 19 Oct 2020 20:58
 Operator : CG/JU
 Sample : L4424-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F4W01

Manual Integrations
 APPROVED

Sohil
 10/20/2020 9:36:11 AM

Quant Time: Oct 20 07:31:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 07:24:17 2020
 Response via : Initial Calibration

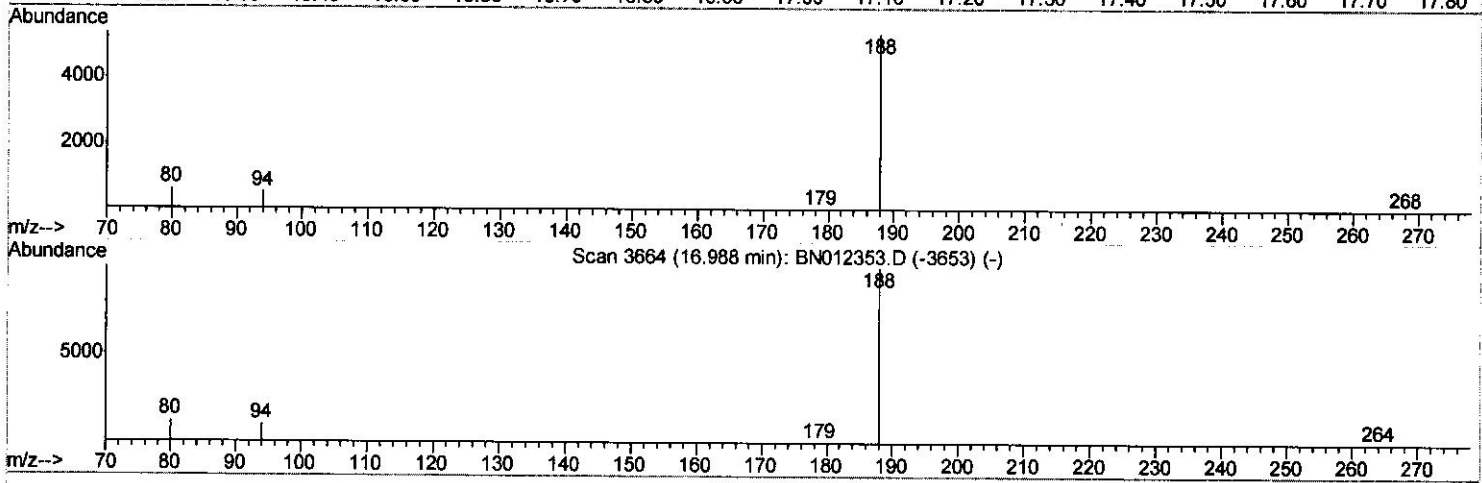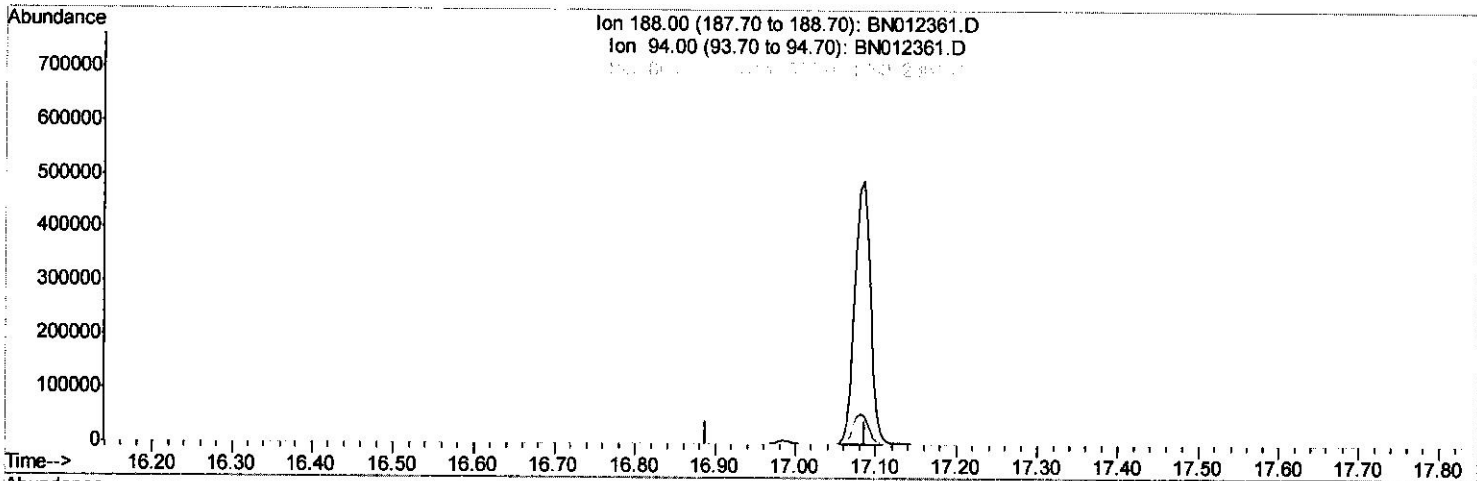

TIC: BN012361.D

(10) Phenanthrene-d10 (I)

16.988min (-16.988) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.20	0.00#
80.00	12.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012361.D
 Acq On : 19 Oct 2020 20:58
 Operator : CG/JU
 Sample : L4424-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 F4W01

Manual Integrations
 APPROVED

Sohil
 10/20/2020 9:36:11 AM

Quant Time: Oct 20 08:11:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 07:24:17 2020
 Response via : Initial Calibration

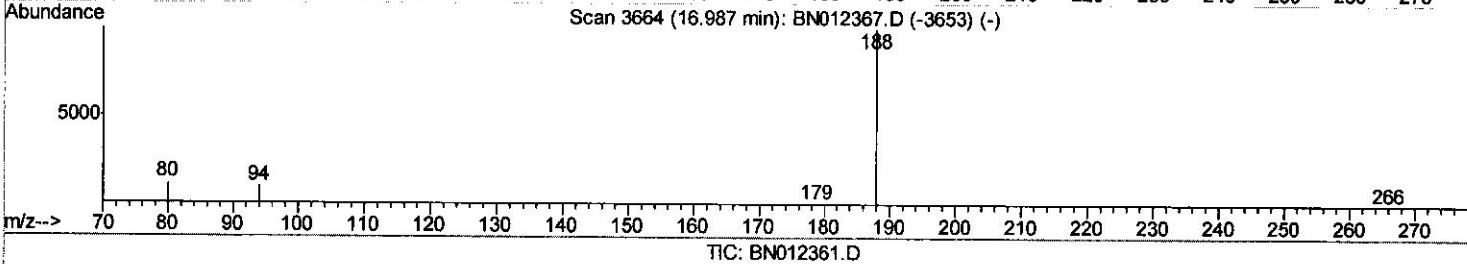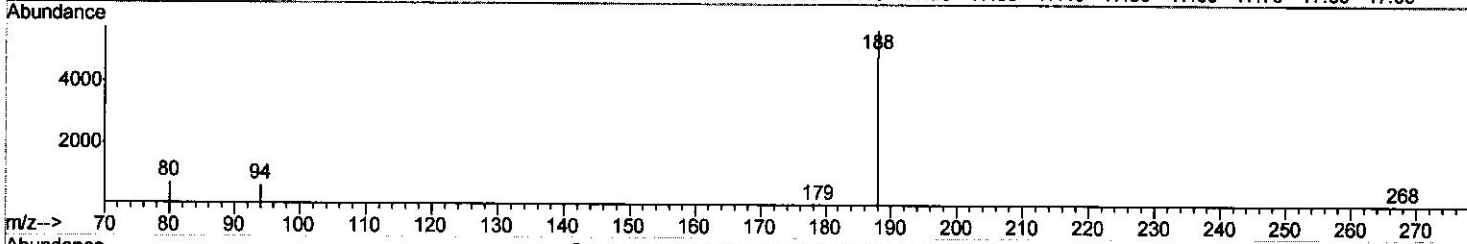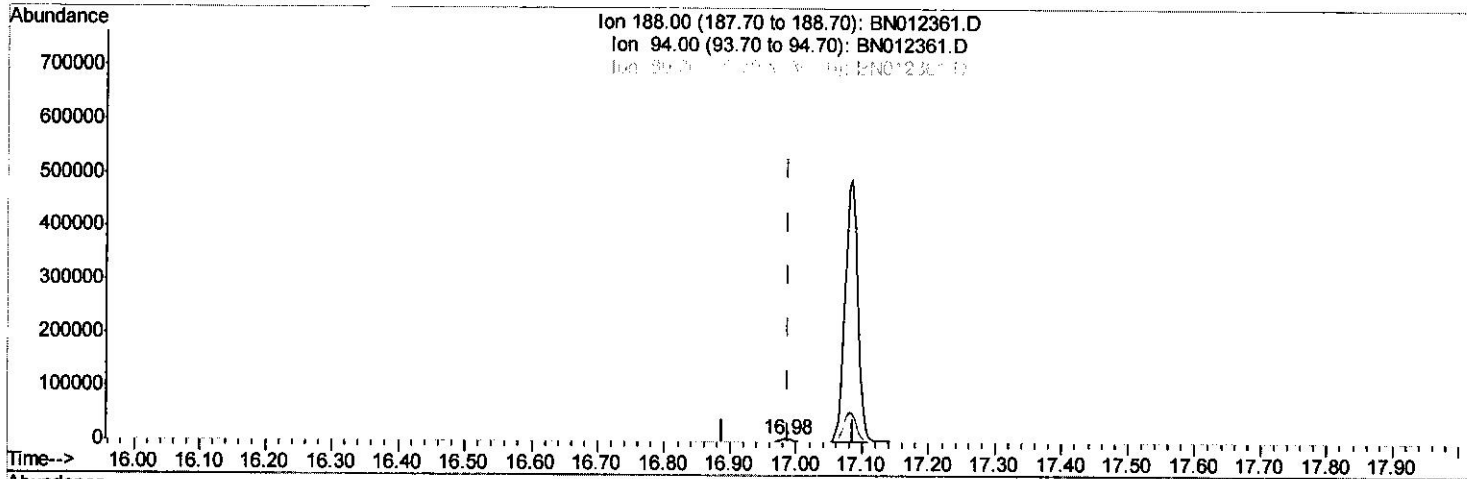

(10) Phenanthrene-d10 (I)

16.983min (-0.004) 0.40ng/ul m } JU
 10/21/2020

response 7908

Ion	Exp%	Act%
188.00	100	100
94.00	10.20	11.18
80.00	12.00	12.37
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012361.D
 Acq On : 19 Oct 2020 20:58
 Operator : CG/JU
 Sample : L4424-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 Client Sampled :
 F4W01

Manual Integrations
 APPROVED

Sohil
 10/20/2020 9:36:11 AM

Quant Time: Oct 20 08:11:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 07:24:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	1536	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	6604	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	3837	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	7908m ¹	0.40	ng/ul	0.00
16) Chrysene-d12	21.19	240	6661	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	6935	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	3091	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	7390	0.34	ng/ul	0.00
Target Compounds				Ovalue		
9) Fluorene	15.29	166	3062	0.196	ng/ul	99
11) Pentachlorophenol	16.64	266	256	0.112	ng/ul	95
12) Phenanthrene	17.03	178	1268	0.050	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed