


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
Data File : BN012365.D
Acq On : 19 Oct 2020 23:23
Operator : CG/JU
Sample : L4424-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F4W05

Manual Integrations
APPROVED

Sohil
10/20/2020 9:36:21 AM

Quant Time: Oct 20 08:21:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 20 07:24:17 2020
Response via : Initial Calibration

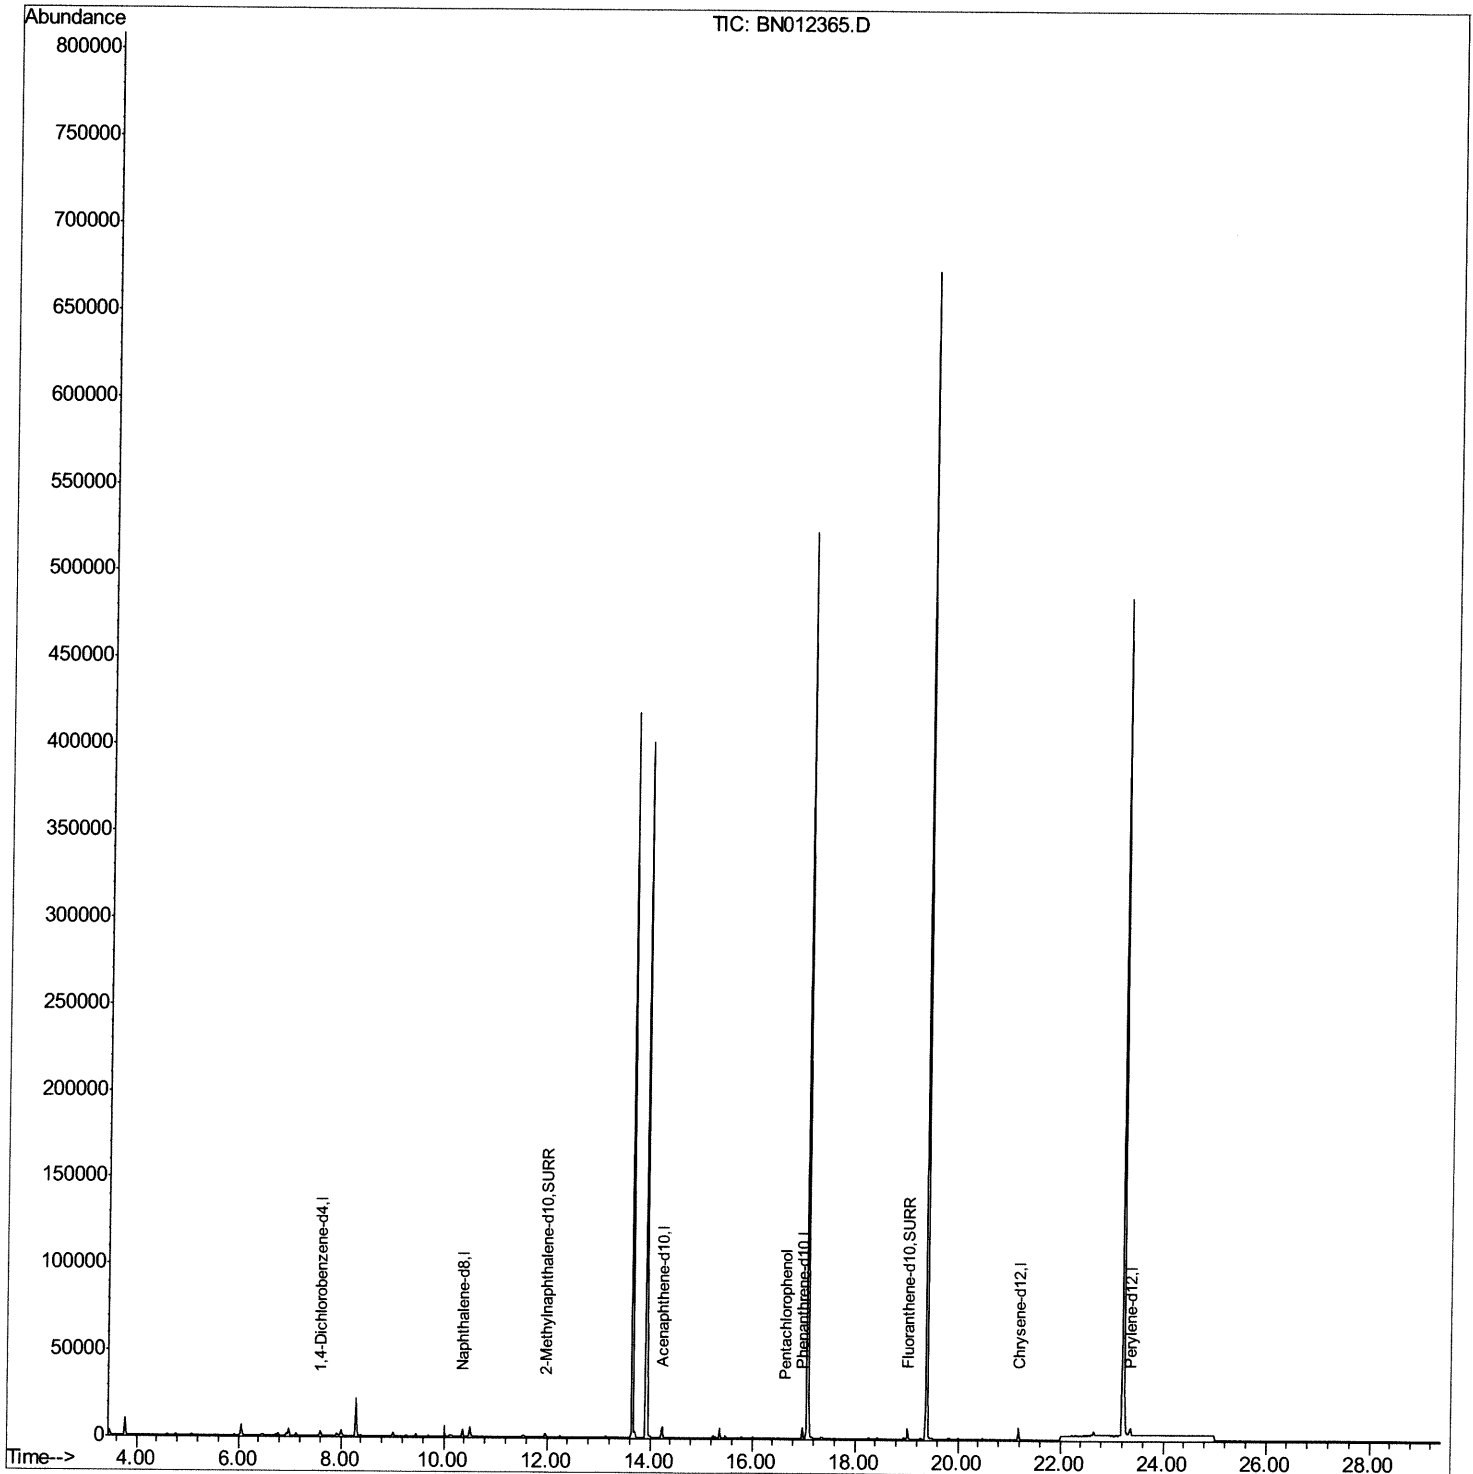

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012365.D
 Acq On : 19 Oct 2020 23:23
 Operator : CG/JU
 Sample : L4424-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F4W05

Manual Integrations
 APPROVED

Sohil
 10/20/2020 9:36:21 AM

Quant Time: Oct 20 07:31:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 07:24:17 2020
 Response via : Initial Calibration

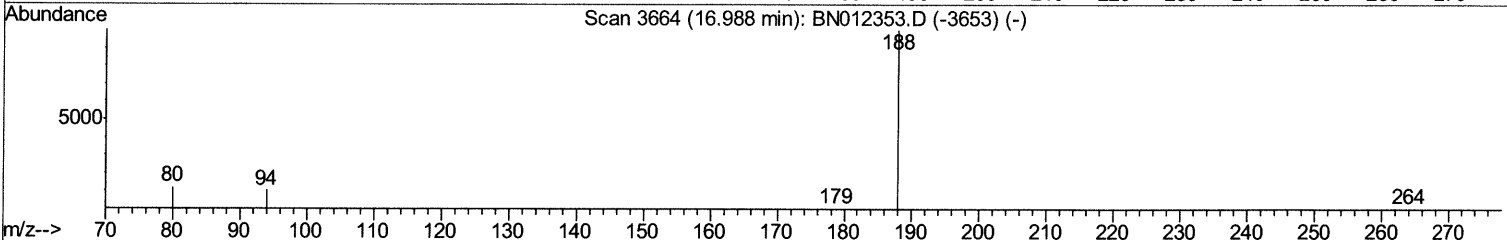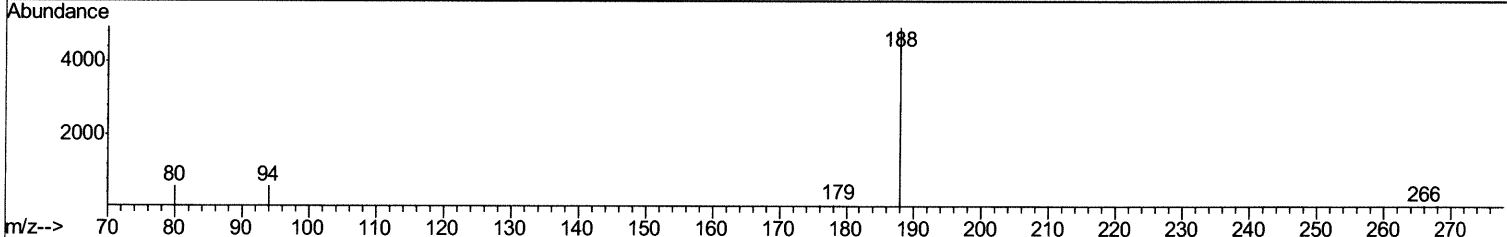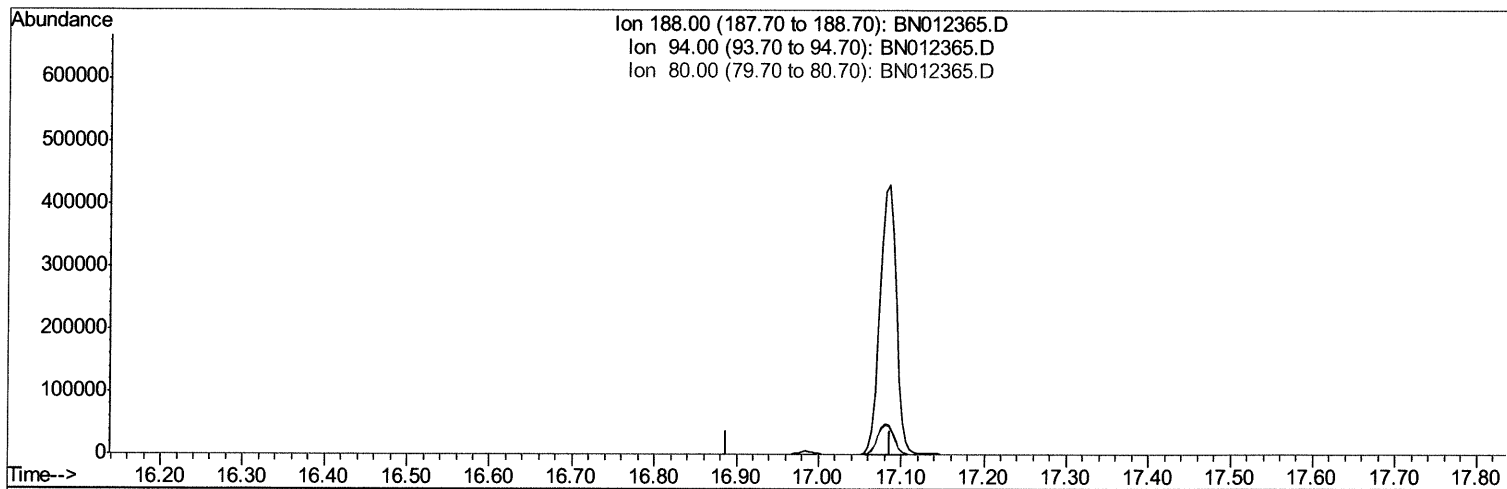

TIC: BN012365.D

(10) Phenanthrene-d10 (I)

16.988min (-16.988) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.20	0.00#
80.00	12.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012365.D
 Acq On : 19 Oct 2020 23:23
 Operator : CG/JU
 Sample : L4424-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F4W05

Manual Integrations
 APPROVED

Sohil
 10/20/2020 9:36:21 AM

Quant Time: Oct 20 07:31:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 07:24:17 2020
 Response via : Initial Calibration

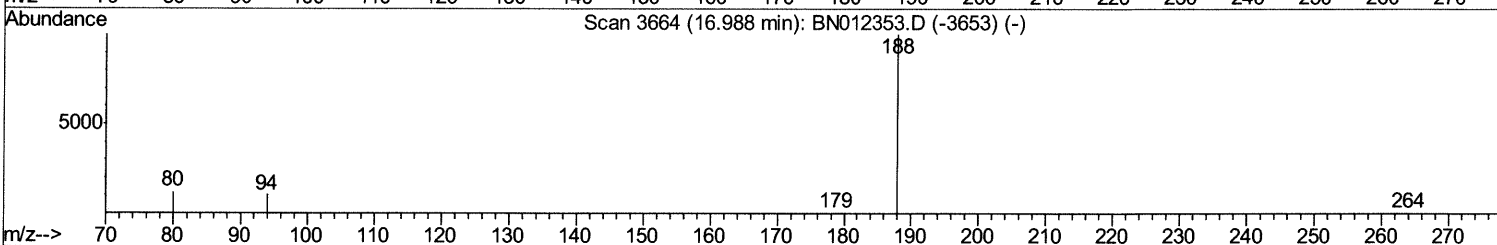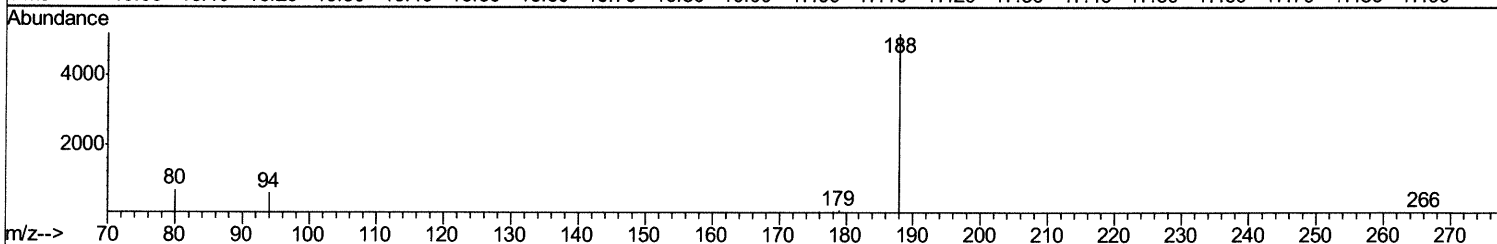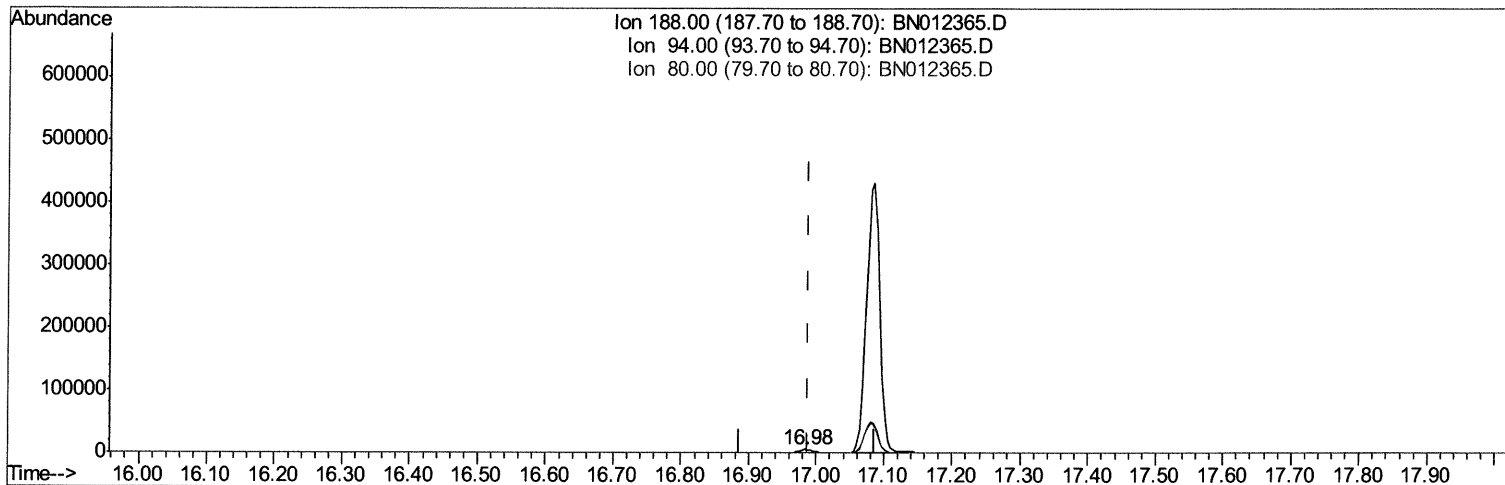

TIC: BN012365.D

(10) Phenanthrene-d10 (I)

16.983min (-0.004) 0.40ng/ul m 10/20/20 JU

response 7178

Ion	Exp%	Act%
188.00	100	100
94.00	10.20	11.80
80.00	12.00	13.34
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012365.D
 Acq On : 19 Oct 2020 23:23
 Operator : CG/JU
 Sample : L4424-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F4W05

Manual Integrations
 APPROVED

Sohil
 10/20/2020 9:36:21 AM

Quant Time: Oct 20 08:21:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 07:24:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	1356	0.40	ng/ul	0.00
2) Naphthalene-d8	10.36	136	5739	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	3423	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	7178m >	0.40	ng/ul >	0.00 10/20/20 54
16) Chrysene-d12	21.18	240	6134	0.40	ng/ul	0.00
20) Perylene-d12	23.35	264	6125	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.96	152	3011	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	6997	0.36	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.64	266	90	0.043	ng/ul	Ovalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed