

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012354.D
 Acq On : 19 Oct 2020 16:45
 Operator : CG/JU
 Sample : L4286-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AR3

Manual Integrations
 APPROVED

Sohil
 10/20/2020 9:35:55 AM

Quant Time: Oct 19 17:16:21 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 19 11:52:04 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	1365	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	5819	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	3362	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.99	188	6712m	0.40	ng/ul	0.00
16) Chrysene-d12	21.19	240	5765	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	5974	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	2744	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	6332	0.34	ng/ul	0.00
Target Compounds						
7) Acenaphthylene	13.95	152	381	0.026	ng/ul#	48
11) Pentachlorophenol	16.64	266	213	0.110	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
Data File : BN012354.D
Acq On : 19 Oct 2020 16:45
Operator : CG/JU
Sample : L4286-01
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AR3

Manual Integrations
APPROVED

Sohil
10/20/2020 9:35:55 AM

Quant Time: Oct 19 17:16:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 19 11:52:04 2020
Response via : Initial Calibration

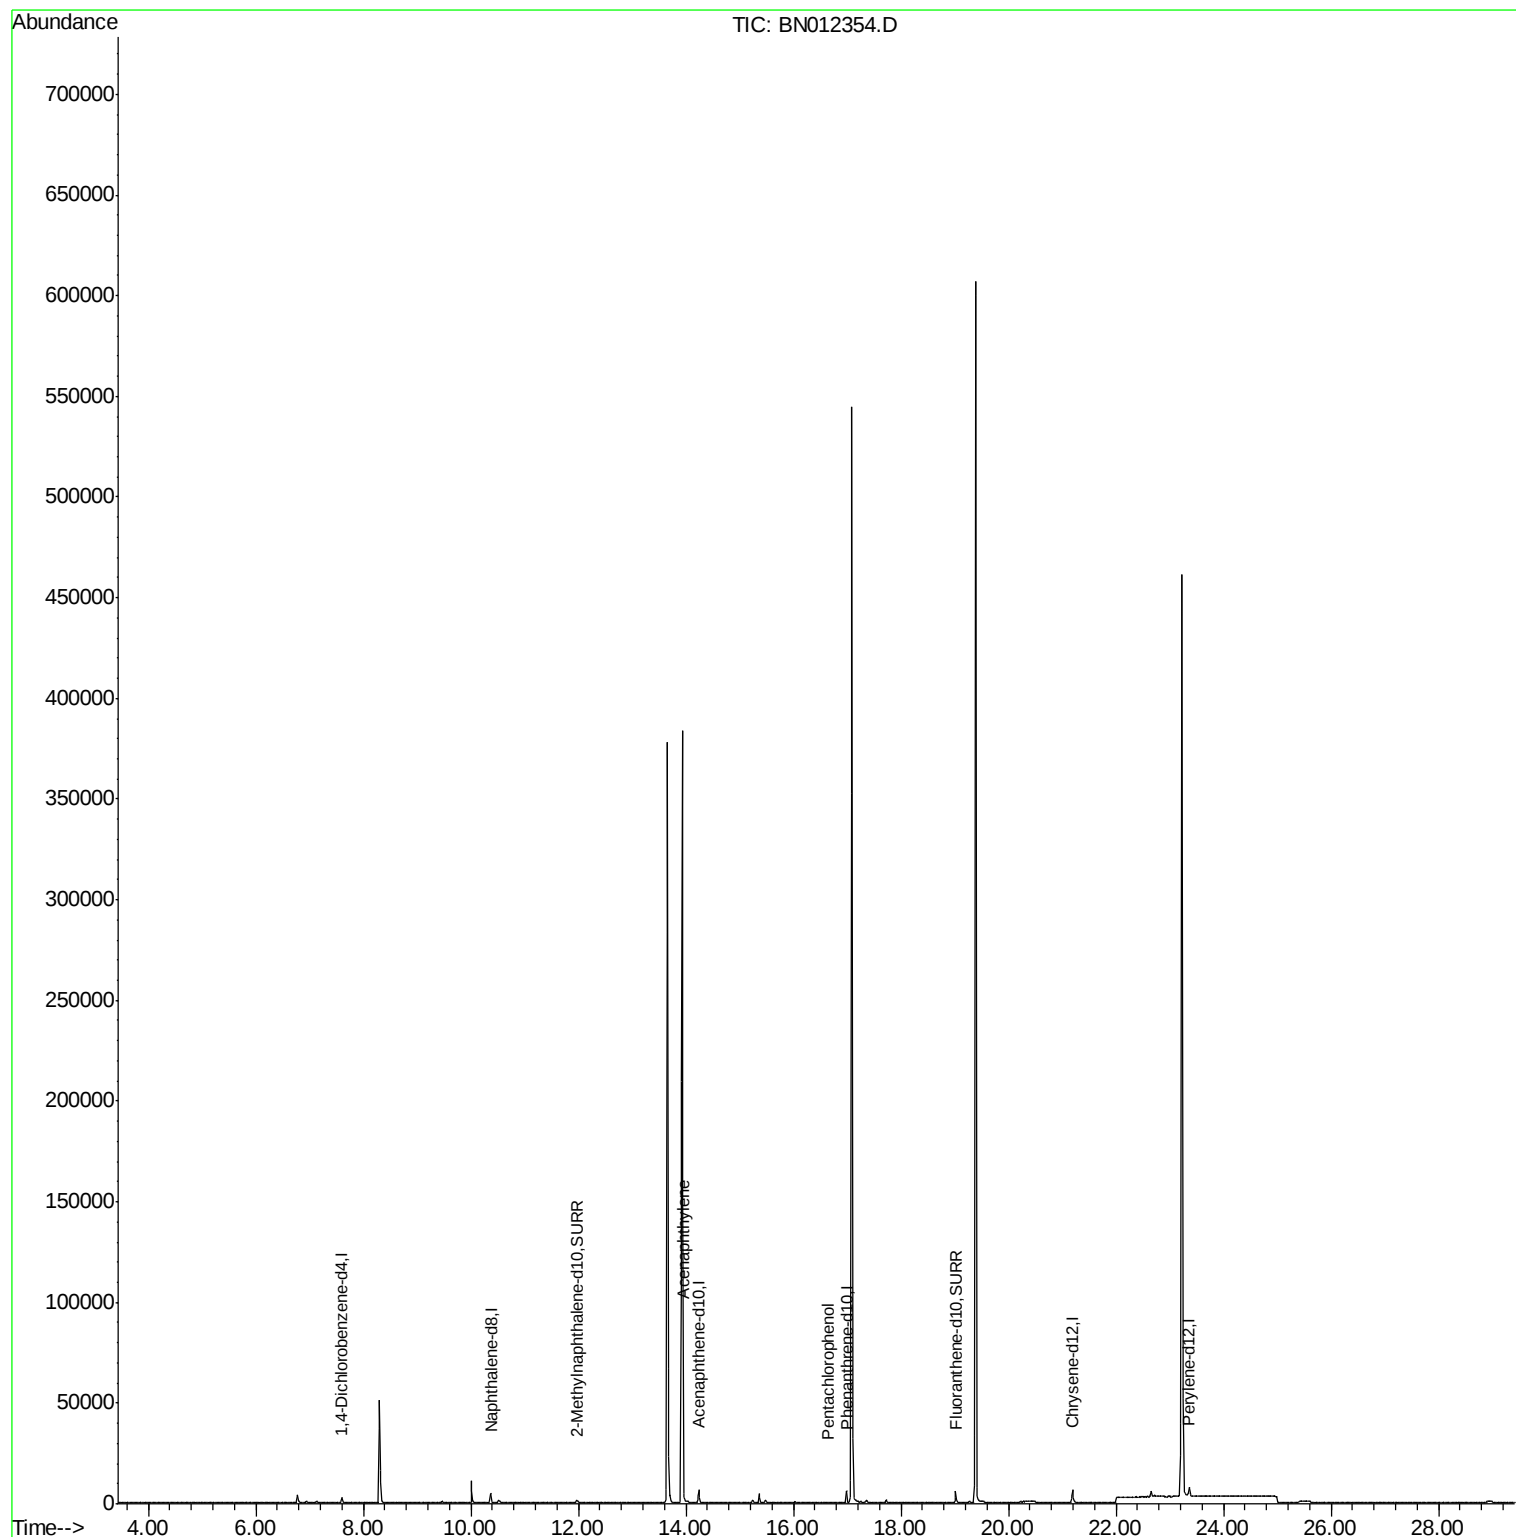

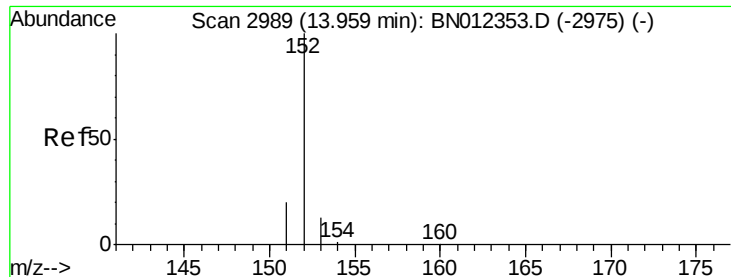

#7

Acenaphthylene

Concen: 0.026 ng/ul

RT: 13.95 min Scan# 2988

Delta R.T. -0.00 min

Lab File: BN012354.D

Acq: 19 Oct 2020 16:45

Instrument :

BNA_N





ClientSampled :

C0AR3

Tot Ion:	152	Resp:	381
Ion Ratio	Lower	Upper	
152	100		
151	43.5	16.6	24.8#
153	37.5	11.4	17.0#

Manual Integrations
APPROVED

Sohil
10/20/2020 9:35:55 AM

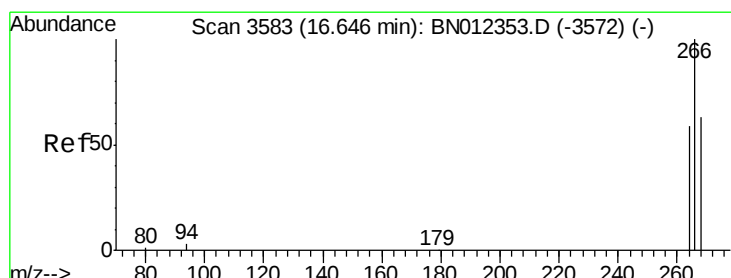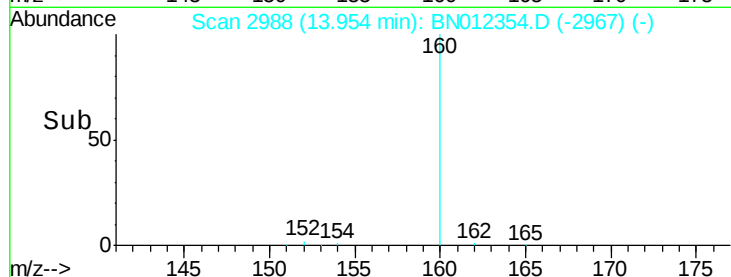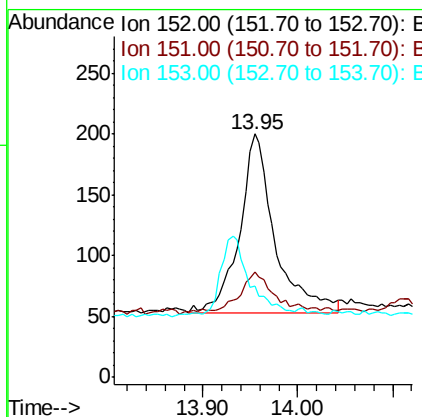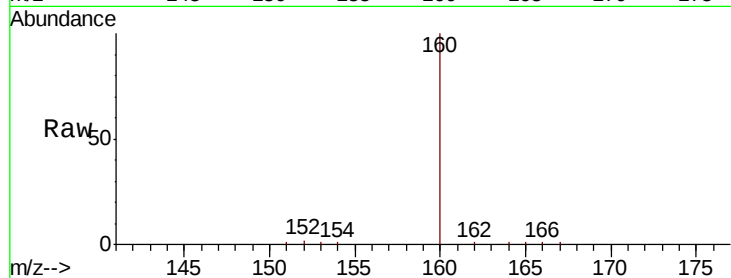

#11

Pentachlorophenol

Concen: 0.110 ng/ul

RT: 16.64 min Scan# 3582

Delta R.T. -0.00 min

Lab File: BN012354.D

Acq: 19 Oct 2020 16:45

Tgt Ion:	266	Resp:	213
Ion Ratio	Lower	Upper	
266	100		
264	64.3	49.5	74.3
268	64.3	50.5	75.7

