

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
 Data File : BN012360.D
 Acq On : 19 Oct 2020 20:22
 Operator : CG/JU
 Sample : L4424-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F4W00

Manual Integrations
 APPROVED

Sohil

10/20/2020 9:36:09 AM

Quant Time: Oct 20 08:09:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 07:24:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	1552	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	6574	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	3771	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	7544m	0.40	ng/ul	0.00
16) Chrysene-d12	21.19	240	6504	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	6833	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	2793	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	6340	0.31	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.65	266	95	0.044	ng/ul	Ovalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101920\
Data File : BN012360.D
Acq On : 19 Oct 2020 20:22
Operator : CG/JU
Sample : L4424-01
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
F4W00




Quant Time: Oct 20 08:09:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 20 07:24:17 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil

10/20/2020 9:36:09 AM

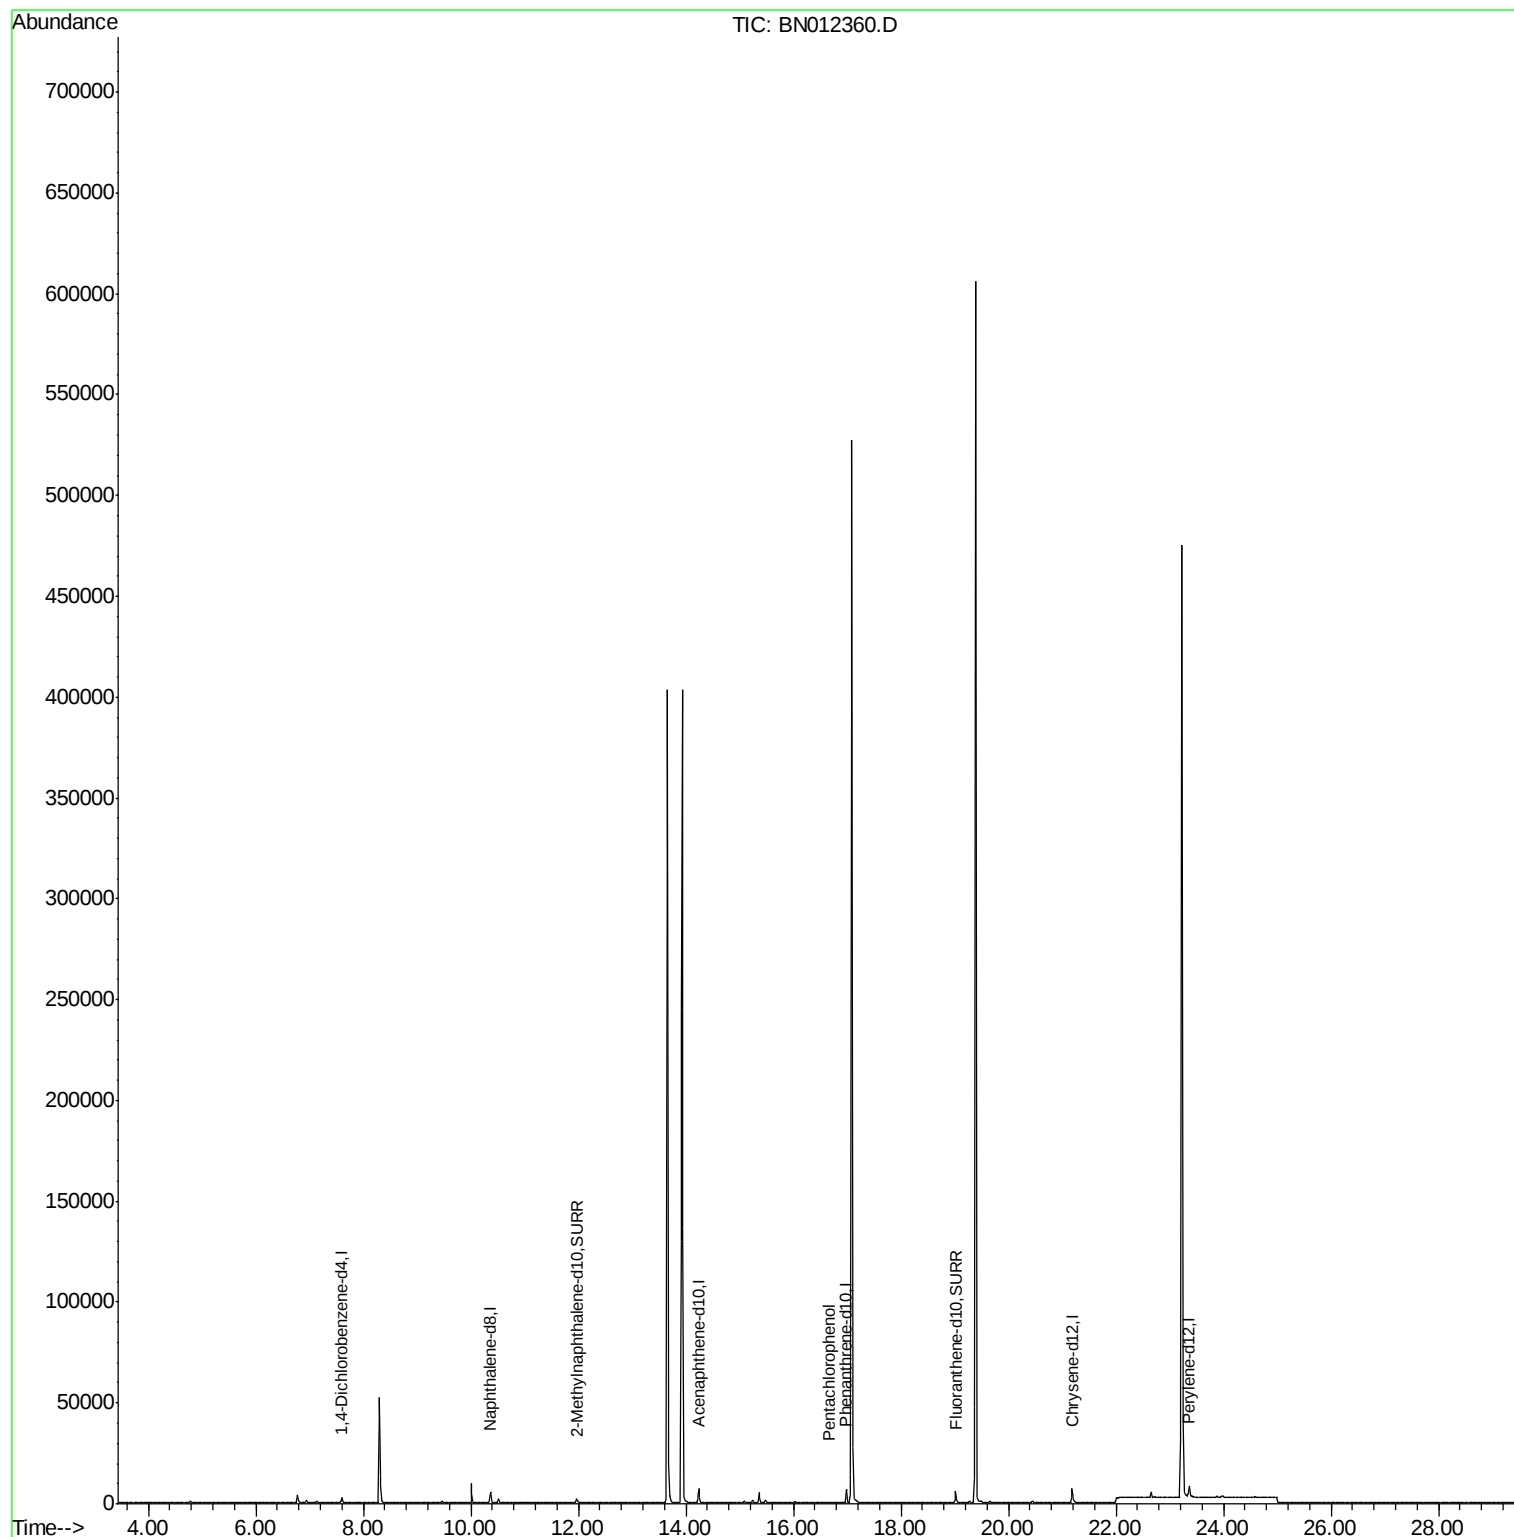

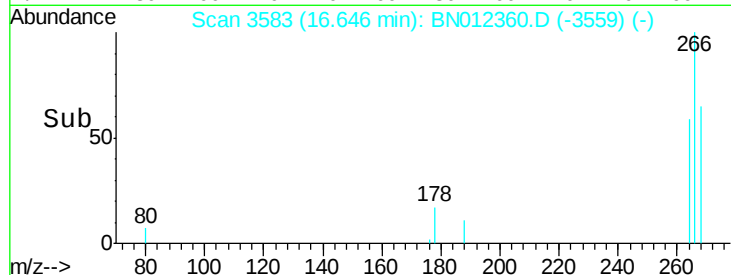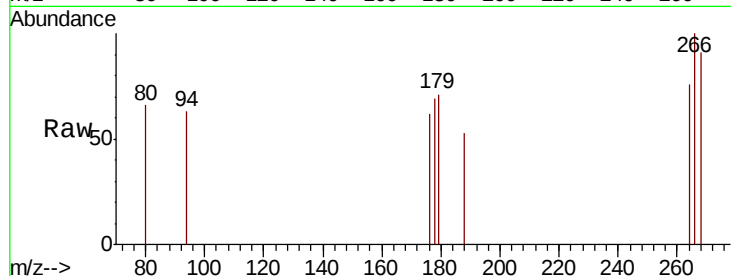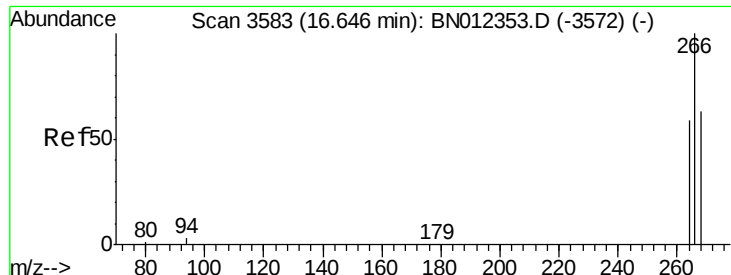

#11
 Pentachlorophenol
 Concen: 0.044 ng/ul
 RT: 16.65 min Scan# 3583
 Delta R.T. 0.00 min
 Lab File: BN012360.D
 Acq: 19 Oct 2020 20:22

Instrument :
 BNA_N
 ClientSampleId :
 F4W00

Tot Ion	Ratio	Lower	Upper
266	100		
264	61.1	49.5	74.3
268	72.6	50.5	75.7

Manual Integrations
 APPROVED

Sohil

10/20/2020 9:36:09 AM

