
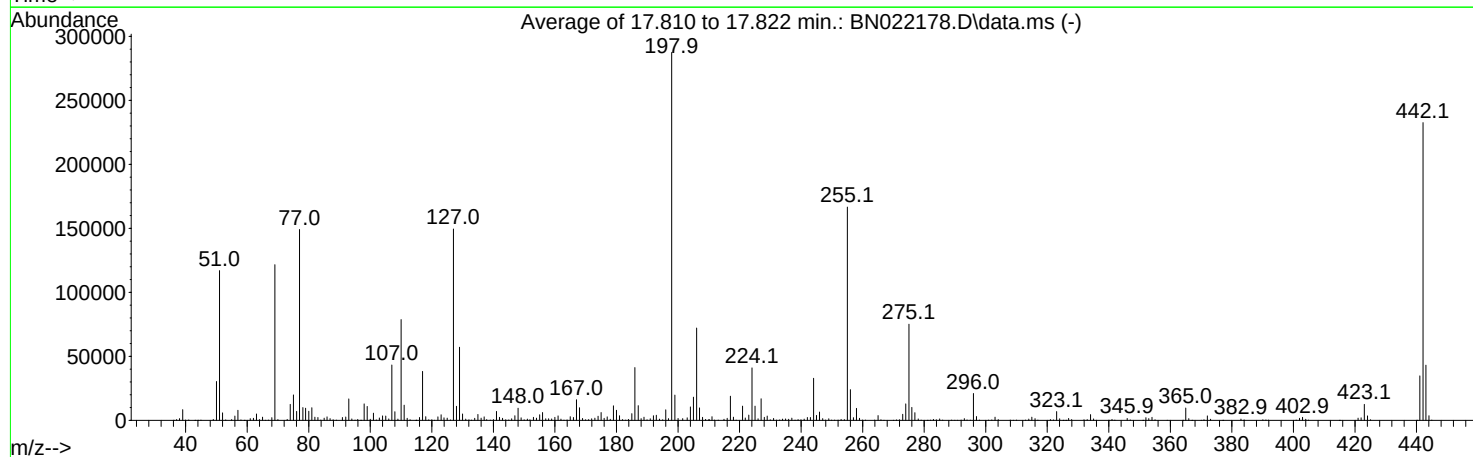


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101922\
 Data File : BN022178.D
 Acq On : 18 Oct 2022 15:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 19 02:07:41 2022

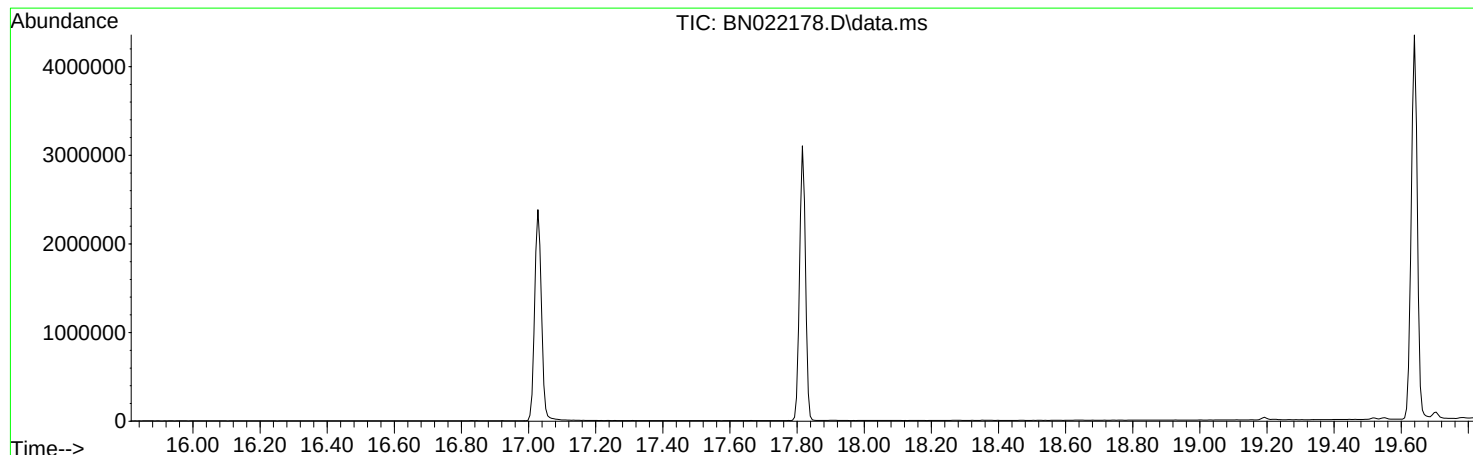




AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	116984	PASS
68	69	0.00	2	1.7	2099	PASS
69	198	0.00	100	42.3	121595	PASS
70	69	0.00	2	0.6	678	PASS
127	198	10	80	52.0	149475	PASS
197	198	0.00	2	0.5	1436	PASS
198	198	100	100	100.0	287424	PASS
199	198	5	9	6.9	19720	PASS
275	198	10	60	26.1	75099	PASS
365	198	1	100	3.4	9657	PASS
441	198	0.01	100	12.1	34725	PASS
442	442	50	100	100.0	232704	PASS
443	442	15	24	18.5	43101	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101922\
 Data File : BN022178.D
 Acq On : 18 Oct 2022 15:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 19 05:54:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 05:54:08 2022
 Response via : Initial Calibration

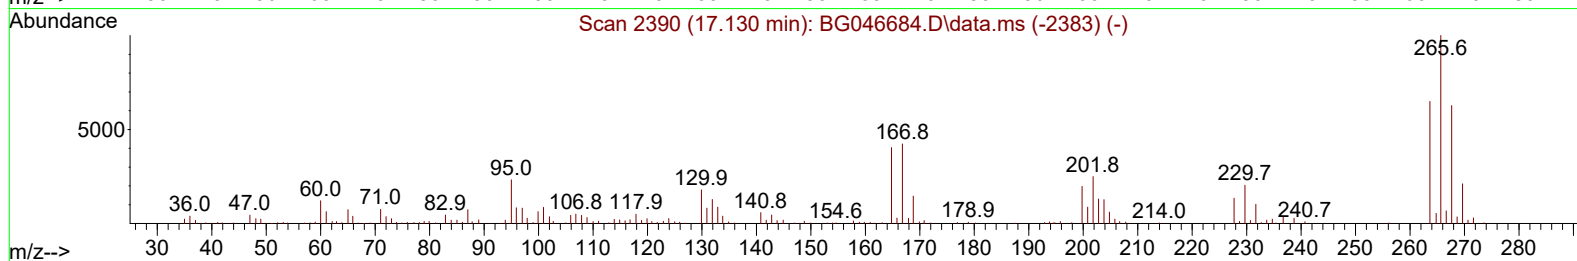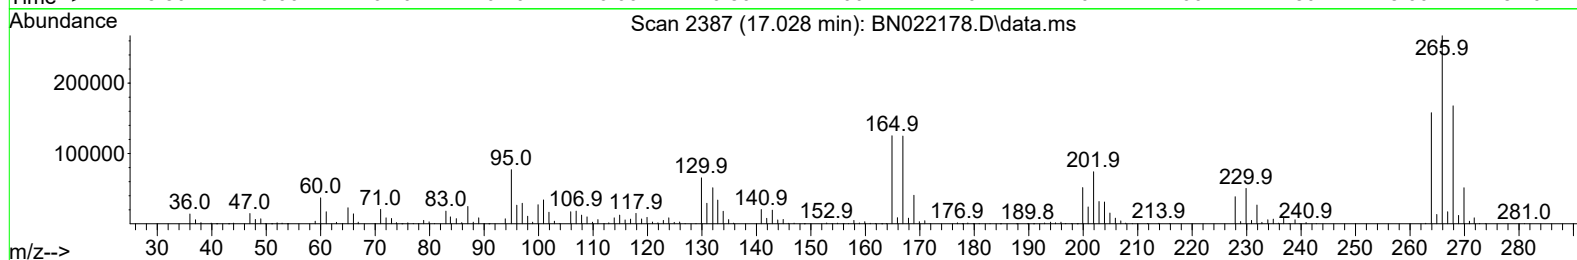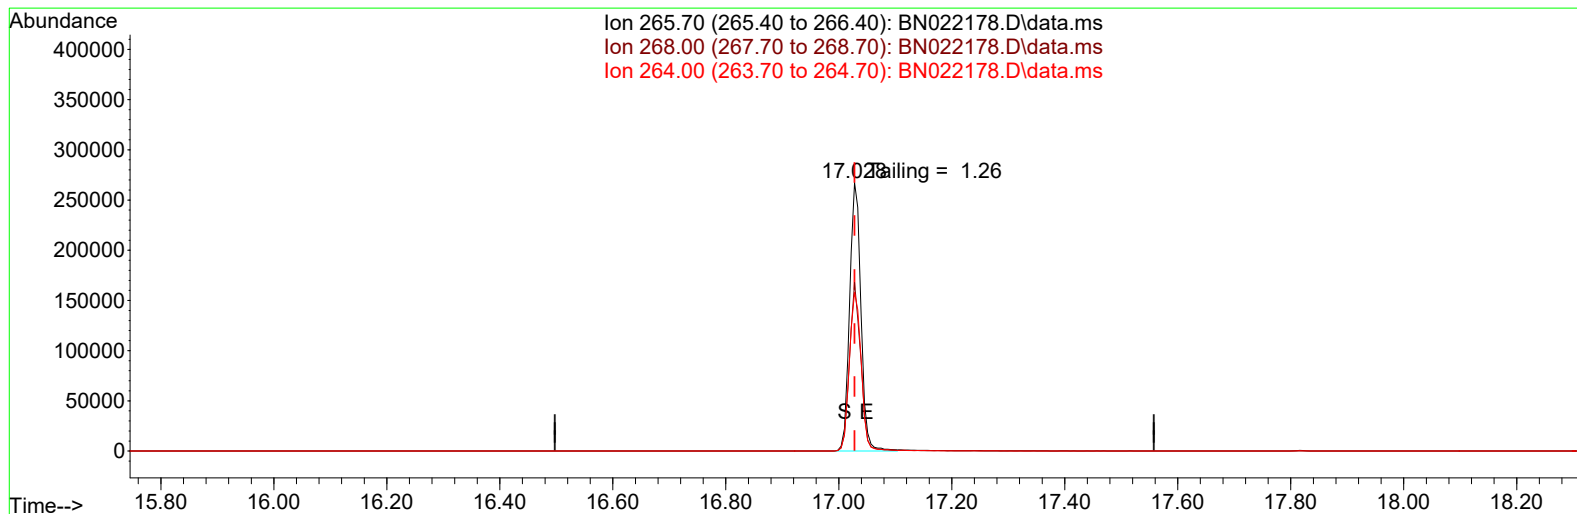

TIC: BN022178.D\data.ms

(70) Pentachlorophenol (C)

17.028min (0.000) 24272.18 ng




response 375059

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.75
264.00	61.60	59.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101922\
Data File : BN022178.D
Acq On : 18 Oct 2022 15:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 19 05:54:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 05:54:08 2022
Response via : Initial Calibration

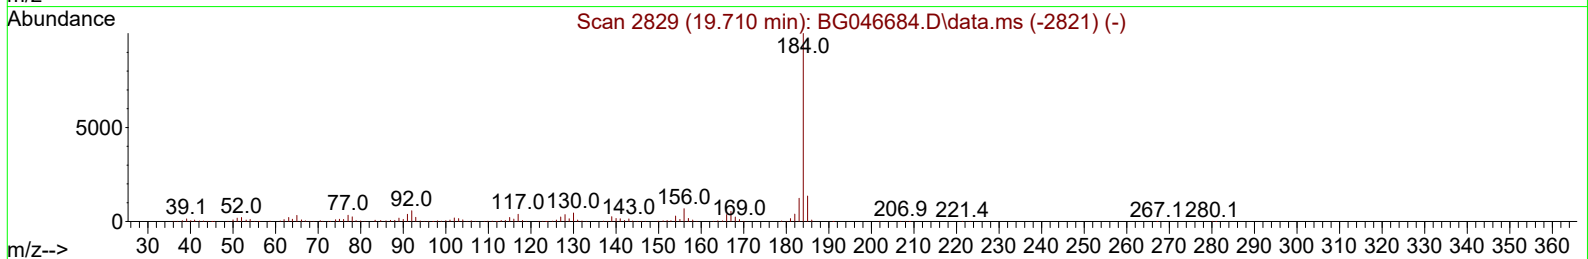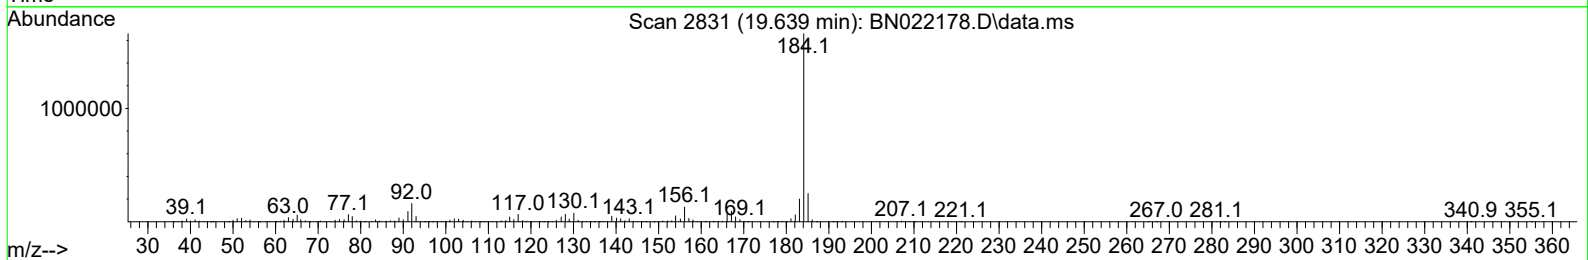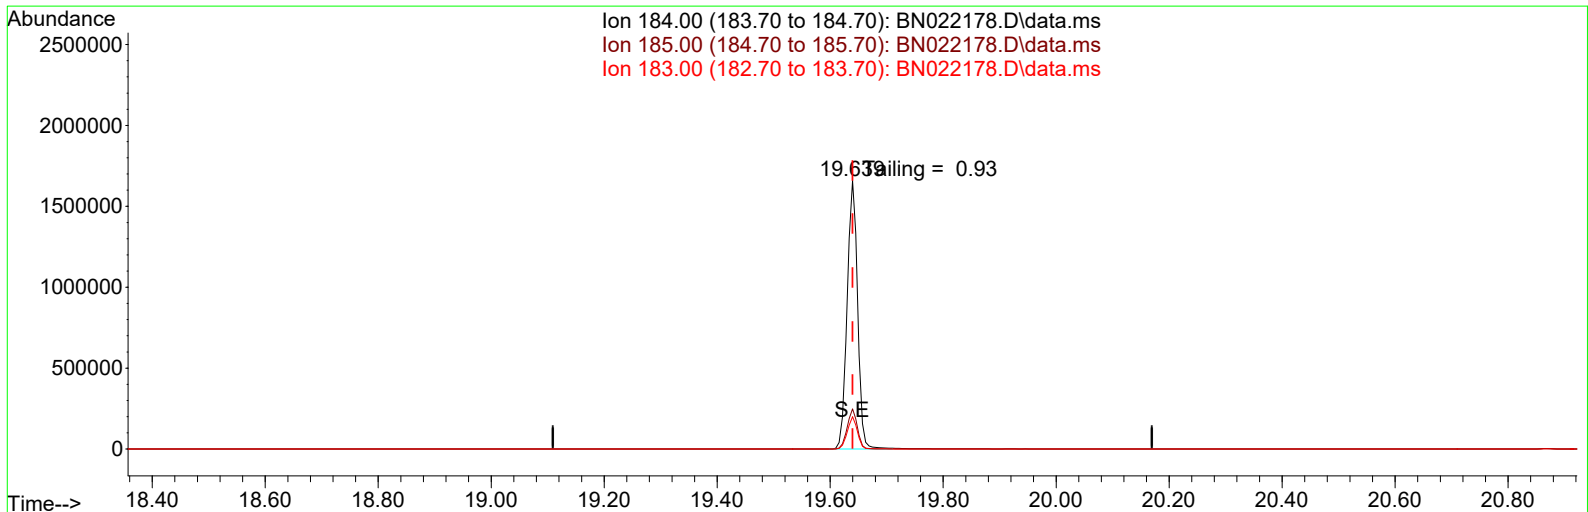

TIC: BN022178.D\data.ms

(77) Benzidine

19.639min (0.000) 106630.09 ng

response 2129919

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.97
183.00	13.20	12.06
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/19/2022	BNA_N	<u>BN022178.D</u>
Compound Name	Response	Retention Time
DDT	855309	20.869
DDD	104291	20.428
DDE	7672	19.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
111963	967272	11.58

Instrument :
BNA_N
ClientSampleId :
DFTPP