


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102020\
 Data File : BN012374.D
 Acq On : 20 Oct 2020 09:18
 Operator : CG/JU
 Sample : DFTPP75
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP75

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 21 12:12:40 2020

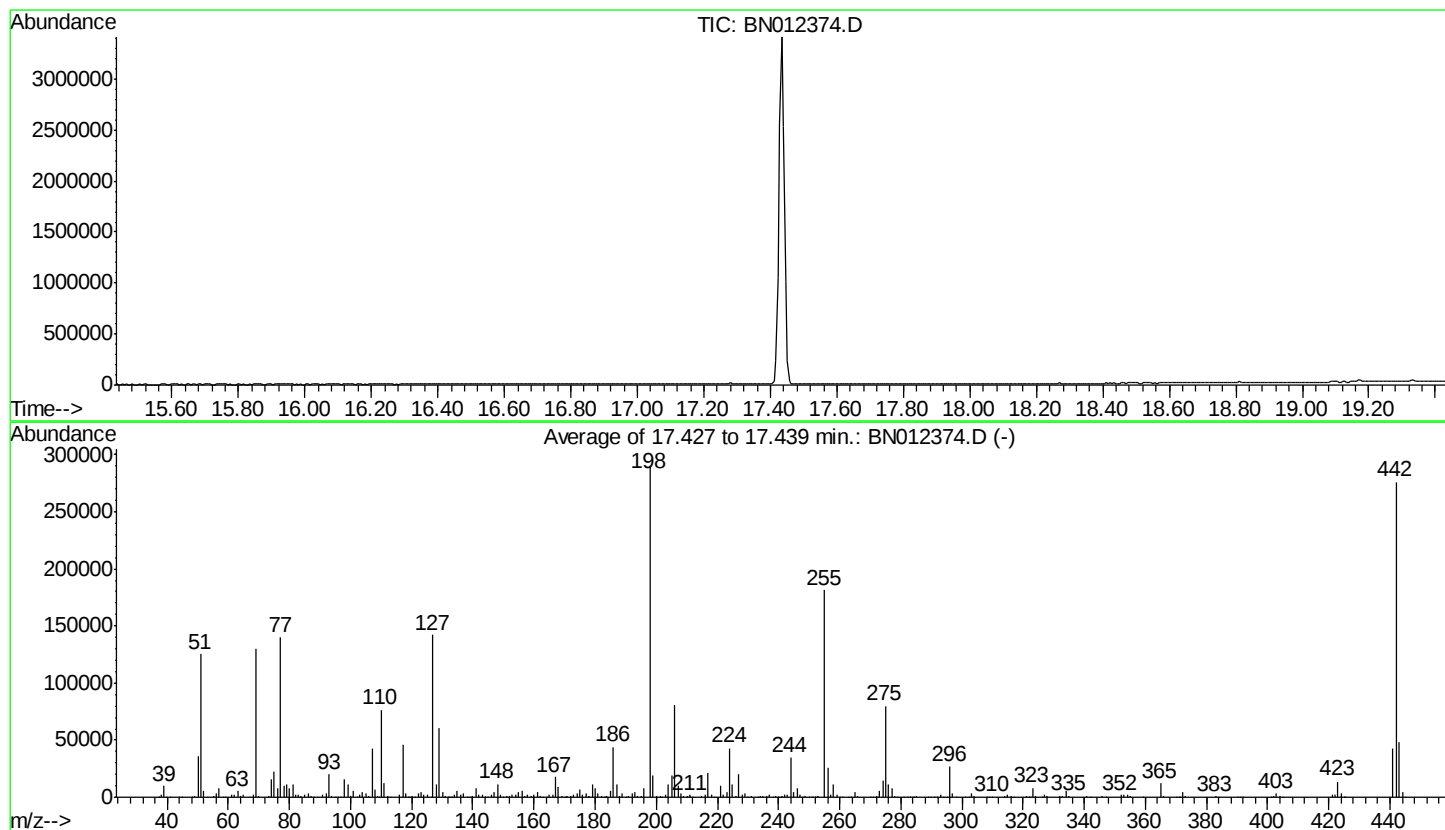

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	125485	PASS
68	69	0.00	2	2.1	2704	PASS
69	198	0.00	100	44.7	129896	PASS
70	69	0.00	2	0.6	831	PASS
127	198	10	80	48.9	142080	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	290432	PASS
199	198	5	9	6.7	19356	PASS
275	198	10	60	27.6	80021	PASS
365	198	1	100	4.1	11968	PASS
441	198	0.01	100	14.6	42485	PASS
442	198	50	100	95.0	275818	PASS
443	442	15	24	17.4	47954	PASS

Scan 2449 (17.392 min): BN012374.D
DFTPP75

m/z	Abundance
39.80	842.0
44.00	1567.0
48.90	526.0
73.10	865.0
96.10	539.0
133.00	320.0
146.90	375.0
193.10	336.0
207.00	2760.0
208.00	772.0
209.00	488.0
221.10	357.0
281.10	734.0

Instrument :

BNA_N

ClientSampleId :

DFTPP75

m/z	Abundance
37.00	891.0
38.00	1771.0
39.00	9811.0
40.00	1200.0
43.90	1889.0
45.00	437.0
48.90	1373.0
50.00	39808.0
51.00	127664.0
52.00	6826.0
55.00	1092.0
56.00	3321.0
57.00	8234.0
58.10	389.0
61.10	1872.0
62.00	2615.0
63.00	5813.0
64.10	893.0
65.00	2751.0
68.10	2837.0
69.00	132672.0
70.00	923.0
73.10	2604.0
74.00	16192.0
75.00	23688.0
76.00	6960.0
77.00	138048.0
78.10	12032.0
79.00	12388.0
80.00	8002.0
81.00	11122.0
82.00	2506.0
83.00	2043.0
83.90	706.0
85.00	2163.0
86.00	2914.0
87.00	1644.0
88.00	497.0
89.00	334.0
90.90	2178.0
92.00	3057.0
93.00	20312.0
93.90	1263.0
95.90	855.0
98.00	16784.0
99.00	11888.0
99.90	918.0
101.00	5257.0
103.00	2324.0
104.00	4181.0
105.00	3896.0
106.00	1406.0
107.00	40336.0
108.00	6909.0
108.90	1720.0
110.00	78712.0
111.00	12504.0
111.90	1263.0
113.00	525.0
116.00	3069.0
117.00	47856.0
118.00	3685.0
118.90	504.0
119.90	529.0
120.90	314.0
122.00	3118.0
122.90	5043.0
123.90	2003.0
125.00	2127.0
127.00	137536.0
128.00	11390.0
129.00	59336.0
130.00	5474.0
131.00	1138.0
131.90	608.0
132.80	518.0
134.00	2181.0
135.00	4535.0
136.00	2304.0
137.00	2968.0
138.00	516.0
138.90	436.0
139.90	1014.0
141.00	7004.0
142.00	3072.0
143.00	1646.0
143.90	554.0
145.00	482.0
146.00	2013.0
147.00	5000.0
148.00	10509.0
149.10	2101.0

Instrument :
BNA_N
ClientSampleId :
DFTPP75

150.00	516.0
151.00	1270.0
152.00	652.0
153.00	2980.0
154.00	2087.0
155.00	4361.0
156.00	4691.0
157.10	1475.0
158.00	1225.0
158.90	1072.0
160.00	2389.0
160.90	3371.0
162.00	769.0
163.00	618.0
164.00	316.0
165.00	2598.0
166.00	2271.0
167.00	16424.0
168.00	10605.0
169.10	1453.0
170.00	681.0
170.90	674.0
172.00	1898.0
172.90	1283.0
174.00	3883.0
175.10	5104.0
175.90	1470.0
176.90	2812.0
177.90	1174.0
178.90	9586.0
180.00	7750.0
180.90	3663.0
182.00	768.0
183.30	355.0
183.90	1032.0
185.00	5942.0
186.00	37328.0
187.00	10719.0
188.00	1100.0
189.00	2925.0
189.90	654.0
191.00	1428.0
191.90	3284.0
193.00	4604.0
194.00	926.0
195.10	645.0
196.00	6979.0
198.00	263680.0
199.00	17752.0
200.00	1373.0
201.30	1102.0
202.90	2011.0
204.00	10510.0
205.00	17176.0
206.10	69880.0
207.10	13088.0
208.10	2905.0
209.00	1165.0
210.10	1186.0
210.90	2998.0
214.90	529.0
216.10	2213.0
217.00	19664.0
218.00	1509.0
218.80	376.0
221.10	7558.0
222.00	2232.0
223.00	3599.0
224.10	39992.0
225.00	9260.0
225.90	1131.0
227.00	17904.0
228.00	2454.0
229.00	3317.0
230.00	639.0
231.00	1182.0
233.90	1205.0
234.90	958.0
236.10	807.0
236.90	2555.0
238.90	709.0
239.80	535.0
240.80	820.0
242.00	2387.0
243.00	2569.0
244.00	29848.0
245.00	4406.0
246.00	6206.0
247.00	1408.0
248.80	1539.0
251.90	329.0
252.90	806.0
255.00	160064.0
256.00	21448.0
257.00	2331.0
258.00	9976.0

Instrument :
BNA_N
ClientSampleId :
DFTPP75

259.10	1522.0
259.90	443.0
263.90	307.0
265.00	3931.0
265.90	501.0
271.00	331.0
272.10	547.0
273.00	4779.0
274.00	11648.0
275.00	63912.0
276.00	9314.0
277.00	7006.0
278.00	1434.0
280.90	702.0
282.00	508.0
282.90	732.0
284.20	451.0
285.00	1050.0
292.90	1382.0
294.00	580.0
296.00	21168.0
296.90	3258.0
302.10	450.0
303.00	2359.0
303.90	514.0
309.00	359.0
314.00	962.0
314.90	1847.0
315.90	1221.0
321.10	773.0
322.00	310.0
323.00	6170.0
324.10	1288.0
327.00	1510.0
327.90	928.0
332.00	467.0
333.00	681.0
334.10	4050.0
335.00	1378.0
340.90	876.0
345.90	1062.0
347.10	481.0
352.00	1677.0
353.00	1258.0
354.00	2694.0
354.90	528.0
364.90	8556.0
366.00	1212.0
370.00	420.0
370.90	494.0
372.00	3269.0
373.00	665.0
383.00	568.0
402.00	1094.0
403.00	2064.0
404.00	1029.0
421.00	899.0
422.00	1494.0
423.00	9718.0
423.90	4735.0
425.00	795.0
441.00	28664.0
442.00	194944.0
443.00	30960.0
444.00	2716.0

Instrument :
BNA_N
ClientSampleId :
DFTPP75

m/z	Abundance
37.00	766.0
38.10	2429.0
39.10	12101.0
39.90	1155.0
41.10	340.0
43.90	1511.0
47.90	426.0
48.90	1877.0
50.00	43000.0
51.00	155200.0
52.00	7299.0
53.00	375.0
55.00	738.0
55.90	4184.0
57.00	9191.0
58.10	530.0
59.00	303.0
60.90	2308.0
62.00	2154.0
63.00	5960.0
63.90	1027.0
65.00	2735.0
66.80	349.0
68.00	3450.0
69.00	158592.0
70.00	962.0
73.10	3059.0
74.00	18384.0
75.00	26664.0
76.10	9237.0
77.10	174464.0
78.00	11534.0
79.00	13169.0
80.00	9261.0
81.00	13003.0
82.00	2966.0
83.00	3294.0
83.80	795.0
85.00	2378.0
86.00	3802.0
87.00	1555.0
88.00	503.0
88.90	530.0
91.00	2820.0
92.00	3679.0
93.00	24840.0
93.90	1642.0
95.90	999.0
98.00	19616.0
99.00	12617.0
100.00	1495.0
100.90	6453.0
102.10	364.0
103.00	2882.0
104.00	4920.0
105.00	4359.0
106.10	1840.0
107.00	53136.0
108.00	8551.0
109.20	1784.0
110.00	89864.0
111.00	15746.0
111.90	1591.0
113.00	931.0
115.90	3409.0
117.00	53520.0
118.00	3271.0
119.10	491.0
120.00	973.0
120.90	387.0
122.00	3789.0
123.00	5226.0
124.00	2518.0
125.00	2614.0
126.20	1687.0
127.00	169984.0
128.00	13215.0
129.00	72688.0
130.00	5863.0
130.90	1561.0
131.90	831.0
133.10	697.0
133.90	2489.0
135.00	6612.0
136.00	2333.0
137.00	2877.0
138.00	593.0
139.90	931.0
141.00	10229.0
141.90	2875.0
143.00	2211.0
144.20	487.0

Instrument :
BNA_N
ClientSampleId :
DFTPP75

144.90	646.0
146.00	2096.0
147.00	5335.0
148.00	13299.0
149.00	2250.0
150.00	594.0
151.00	1450.0
151.80	701.0
152.90	2738.0
153.90	2363.0
155.00	5907.0
156.00	7579.0
156.90	1368.0
157.90	2469.0
159.00	1016.0
160.00	3726.0
161.00	5364.0
162.00	919.0
163.00	496.0
164.00	623.0
165.00	2934.0
166.00	2473.0
167.00	21552.0
168.00	10768.0
169.00	1644.0
170.00	770.0
170.90	933.0
171.90	1270.0
173.00	2443.0
174.00	4595.0
175.00	8208.0
175.90	2452.0
177.00	4482.0
177.90	1918.0
179.00	14410.0
180.00	10340.0
181.00	4526.0
182.10	704.0
182.90	447.0
184.00	1247.0
185.00	6785.0
186.00	56280.0
187.00	14337.0
188.00	2230.0
188.90	3608.0
190.00	621.0
191.00	1965.0
191.90	4359.0
193.00	5733.0
194.00	1066.0
194.90	764.0
196.00	10653.0
198.00	348672.0
199.00	24368.0
200.00	1976.0
201.30	1598.0
203.00	3308.0
204.00	13922.0
205.00	22112.0
206.00	100312.0
207.00	14683.0
208.00	4531.0
209.00	1843.0
210.00	1592.0
211.10	3523.0
211.80	812.0
215.00	1130.0
216.10	2162.0
217.00	26376.0
218.00	3444.0
218.90	360.0
221.00	13745.0
222.00	3118.0
223.00	5523.0
224.00	50816.0
225.00	14320.0
226.00	1815.0
227.00	25112.0
228.00	3221.0
229.00	4919.0
229.80	457.0
231.00	2033.0
233.00	495.0
234.00	1680.0
234.90	1830.0
235.90	1328.0
237.00	2968.0
238.00	394.0
238.90	915.0
240.00	1198.0
241.00	2001.0
242.00	2773.0
243.00	2762.0
244.00	41024.0
245.00	5729.0
246.00	8919.0

Instrument :
BNA_N
ClientSampleId :
DFTPP75

247.00	2358.0
248.90	1419.0
250.80	404.0
252.10	484.0
253.00	1637.0
255.00	218368.0
256.00	31424.0
256.90	2813.0
258.00	14130.0
259.00	2883.0
262.90	327.0
263.90	466.0
265.00	6803.0
266.00	712.0
269.90	433.0
270.90	441.0
272.10	803.0
273.00	6294.0
274.00	17440.0
275.00	103528.0
276.00	14177.0
277.00	8957.0
278.00	2251.0
278.90	541.0
281.00	1124.0
282.00	373.0
283.10	1102.0
283.80	840.0
284.80	1249.0
288.90	307.0
289.80	362.0
291.00	357.0
291.90	621.0
293.00	2551.0
293.80	404.0
295.10	1067.0
296.00	32816.0
296.90	4379.0
298.00	313.0
301.00	310.0
302.00	600.0
303.10	3046.0
304.00	1116.0
308.00	313.0
308.80	360.0
310.00	348.0
314.00	1558.0
314.90	3116.0
315.90	2120.0
317.10	513.0
321.00	865.0
322.20	592.0
323.00	10177.0
324.00	1384.0
326.90	1574.0
328.00	897.0
331.90	578.0
333.00	819.0
334.00	5831.0
335.00	1738.0
341.00	1041.0
341.90	444.0
346.00	1813.0
346.90	552.0
352.00	2516.0
353.00	2573.0
354.00	3032.0
355.00	966.0
359.10	389.0
365.00	15010.0
366.00	1312.0
371.20	889.0
372.00	5748.0
373.00	1109.0
383.00	1521.0
384.00	656.0
390.00	799.0
391.00	477.0
392.00	396.0
402.00	2222.0
402.90	3911.0
404.00	1372.0
404.90	372.0
421.00	2021.0
421.90	2746.0
423.00	15663.0
424.10	5054.0
425.20	730.0
441.00	50944.0
442.00	304576.0
443.00	60304.0
444.00	4725.0
444.90	502.0

Instrument :
BNA_N
ClientSampleId :
DFTPP75

m/z	Abundance
37.20	441.0
38.00	1737.0
39.00	7405.0
40.00	935.0
44.00	2069.0
44.90	500.0
48.90	1527.0
50.00	25936.0
51.00	93592.0
52.10	3912.0
53.00	351.0
55.10	703.0
55.90	2594.0
57.00	6263.0
61.10	1055.0
62.10	1549.0
63.10	4271.0
64.10	740.0
65.00	2228.0
66.90	320.0
68.10	1825.0
69.00	98424.0
70.00	609.0
73.00	1826.0
74.00	11811.0
75.00	15654.0
76.00	6047.0
77.00	106968.0
78.00	6369.0
79.00	8337.0
80.00	6258.0
81.00	8838.0
82.00	2239.0
82.90	2418.0
83.90	575.0
85.00	1712.0
86.00	2577.0
87.10	1299.0
87.90	313.0
89.00	431.0
91.00	2114.0
92.00	1884.0
93.00	14457.0
93.80	658.0
95.10	397.0
96.00	677.0
96.80	436.0
98.00	11851.0
99.00	8665.0
100.10	790.0
101.00	4442.0
102.00	526.0
103.00	1707.0
103.90	3474.0
105.00	3360.0
105.90	1193.0
107.00	36016.0
108.00	5751.0
109.00	1600.0
110.00	61248.0
111.00	10377.0
112.00	1278.0
116.10	1955.0
117.00	37160.0
118.00	2504.0
118.90	456.0
120.10	502.0
122.00	2777.0
123.00	4748.0
124.00	1718.0
125.00	1419.0
127.00	118720.0
128.00	8950.0
129.00	48616.0
130.00	3847.0
131.00	795.0
132.10	481.0
133.00	379.0
134.00	1725.0
134.90	4636.0
136.00	1504.0
136.90	2793.0
138.00	557.0
139.90	869.0
141.00	5941.0
142.00	2458.0
142.90	1688.0
144.10	337.0
145.90	1359.0
147.00	3789.0
148.00	9974.0
149.00	1723.0

Instrument :
BNA_N
ClientSampleId :
DFTPP75

150.00	562.0
151.10	1010.0
151.80	711.0
152.90	1884.0
154.10	1282.0
155.00	3757.0
156.00	6015.0
157.00	733.0
157.90	1675.0
158.90	783.0
159.90	1578.0
161.00	3618.0
161.80	883.0
163.90	329.0
164.90	2929.0
166.10	2568.0
167.00	15583.0
168.00	7281.0
169.00	1019.0
170.20	492.0
171.00	581.0
171.90	1385.0
172.90	1899.0
174.00	2540.0
175.00	5765.0
175.90	1398.0
177.00	3293.0
178.10	856.0
179.00	10368.0
180.00	6935.0
181.00	2987.0
182.10	448.0
183.00	427.0
184.00	987.0
185.00	5083.0
186.00	38120.0
187.00	9595.0
188.00	1233.0
189.00	2959.0
190.00	494.0
191.00	1454.0
192.00	3534.0
193.00	3793.0
193.90	891.0
195.00	590.0
195.90	5961.0
198.00	258944.0
199.00	15950.0
199.90	1244.0
201.30	1459.0
201.70	982.0
203.00	2338.0
204.00	9425.0
205.00	16880.0
206.00	73240.0
207.00	11551.0
208.00	3680.0
208.90	1180.0
210.30	1604.0
211.00	2103.0
214.80	778.0
216.00	1530.0
217.00	19280.0
217.90	2598.0
221.00	10367.0
223.00	4966.0
224.00	38416.0
225.00	10534.0
226.00	1249.0
227.00	19088.0
228.00	2723.0
229.00	3332.0
229.90	477.0
231.00	1153.0
234.10	1128.0
235.00	1504.0
236.00	858.0
237.00	2295.0
239.00	489.0
239.90	624.0
241.00	1438.0
242.00	1963.0
243.00	2748.0
244.00	32640.0
245.00	4022.0
246.00	7303.0
246.90	1444.0
247.90	521.0
248.90	1053.0
249.90	323.0
251.00	486.0
253.00	967.0
255.00	165824.0
256.00	23880.0
256.90	1830.0
257.90	10880.0

Instrument :
BNA_N
ClientSampleId :
DFTPP75

259.00	1593.0
260.80	433.0
264.90	3703.0
265.90	722.0
270.00	393.0
272.00	482.0
273.00	5054.0
274.00	15192.0
275.00	72624.0
276.00	11156.0
277.00	7439.0
278.00	1454.0
279.00	431.0
281.00	906.0
282.10	674.0
282.90	924.0
284.10	402.0
285.00	1264.0
289.00	431.0
292.00	322.0
293.00	2326.0
293.90	535.0
295.10	693.0
296.00	26312.0
297.00	3189.0
297.90	324.0
302.10	413.0
303.00	3594.0
303.90	674.0
310.00	372.0
314.00	989.0
315.00	3306.0
315.90	1759.0
320.90	725.0
323.00	8863.0
324.00	1341.0
326.00	328.0
327.00	2246.0
327.90	590.0
332.00	814.0
333.00	1116.0
334.00	5821.0
334.90	1457.0
341.00	1139.0
341.90	376.0
346.00	1863.0
352.10	2516.0
352.90	1741.0
354.00	2400.0
355.10	688.0
365.00	12339.0
366.00	1940.0
370.90	846.0
372.10	4029.0
373.10	1311.0
383.00	944.0
390.00	463.0
401.00	372.0
401.90	1692.0
402.90	2660.0
404.00	739.0
421.00	2269.0
422.00	2497.0
423.00	16278.0
424.00	4426.0
425.00	698.0
441.00	47848.0
442.00	327936.0
443.00	52600.0
444.00	5672.0
444.90	351.0

Instrument :
BNA_N
ClientSampleId :
DFTPP75