

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
 Data File : BN022198.D
 Acq On : 19 Oct 2022 16:18
 Operator : CG/JU
 Sample : PB148240BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK240

Quant Time: Oct 20 01:06:57 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.953	152	4267	0.400	ng/ul	0.00
4) Naphthalene-d8	10.778	136	13754	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.628	164	8137	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.383	188	17621	0.400	ng/ul	0.00
17) Chrysene-d12	21.585	240	12807	0.400	ng/ul	0.00
23) Perylene-d12	24.049	264	11171	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	34991	6.310	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.378	152	7613	0.366	ng/ul	0.00
18) Fluoranthene-d10	19.416	212	15890	0.370	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.622	166	2416	0.068	ng/ul#	13
20) Pyrene	19.784	202	2132	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.891	252	4050	0.091	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
Data File : BN022198.D
Acq On : 19 Oct 2022 16:18
Operator : CG/JU
Sample : PB148240BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK240

Quant Time: Oct 20 01:06:57 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration




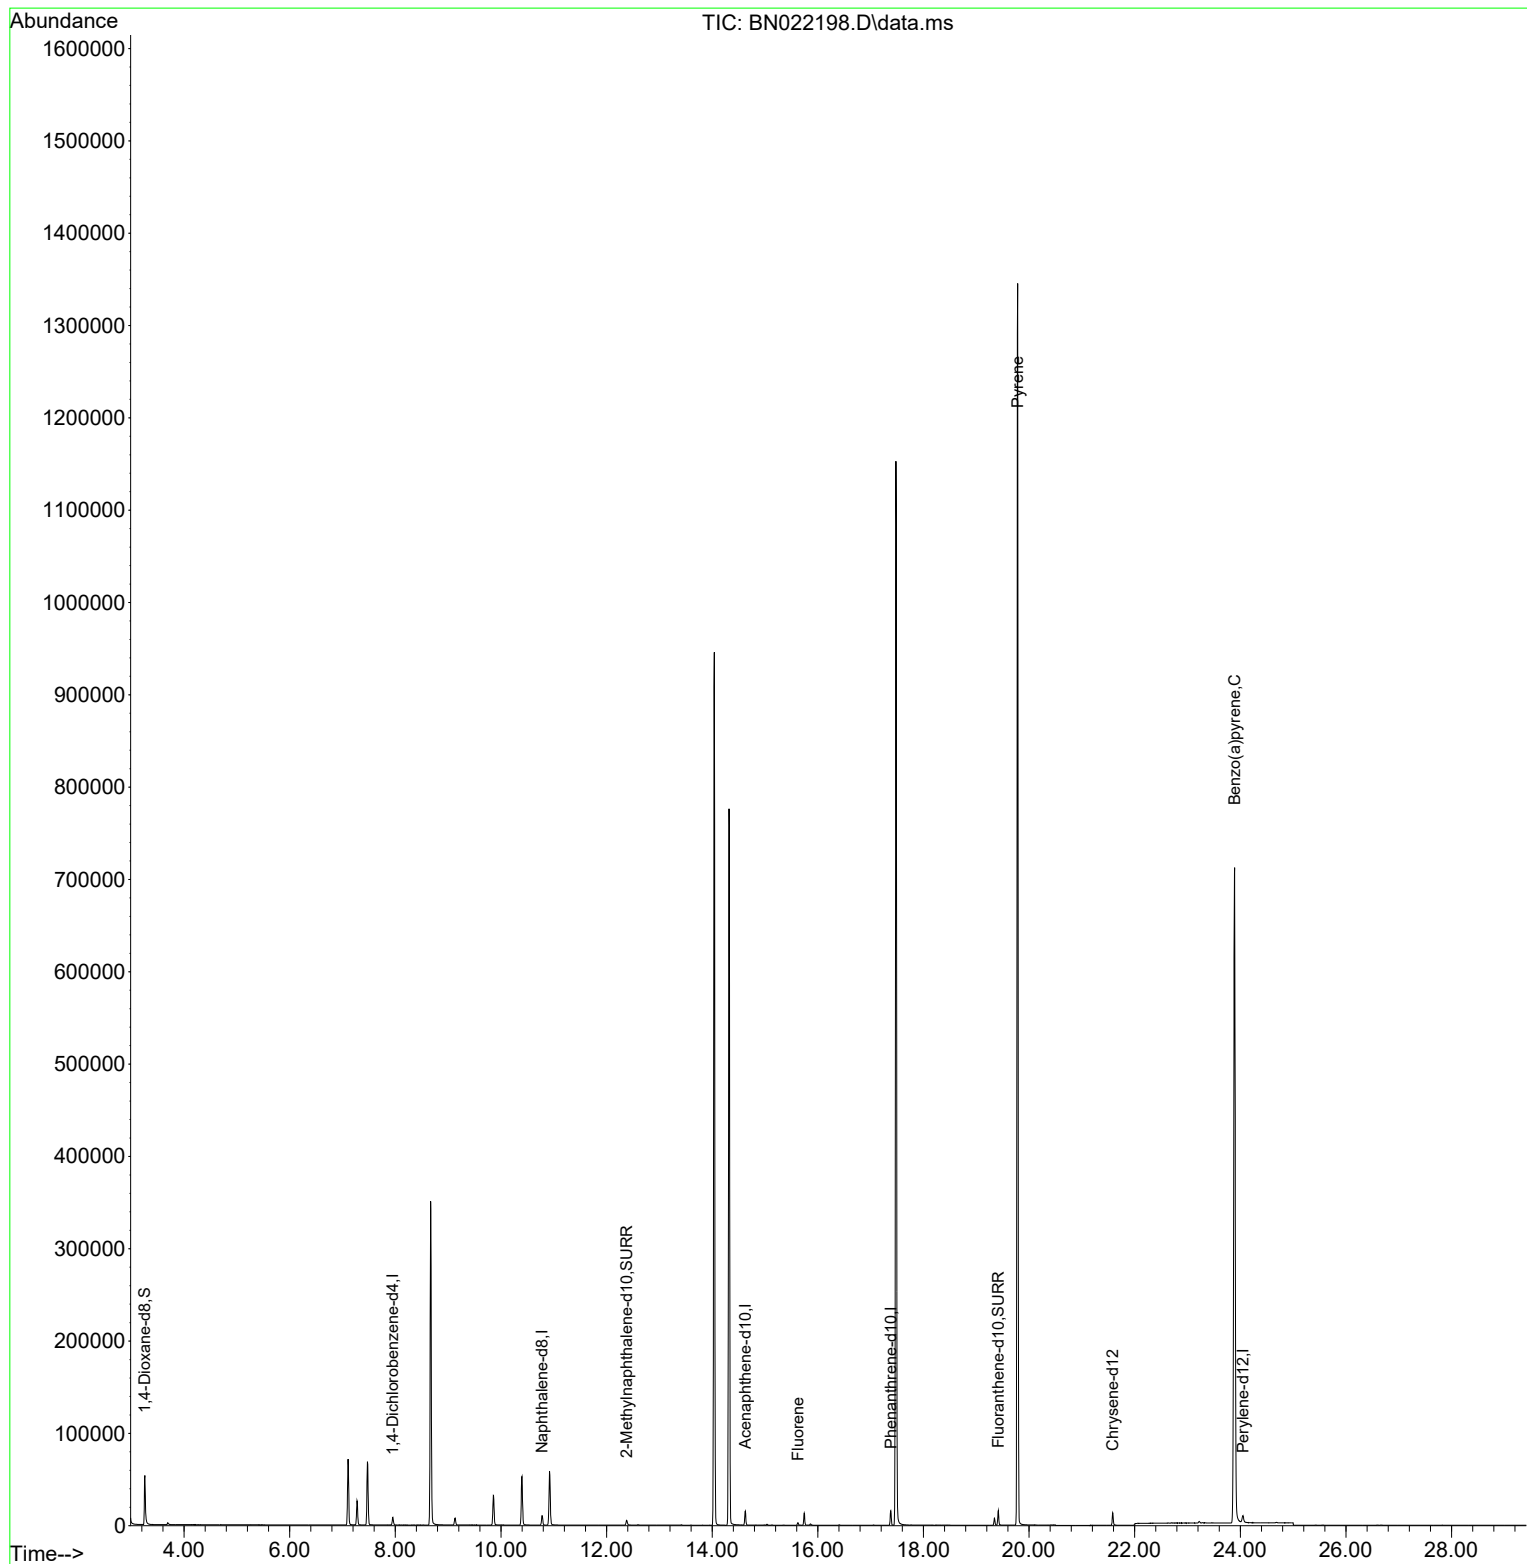


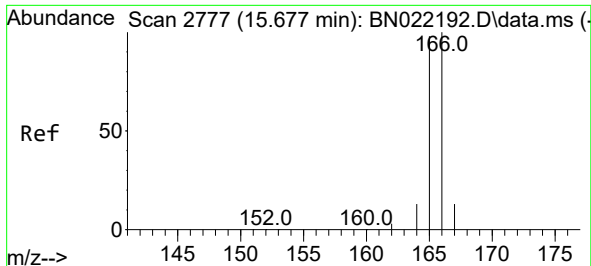

#12
Fluorene
Concen: 0.068 ng/ul
RT: 15.622 min Scan# 21
Delta R.T. -0.054 min
Lab File: BN022198.D
Acq: 19 Oct 2022 16:18




Instrument :
BNA_N
ClientSampleId :
SBLK240


Tgt Ion:166 Resp: 2416
Ion Ratio Lower Upper
166 100
165 7.0 78.2 117.2#
167 33.7 11.0 16.4#

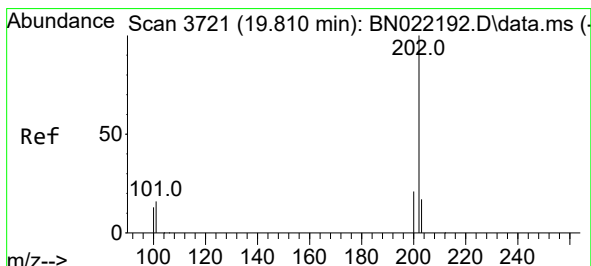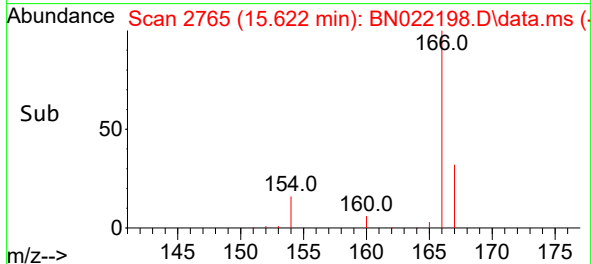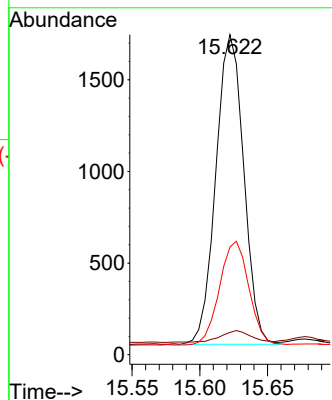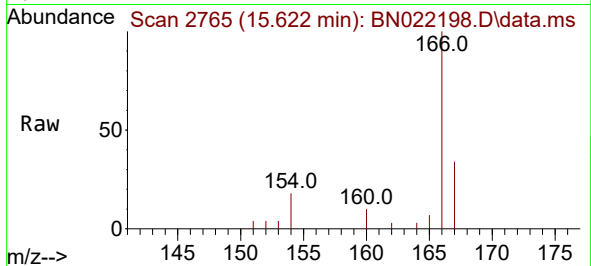

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.784 min Scan# 3715
Delta R.T. -0.027 min
Lab File: BN022198.D
Acq: 19 Oct 2022 16:18


Tgt Ion:202 Resp: 2132
Ion Ratio Lower Upper
202 100
101 176.8 13.1 19.7#
100 1294.1 10.6 16.0#

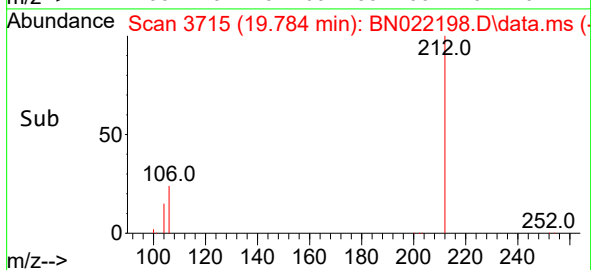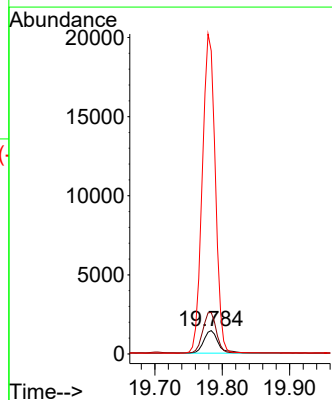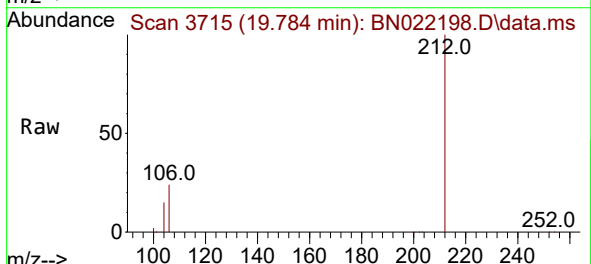

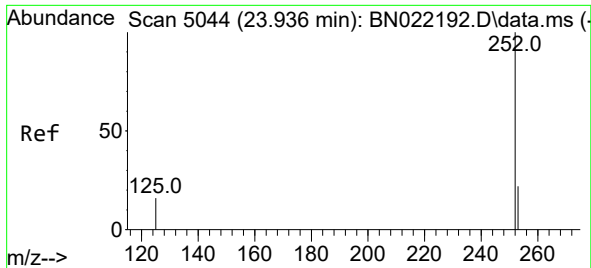

#26
Benzo(a)pyrene
Concen: 0.091 ng/ul
RT: 23.891 min Scan# 50
Delta R.T. -0.045 min
Lab File: BN022198.D
Acq: 19 Oct 2022 16:18

Instrument :
BNA_N
ClientSampleId :
SBLK240

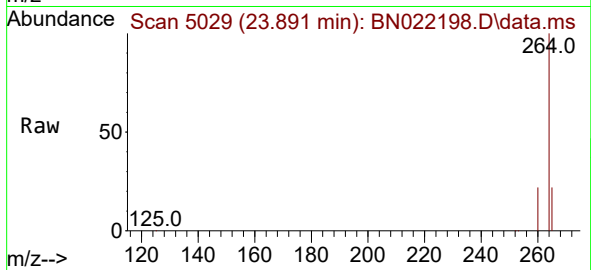

Tgt Ion:252 Resp: 4050
Ion Ratio Lower Upper
252 100
253 42.6 21.0 31.6#
125 44.6 17.9 26.9#

