

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
 Data File : BN022231.D
 Acq On : 20 Oct 2022 13:34
 Operator : CG/JU
 Sample : PB148278BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK278

Quant Time: Oct 21 01:50:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.948	152	5214	0.400	ng/ul	0.00
4) Naphthalene-d8	10.778	136	17215	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.623	164	9813	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.378	188	20264	0.400	ng/ul	0.00
17) Chrysene-d12	21.582	240	12635	0.400	ng/ul	0.00
23) Perylene-d12	24.043	264	9938	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	34851	5.143	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.378	152	7289	0.280	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	14463	0.341	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.779	202	2381	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.882	252	3255	0.082	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
Data File : BN022231.D
Acq On : 20 Oct 2022 13:34
Operator : CG/JU
Sample : PB148278BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK278

Quant Time: Oct 21 01:50:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration




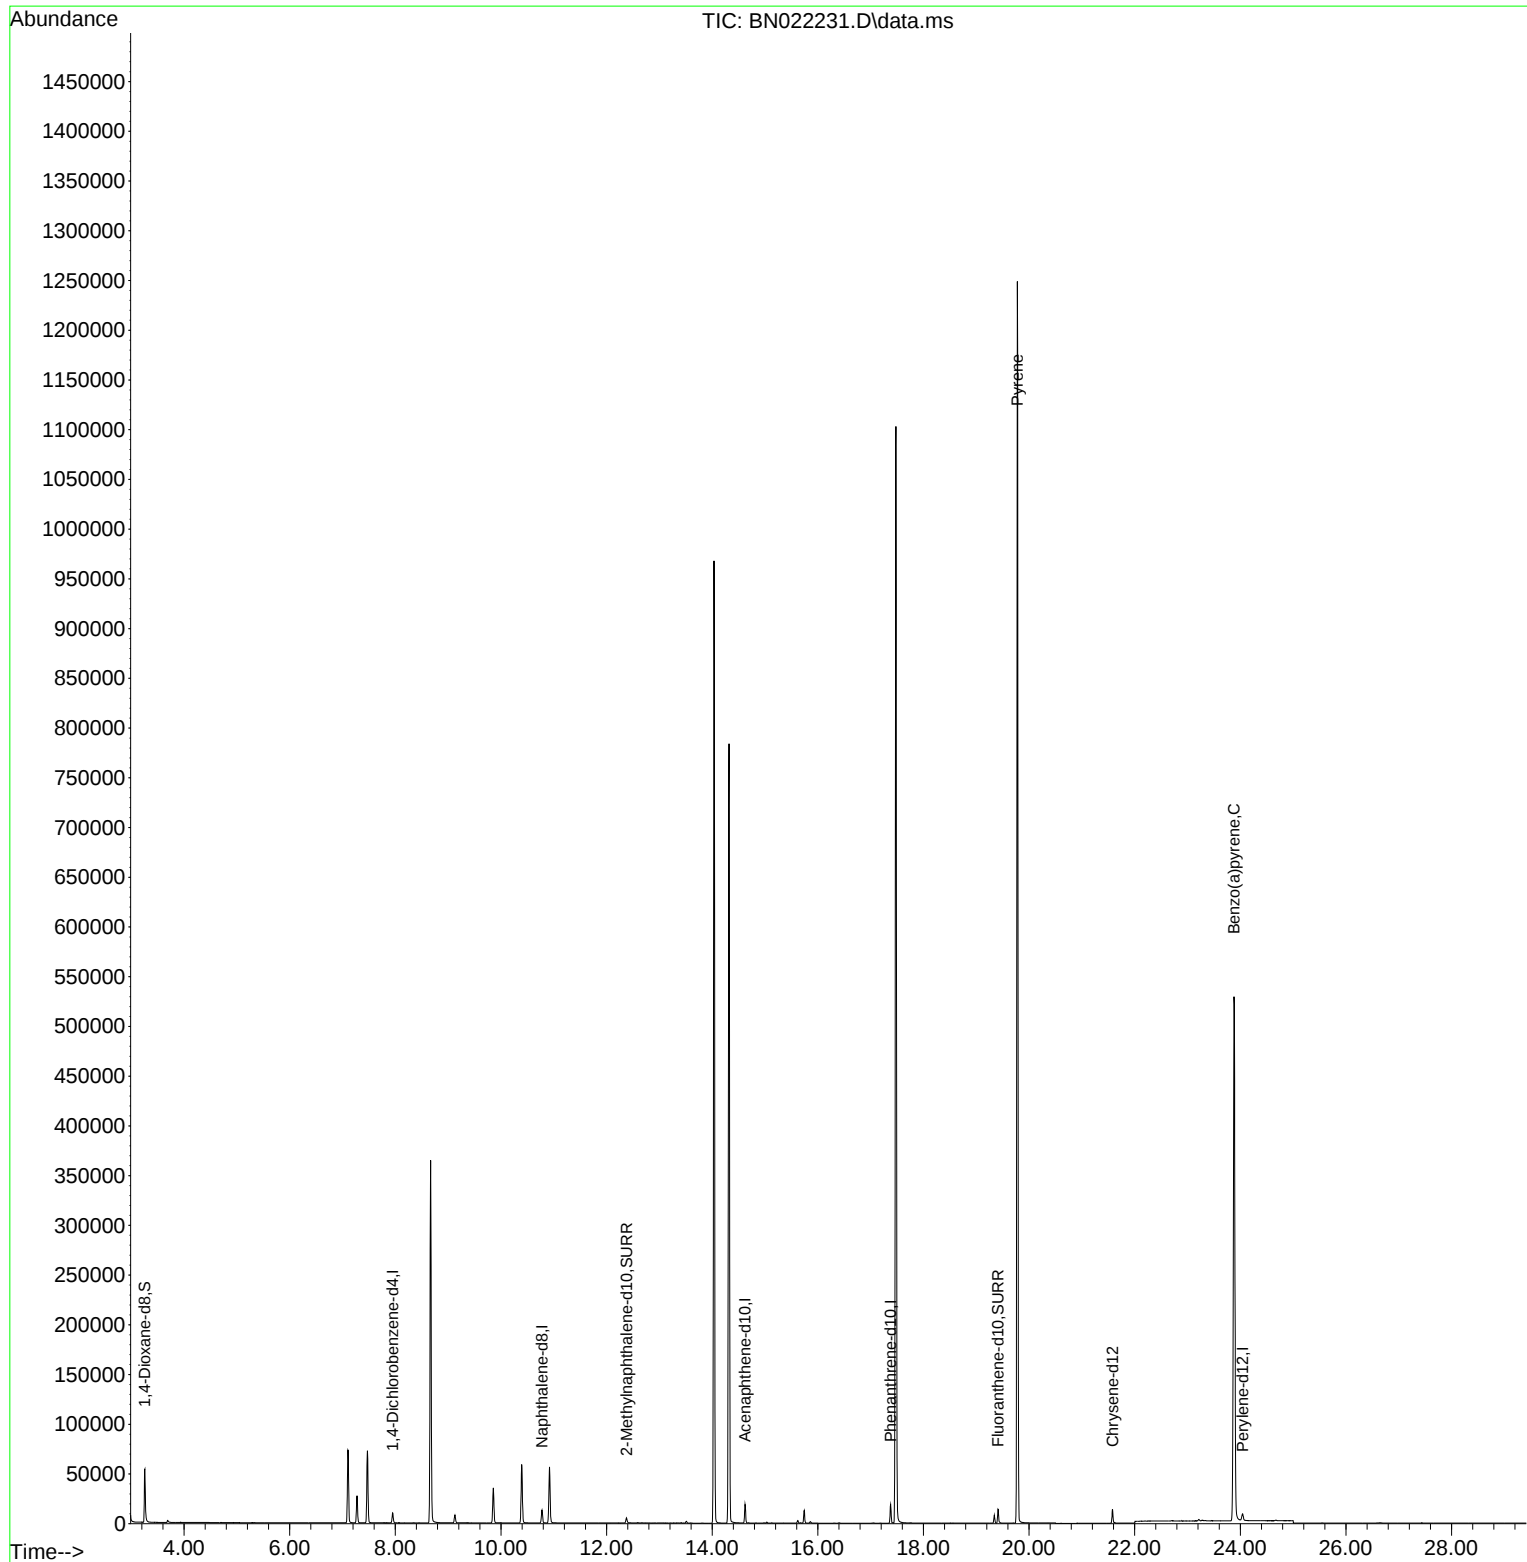


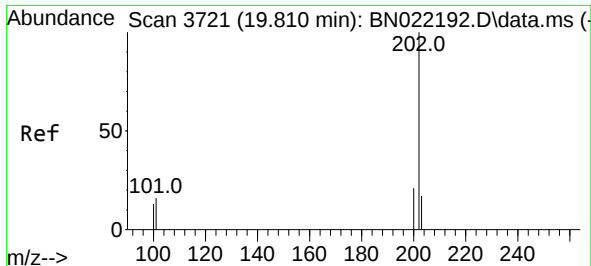

#20
Pyrene
Concen: 0.041 ng/u1
RT: 19.779 min Scan# 31
Delta R.T. -0.031 min
Lab File: BN022231.D
Acq: 20 Oct 2022 13:34

Instrument :
BNA_N
ClientSampleId :
SBLK278

Tgt Ion:202 Resp: 2381
Ion Ratio Lower Upper
202 100
101 181.4 13.1 19.7#
100 1347.7 10.6 16.0#

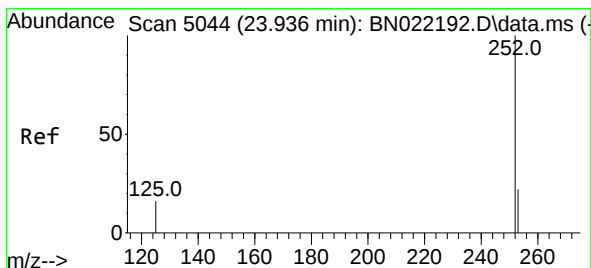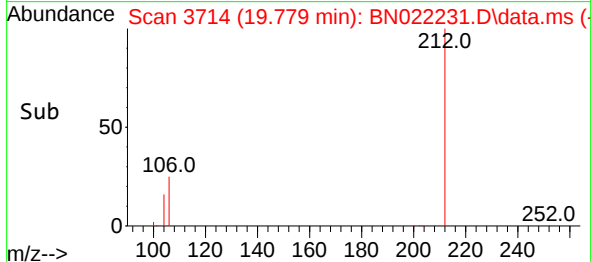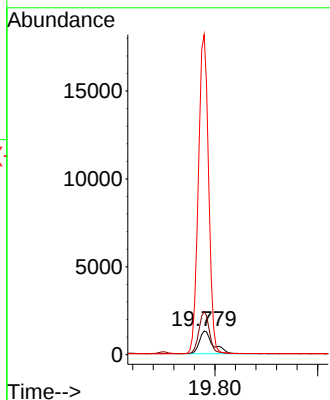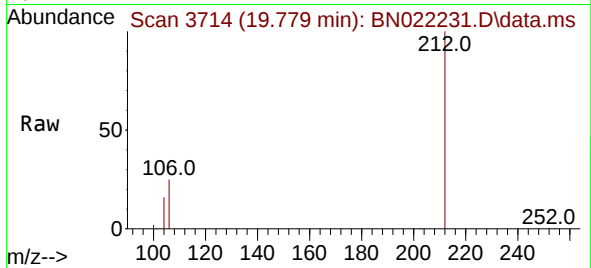

#26
Benzo(a)pyrene
Concen: 0.082 ng/u1
RT: 23.882 min Scan# 5026
Delta R.T. -0.053 min
Lab File: BN022231.D
Acq: 20 Oct 2022 13:34

Tgt Ion:252 Resp: 3255
Ion Ratio Lower Upper
252 100
253 47.2 21.0 31.6#
125 50.1 17.9 26.9#

