




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
Data File : BN022221.D
Acq On : 20 Oct 2022 06:51
Operator : CG/JU
Sample : N5023-17DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC8DL

Manual IntegrationsAPPROVED

Quant Time: Oct 20 07:23:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/20/2022
Supervised By :mohammad ahmed 10/21/2022

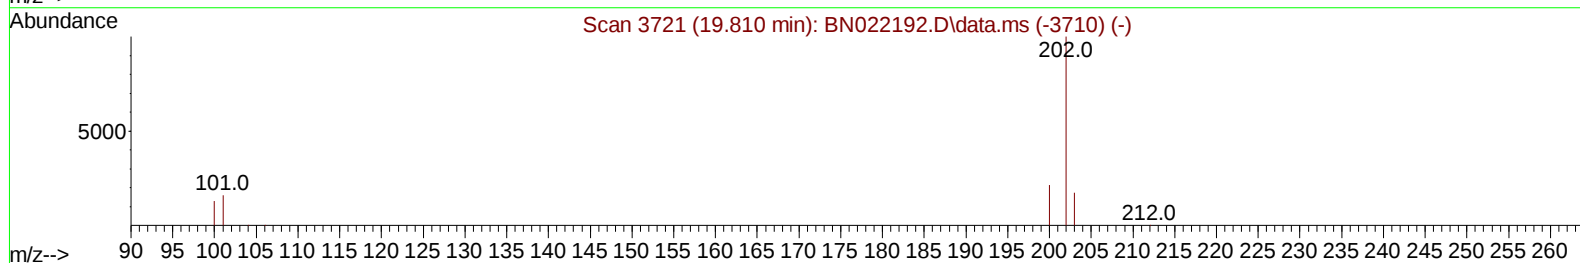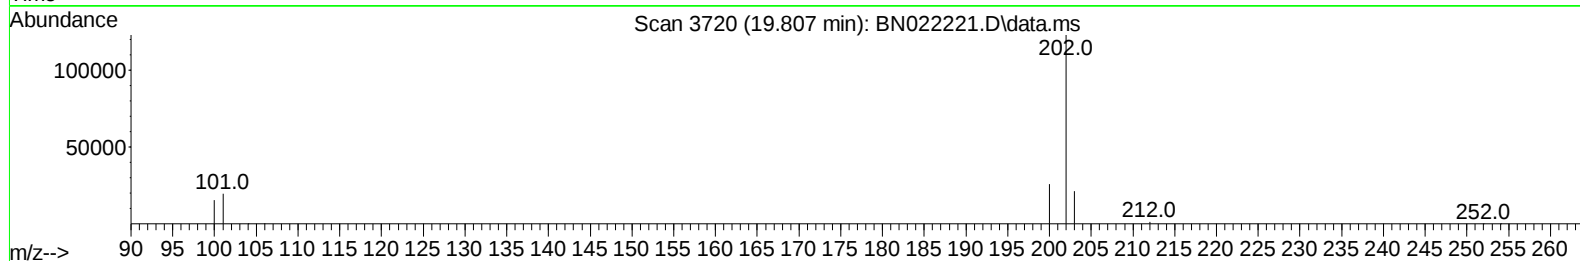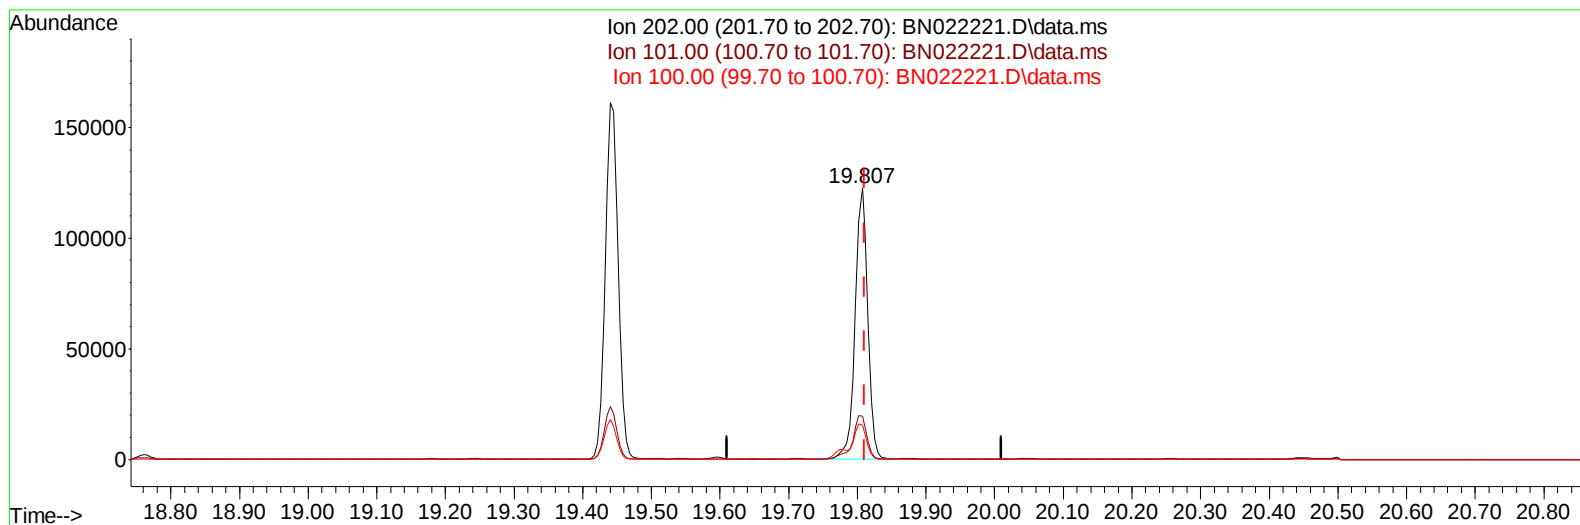

TIC: BN022221.D\data.ms

(20) Pyrene

19.807min (-0.003) 2.13 ng/u1

response 158875

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	16.40	16.02
100.00	13.30	12.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
Data File : BN022221.D
Acq On : 20 Oct 2022 06:51
Operator : CG/JU
Sample : N5023-17DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC8DL

Manual IntegrationsAPPROVED

Quant Time: Oct 20 07:23:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/20/2022
Supervised By :mohammad ahmed 10/21/2022

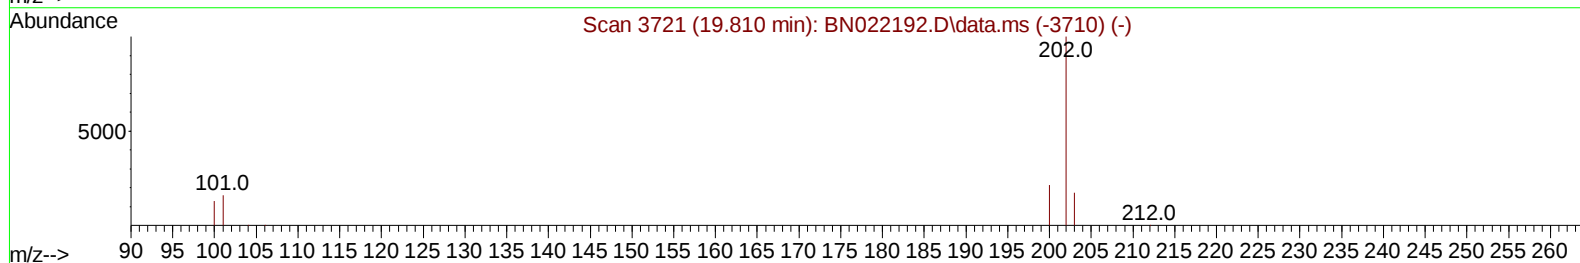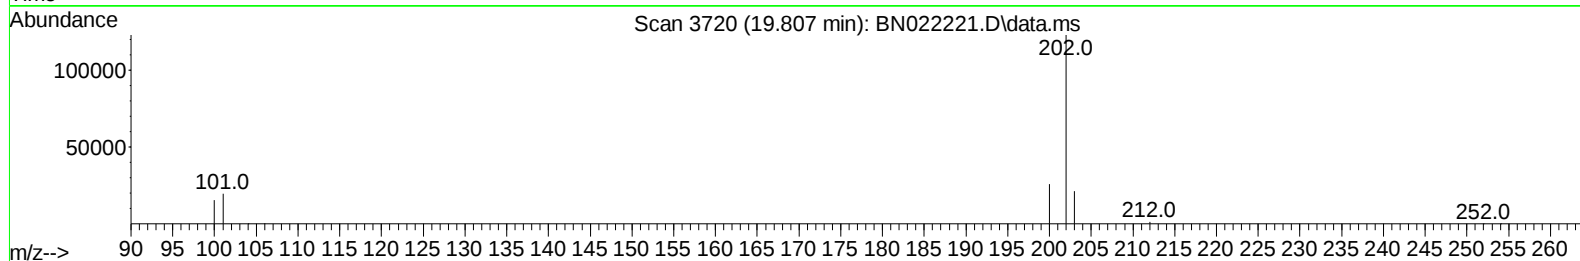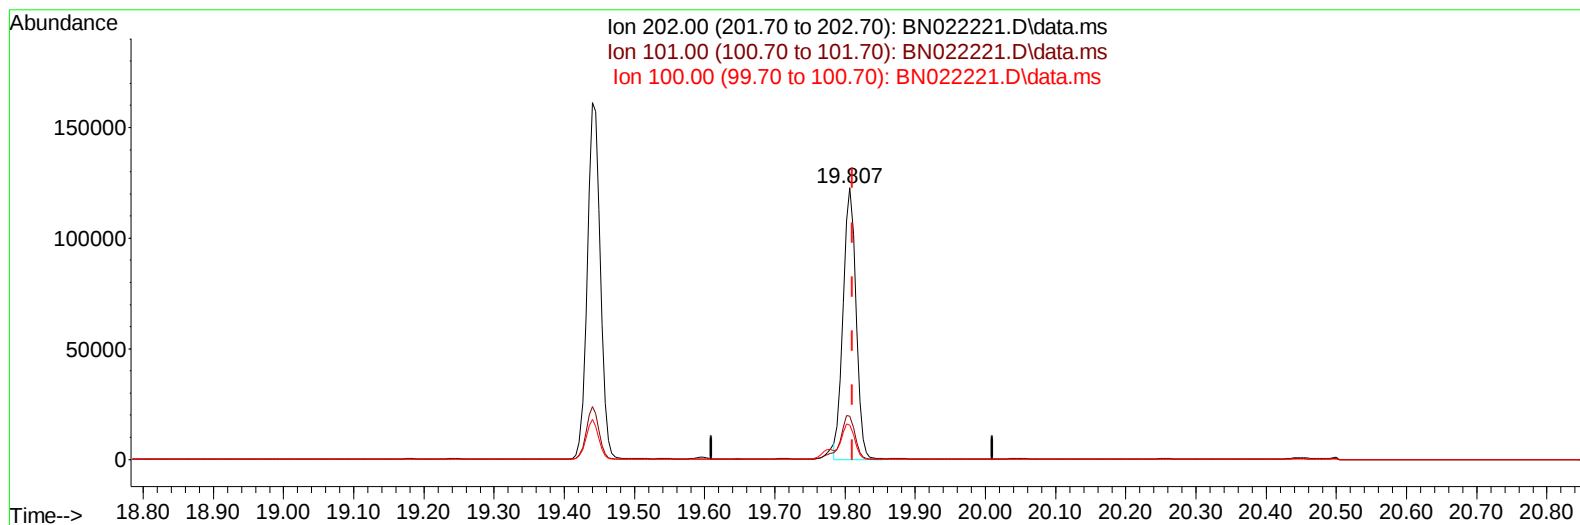

TIC: BN022221.D\data.ms

(20) Pyrene

19.807min (-0.003) 2.07 ng/u1 m

response 154734

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	16.40	16.02
100.00	13.30	12.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
Data File : BN022221.D
Acq On : 20 Oct 2022 06:51
Operator : CG/JU
Sample : N5023-17DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC8DL

Manual IntegrationsAPPROVED

Quant Time: Oct 20 07:23:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/20/2022
Supervised By :mohammad ahmed 10/21/2022

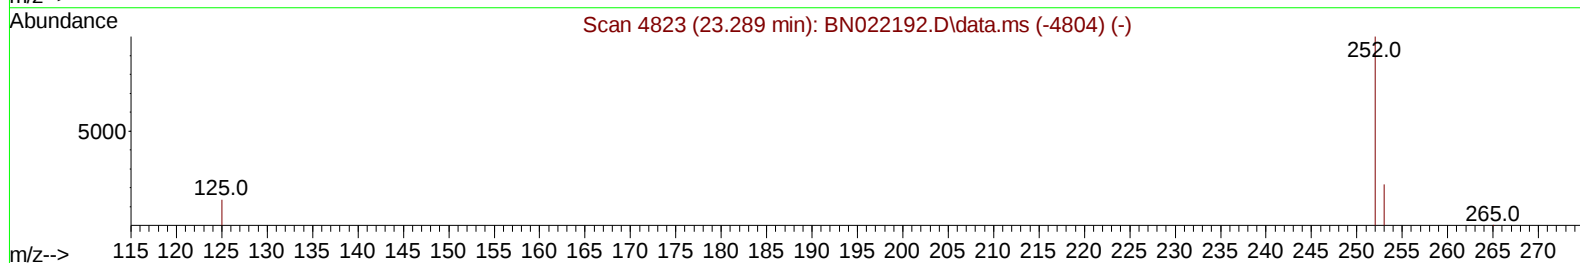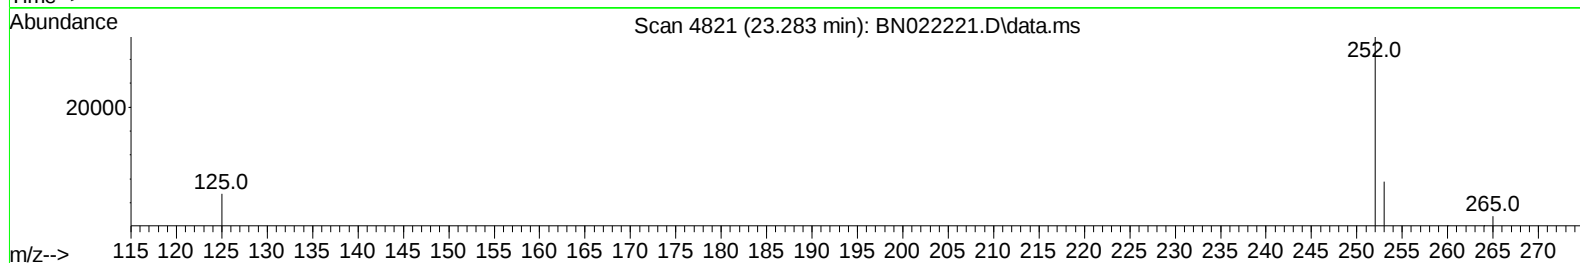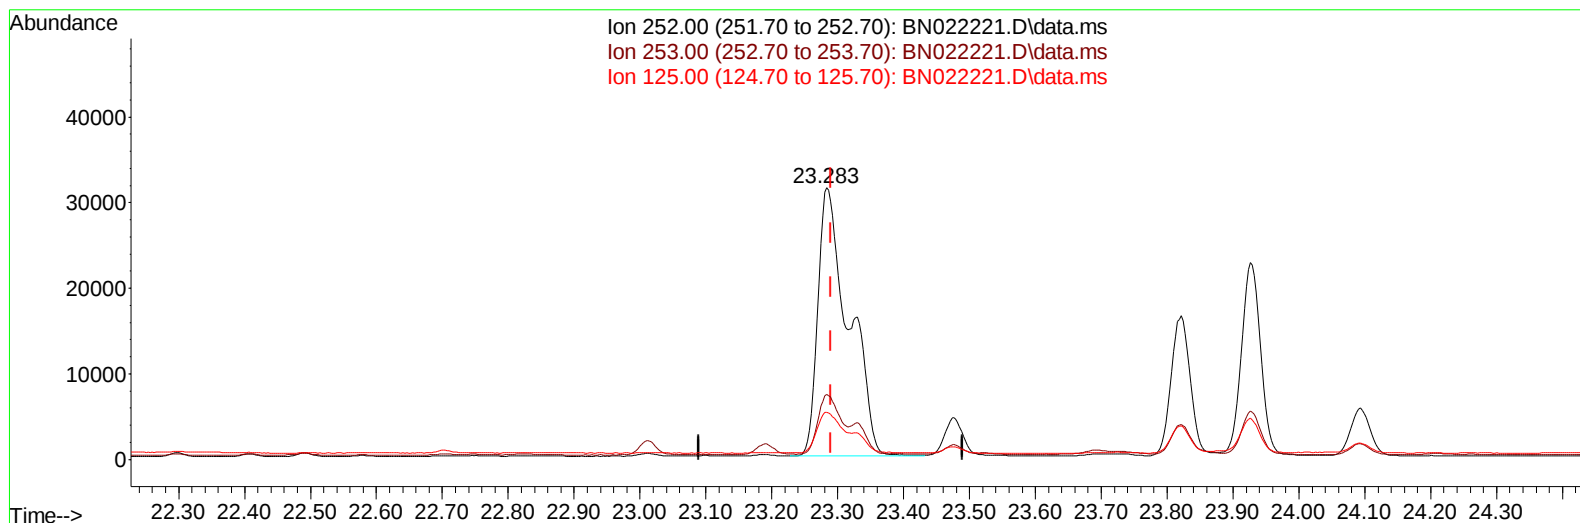

TIC: BN022221.D\data.ms

(24) Benzo(b)fluoranthene

23.283min (-0.006) 1.72 ng/u1

response 102290

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	24.50	23.89
125.00	17.60	17.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
 Data File : BN022221.D
 Acq On : 20 Oct 2022 06:51
 Operator : CG/JU
 Sample : N5023-17DL 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC8DL

Manual IntegrationsAPPROVED

Quant Time: Oct 20 07:23:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/20/2022
 Supervised By :mohammad ahmed 10/21/2022

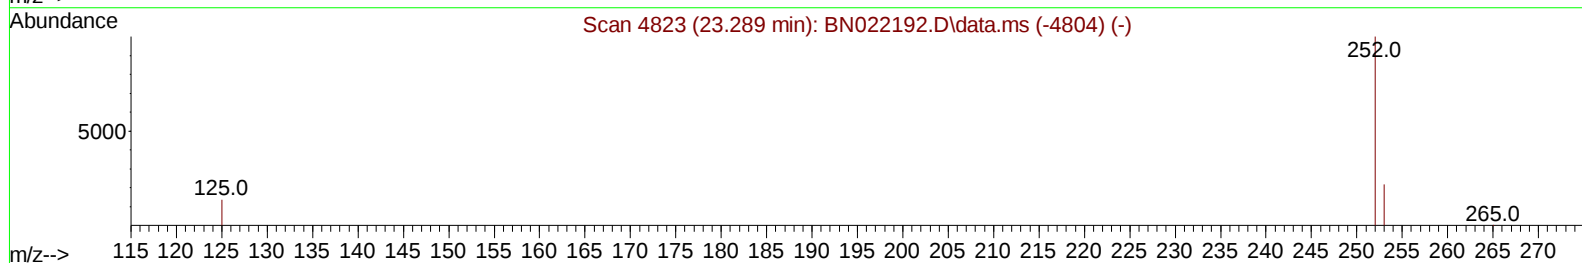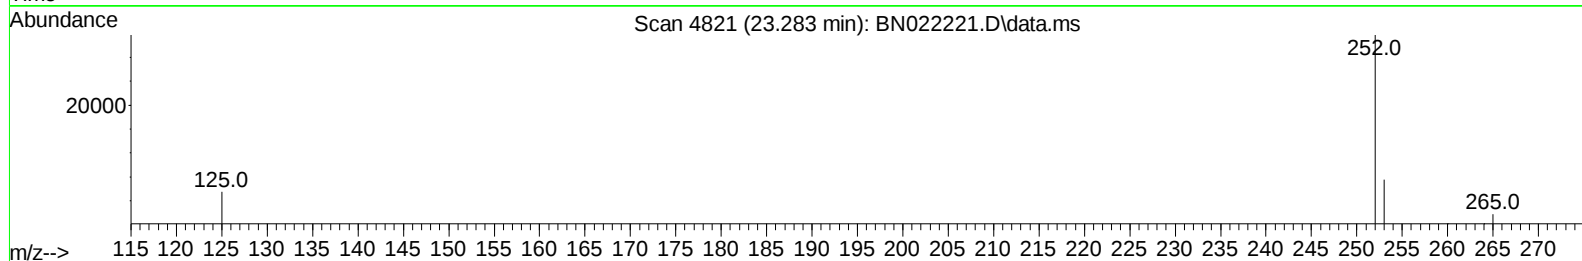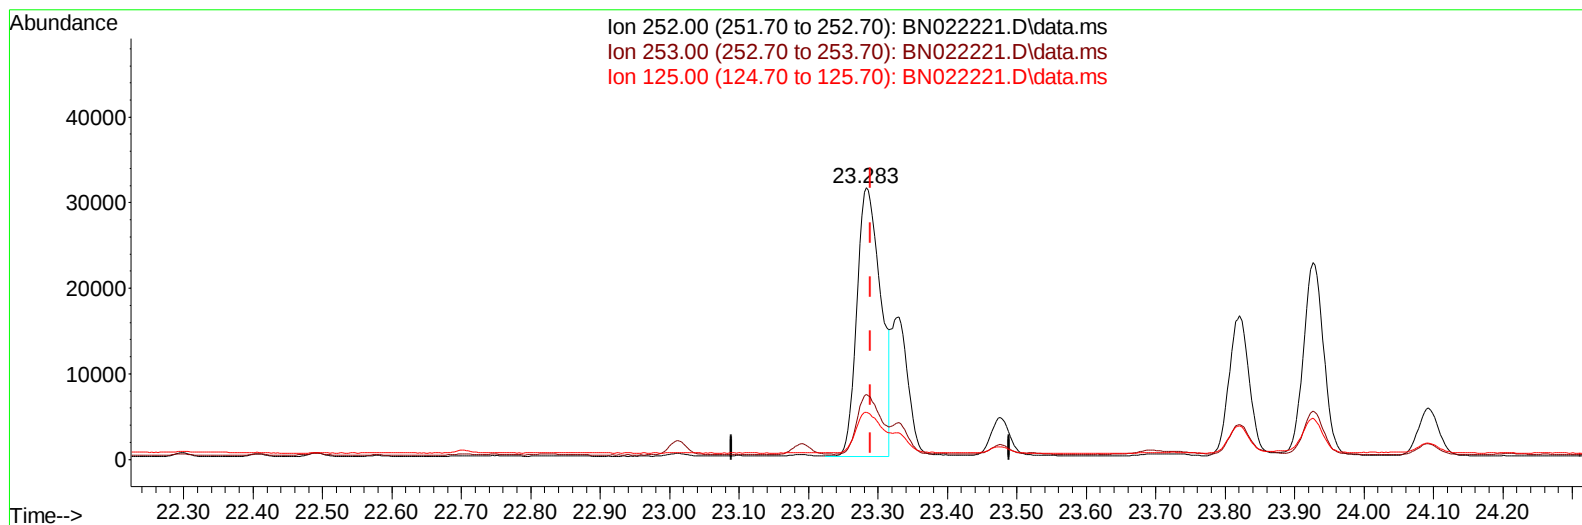

TIC: BN022221.D\data.ms

(24) Benzo(b)fluoranthene

23.283min (-0.006) 1.26 ng/ul m

response 74467

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	24.50	23.89
125.00	17.60	17.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
 Data File : BN022221.D
 Acq On : 20 Oct 2022 06:51
 Operator : CG/JU
 Sample : N5023-17DL 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC8DL

Manual IntegrationsAPPROVED

Quant Time: Oct 20 07:23:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/20/2022
 Supervised By :mohammad ahmed 10/21/2022

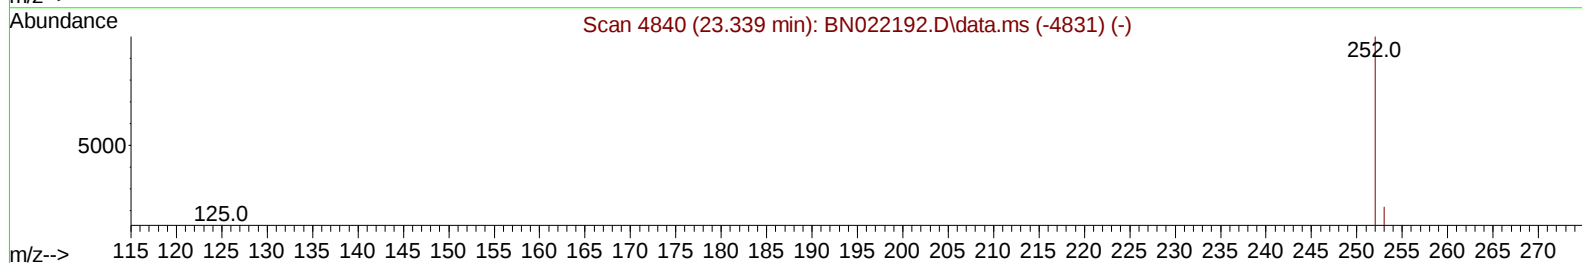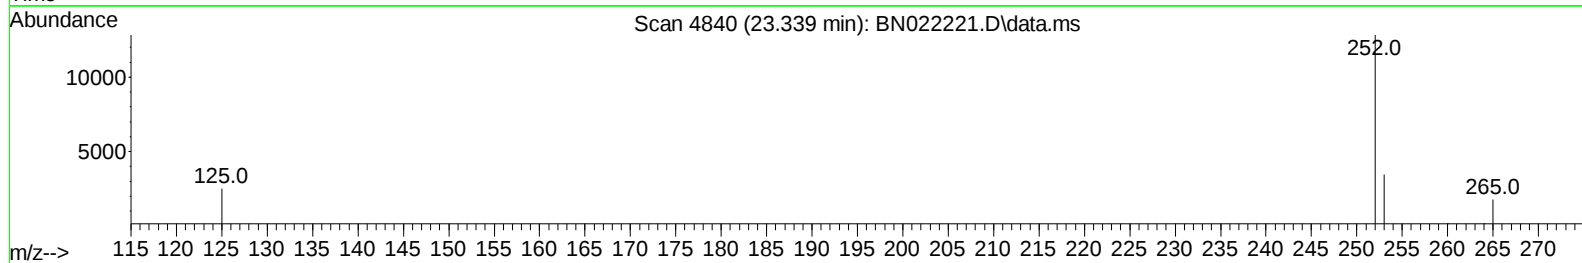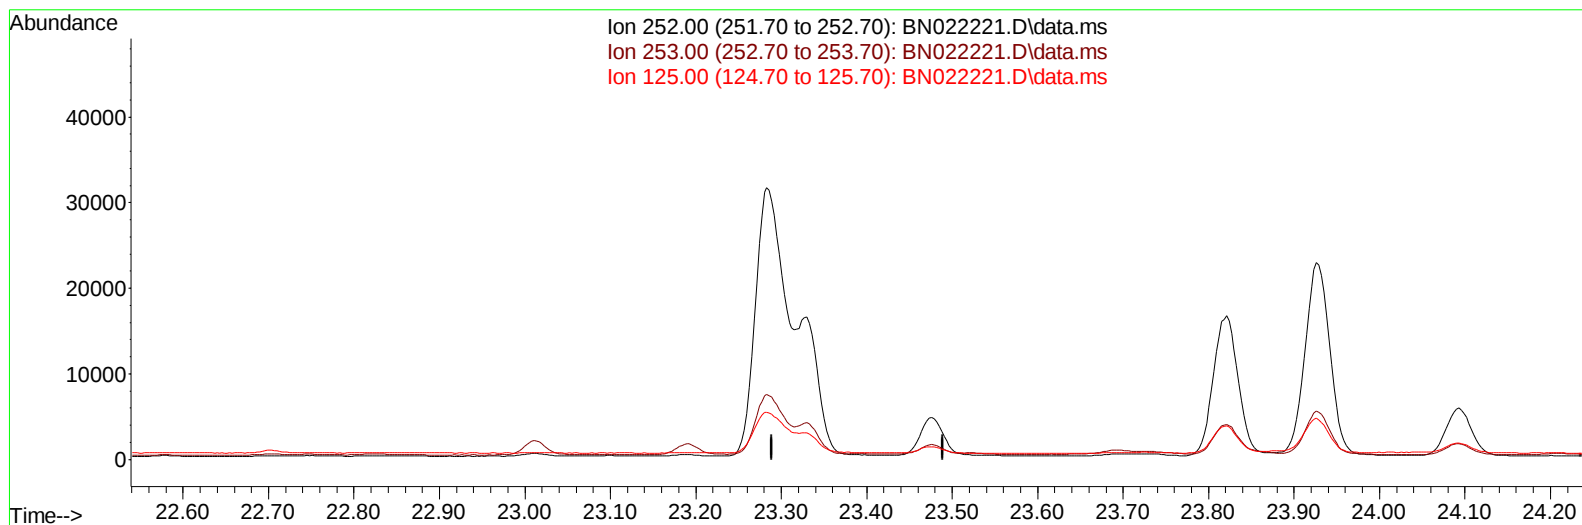

TIC: BN022221.D\data.ms

(25) Benzo(k)fluoranthene

23.339min (-23.339) 0.00 ng/u1

response 0

Ion	Exp%	Act%
252.00	100.00	0.00
253.00	24.60	0.00#
125.00	17.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
 Data File : BN022221.D
 Acq On : 20 Oct 2022 06:51
 Operator : CG/JU
 Sample : N5023-17DL 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC8DL

Manual IntegrationsAPPROVED

Quant Time: Oct 20 07:23:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/20/2022
 Supervised By :mohammad ahmed 10/21/2022

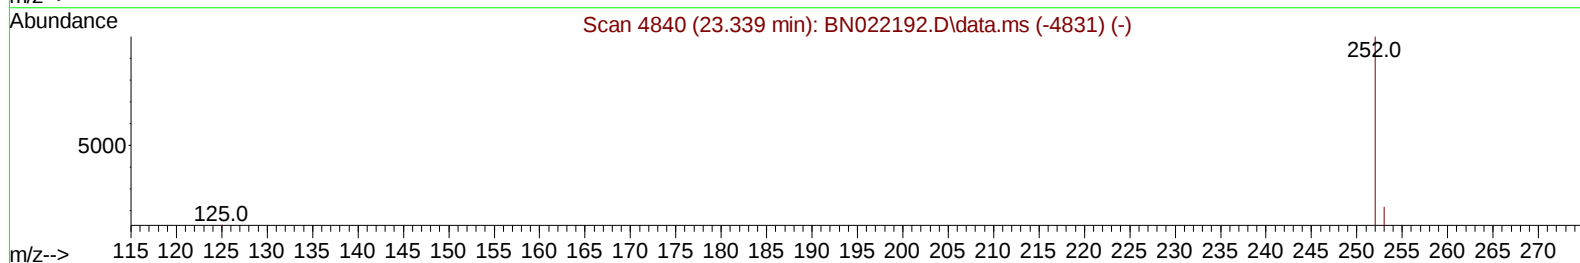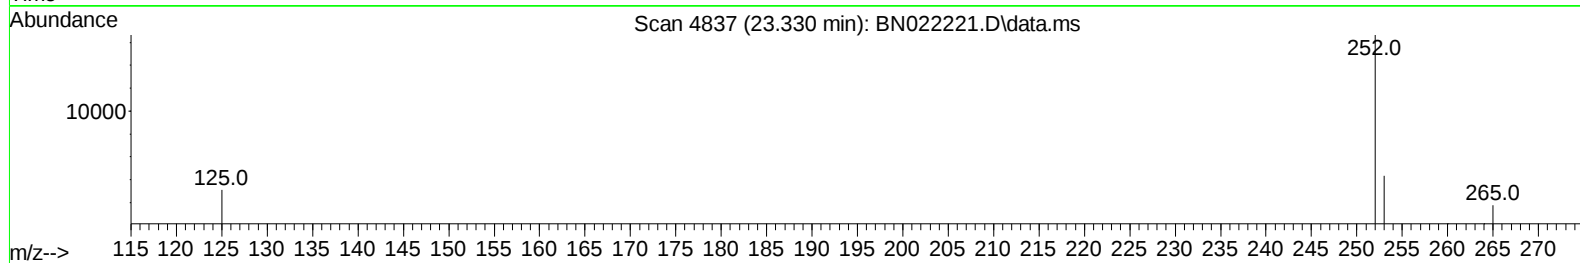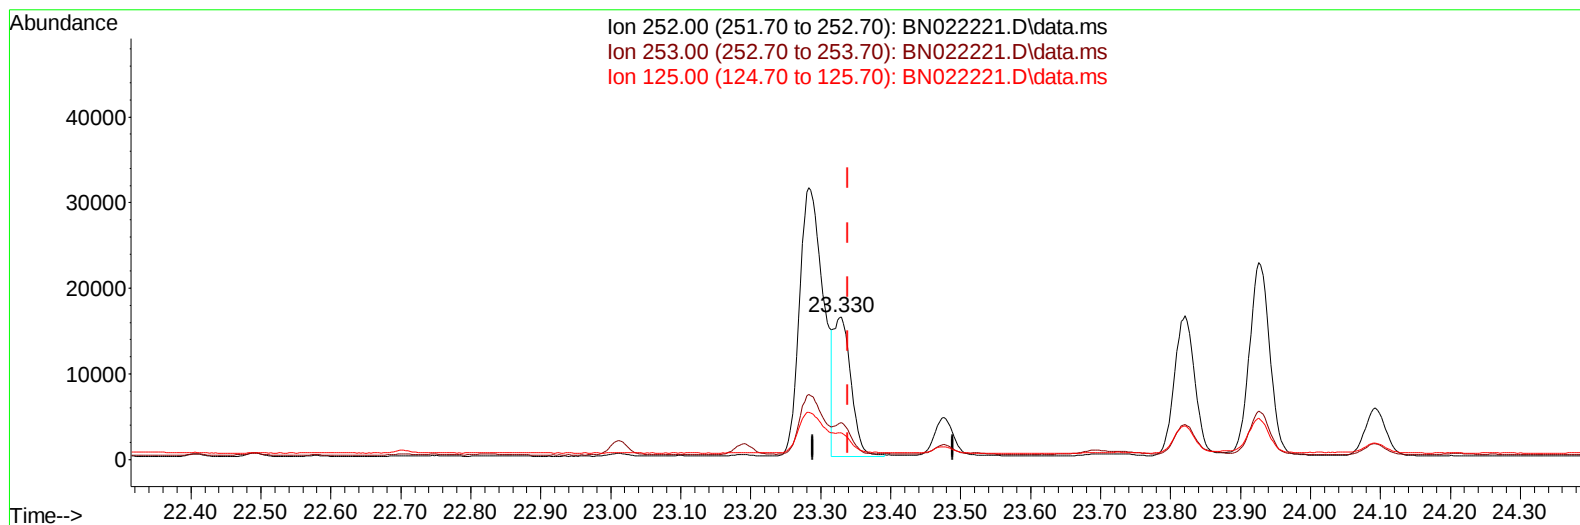

TIC: BN022221.D\data.ms

(25) Benzo(k)fluoranthene

23.330min (-0.009) 0.49 ng/ul m

response 28098

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	24.60	25.95
125.00	17.50	18.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
 Data File : BN022221.D
 Acq On : 20 Oct 2022 06:51
 Operator : CG/JU
 Sample : N5023-17DL 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC8DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/20/2022
 Supervised By :mohammad ahmed 10/21/2022

Quant Time: Oct 20 07:23:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.949	152	5526	0.400	ng/ul	0.00
4) Naphthalene-d8	10.778	136	18746	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.623	164	10605	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.379	188	21793	0.400	ng/ul	0.00
17) Chrysene-d12	21.579	240	16224	0.400	ng/ul	0.00
23) Perylene-d12	24.037	264	11813	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	5161	0.719	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.373	152	1413	0.050	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	3026	0.056	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.827	128	4393	0.079	ng/ul	96
7) 2-Methylnaphthalene	12.450	142	2838	0.081	ng/ul	100
8) 1-Methylnaphthalene	12.664	142	2645	0.074	ng/ul	99
10) Acenaphthylene	14.341	152	2992	0.063	ng/ul#	91
11) Acenaphthene	14.683	153	4034	0.100	ng/ul	99
12) Fluorene	15.673	166	5637	0.121	ng/ul	99
15) Phenanthrene	17.417	178	115015	1.572	ng/ul	99
16) Anthracene	17.509	178	20810	0.338	ng/ul	99
19) Fluoranthene	19.440	202	209823	2.824	ng/ul	100
20) Pyrene	19.807	202	154734m	2.073	ng/ul	
21) Benzo(a)anthracene	21.561	228	64988	1.069	ng/ul	99
22) Chrysene	21.614	228	68549	1.064	ng/ul	97
24) Benzo(b)fluoranthene	23.283	252	74467m	1.255	ng/ul	
25) Benzo(k)fluoranthene	23.330	252	28098m	0.487	ng/ul	
26) Benzo(a)pyrene	23.926	252	45764	0.968	ng/ul	97
27) Indeno(1,2,3-cd)pyrene	26.618	276	30263	0.515	ng/ul	92
28) Dibenzo(a,h)anthracene	26.628	278	7411	0.158	ng/ul#	81
29) Benzo(g,h,i)perylene	27.417	276	24581	0.513	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
Data File : BN022221.D
Acq On : 20 Oct 2022 06:51
Operator : CG/JU
Sample : N5023-17DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC8DL

Manual IntegrationsAPPROVED

Quant Time: Oct 20 07:23:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/20/2022
Supervised By :mohammad ahmed 10/21/2022

