

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
 Data File : BN022211.D
 Acq On : 20 Oct 2022 00:15
 Operator : CG/JU
 Sample : N4982-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BB5

Quant Time: Oct 20 01:08:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.948	152	4006	0.400	ng/ul	0.00
4) Naphthalene-d8	10.778	136	13666	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.623	164	8244	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.378	188	18064	0.400	ng/ul	0.00
17) Chrysene-d12	21.576	240	13176	0.400	ng/ul	0.00
23) Perylene-d12	24.037	264	11281	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.253	96	24544	4.714	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.373	152	7577	0.366	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	18245	0.412	ng/ul	0.00
Target Compounds						
						Qvalue
11) Acenaphthene	14.688	153	831	0.027	ng/ul	95
12) Fluorene	15.673	166	902	0.025	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
Data File : BN022211.D
Acq On : 20 Oct 2022 00:15
Operator : CG/JU
Sample : N4982-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BB5

Quant Time: Oct 20 01:08:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration




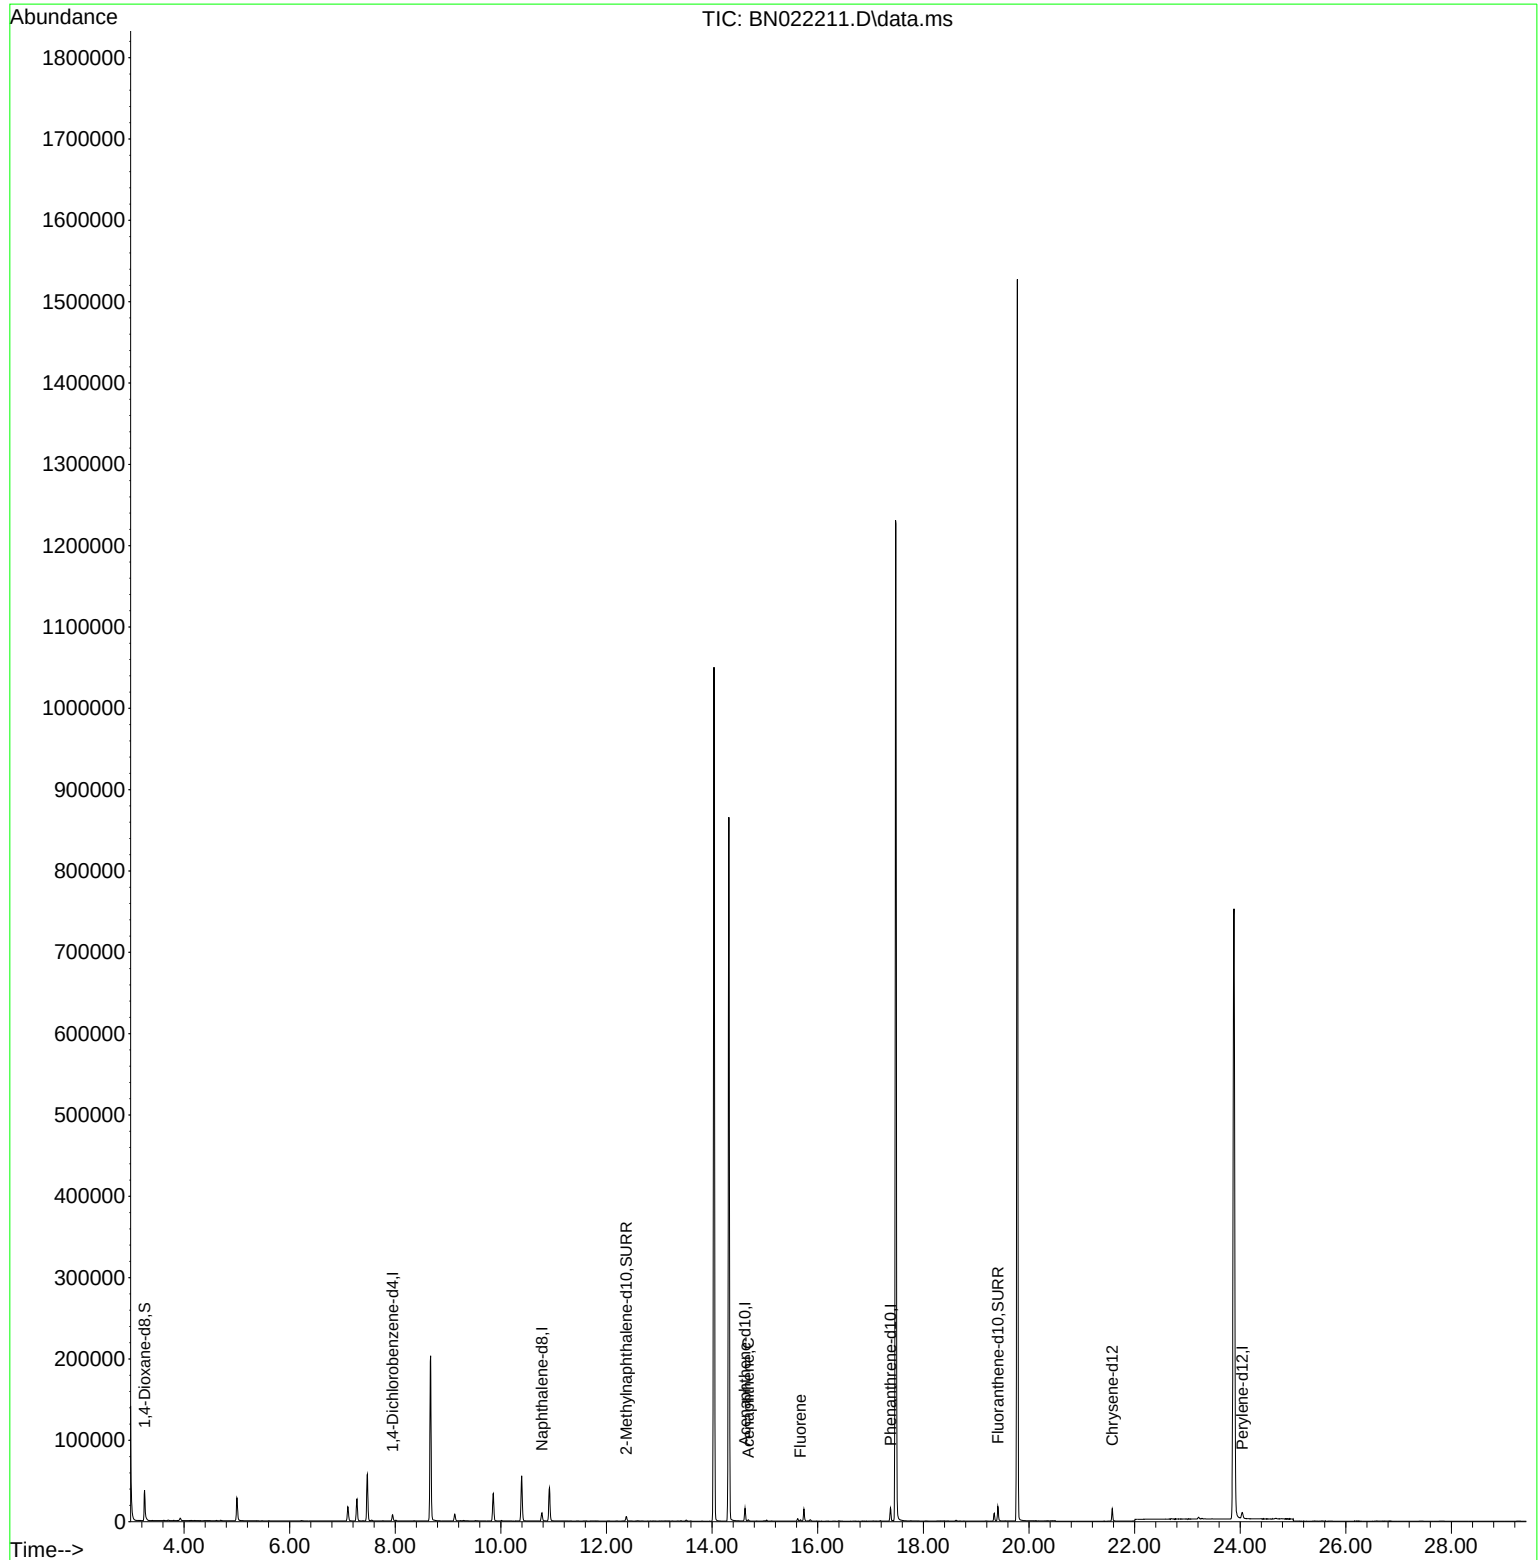


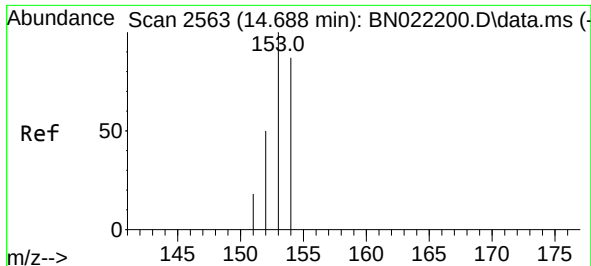

#11
Acenaphthene
Concen: 0.027 ng/ul
RT: 14.688 min Scan# 2563
Delta R.T. 0.001 min
Lab File: BN022211.D
Acq: 20 Oct 2022 00:15

Instrument :
BNA_N
ClientSampleId :
C1BB5

Tgt Ion:153 Resp: 831
Ion Ratio Lower Upper
153 100
152 56.5 40.6 61.0
154 91.5 70.6 106.0

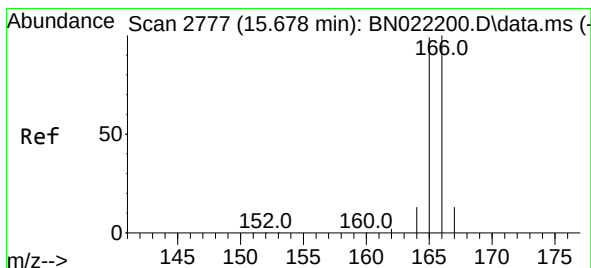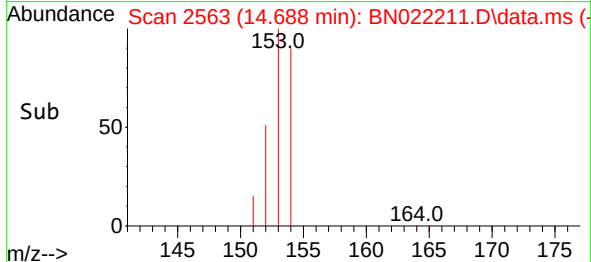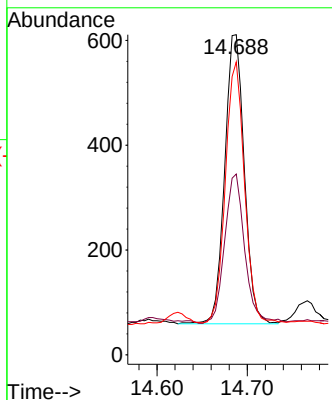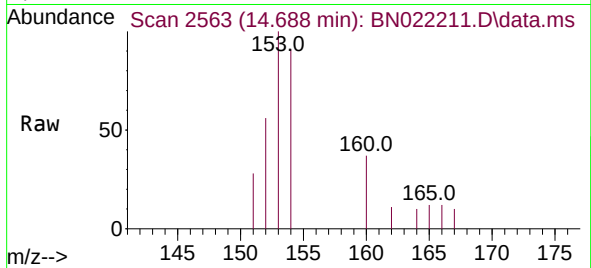

#12
Fluorene
Concen: 0.025 ng/ul
RT: 15.673 min Scan# 2776
Delta R.T. -0.004 min
Lab File: BN022211.D
Acq: 20 Oct 2022 00:15

Tgt Ion:166 Resp: 902
Ion Ratio Lower Upper
166 100
165 99.1 78.2 117.2
167 22.2 11.0 16.4#

