

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
 Data File : BN022234.D
 Acq On : 20 Oct 2022 15:25
 Operator : CG/JU
 Sample : N5060-08
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BG8

Quant Time: Oct 21 01:50:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.949	152	4410	0.400	ng/ul	0.00
4) Naphthalene-d8	10.778	136	15035	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.623	164	9240	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.378	188	18689	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.582	240	12381	0.400	ng/ul	# 0.00
23) Perylene-d12	24.043	264	9170	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.253	96	21697	3.786	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.373	152	6880	0.302	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	16727	0.402	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.827	128	2044	0.046	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
Data File : BN022234.D
Acq On : 20 Oct 2022 15:25
Operator : CG/JU
Sample : N5060-08
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BG8


Quant Time: Oct 21 01:50:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration

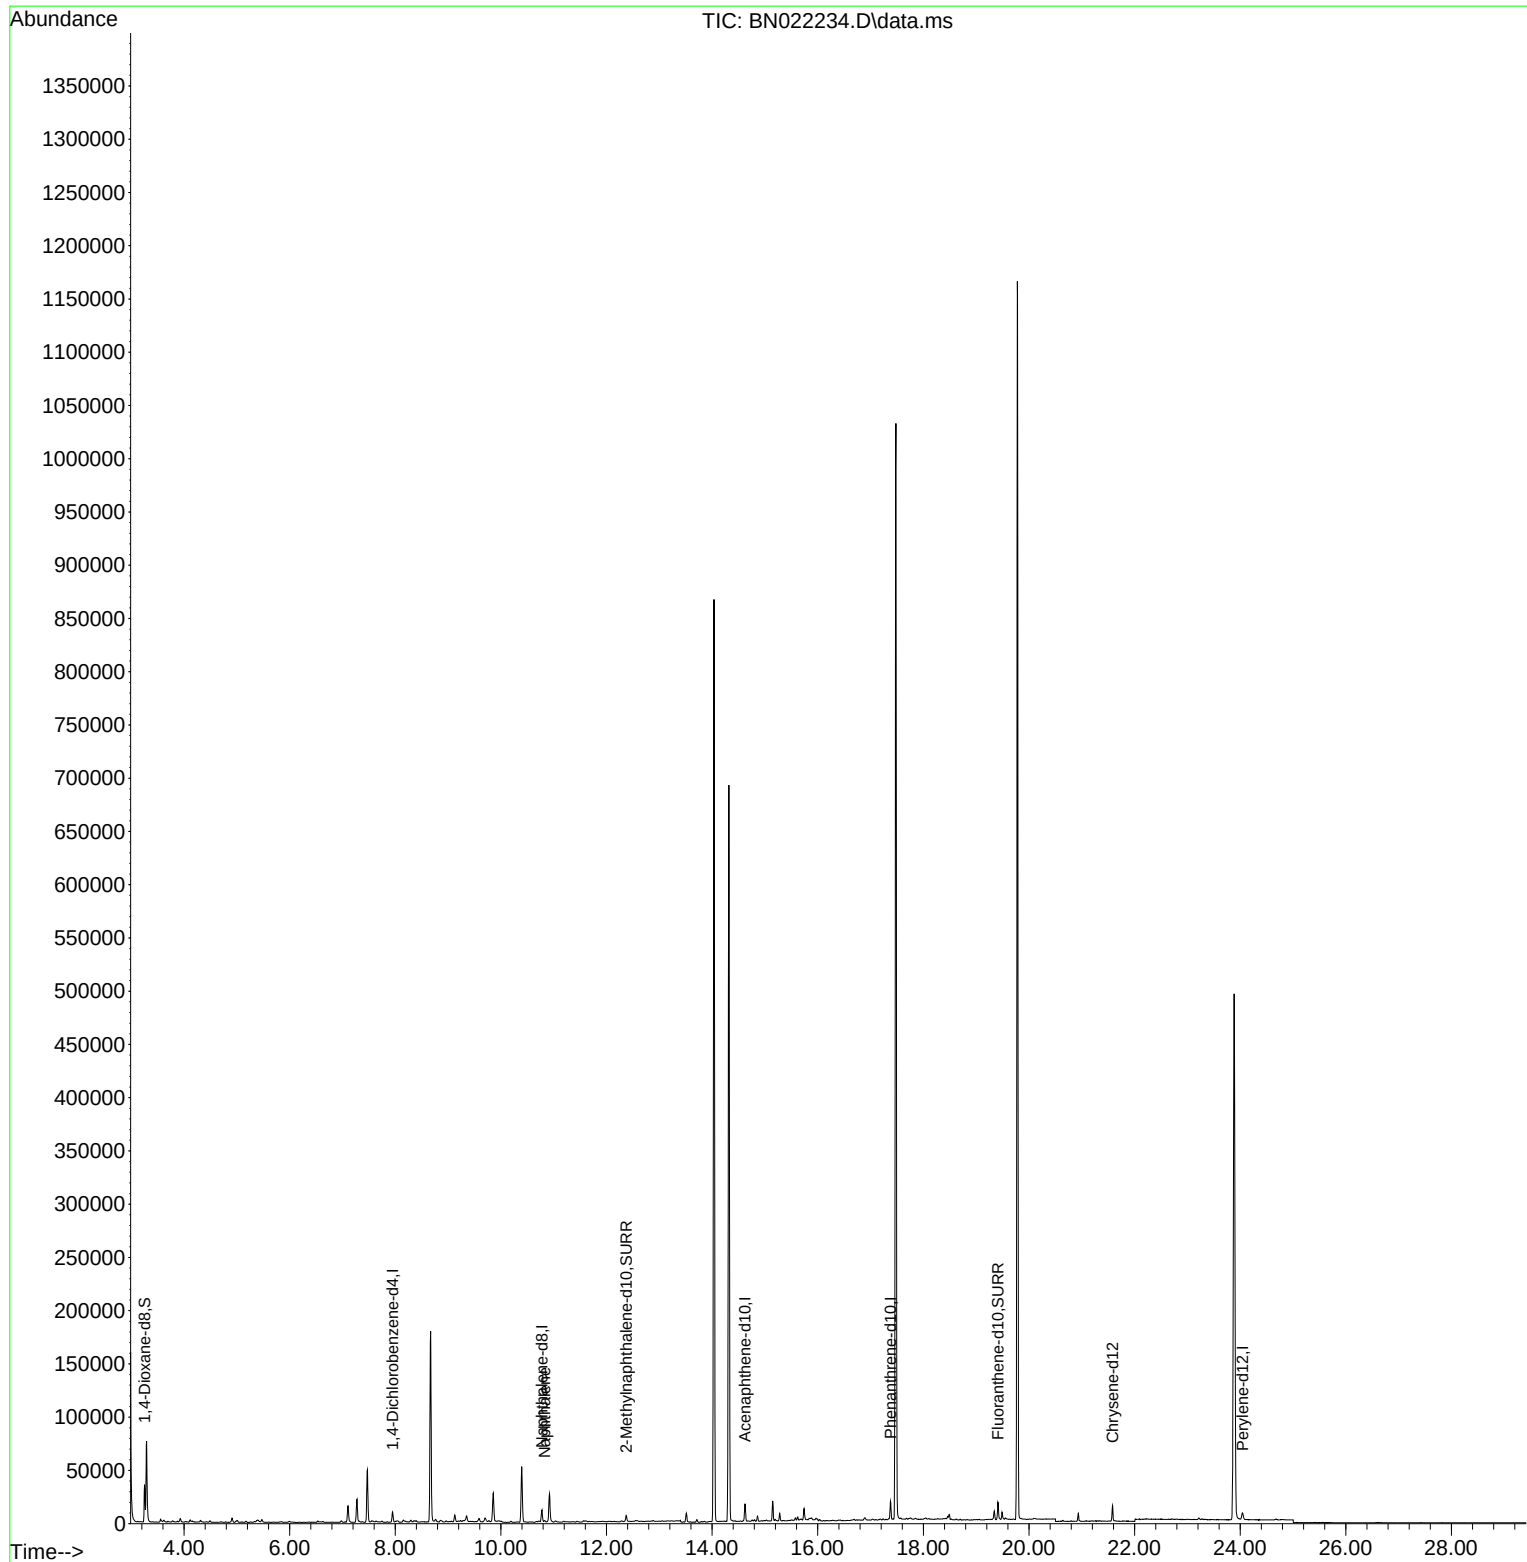

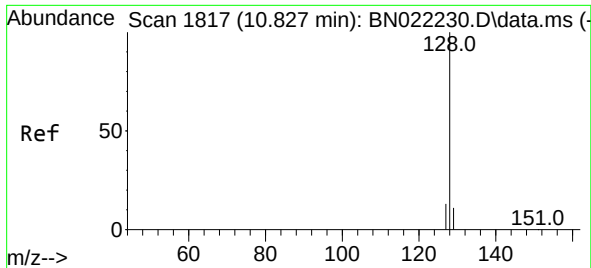

#5
Naphthalene
Concen: 0.046 ng/ul
RT: 10.827 min Scan# 1817
Delta R.T. -0.004 min
Lab File: BN022234.D
Acq: 20 Oct 2022 15:25

Instrument :
BNA_N
ClientSampleId :
C1BG8

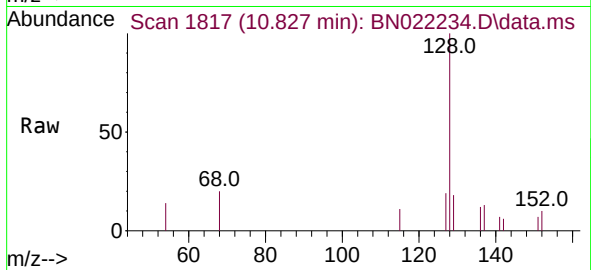

Tgt Ion:128 Resp: 2044
Ion Ratio Lower Upper
128 100
129 18.1 9.3 13.9#
127 19.4 10.7 16.1#

