

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
 Data File : BN022238.D
 Acq On : 20 Oct 2022 17:54
 Operator : CG/JU
 Sample : N5060-16
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BD7

Quant Time: Oct 21 01:51:47 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.949	152	4798	0.400	ng/ul	0.00
4) Naphthalene-d8	10.778	136	15965	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.623	164	9339	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.378	188	19392	0.400	ng/ul	0.00
17) Chrysene-d12	21.582	240	12941	0.400	ng/ul	0.00
23) Perylene-d12	24.043	264	10056	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	26584	4.263	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.373	152	7598	0.315	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	16265	0.374	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.827	128	1112	0.024	ng/ul#	Qvalue 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
Data File : BN022238.D
Acq On : 20 Oct 2022 17:54
Operator : CG/JU
Sample : N5060-16
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BD7


Quant Time: Oct 21 01:51:47 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration

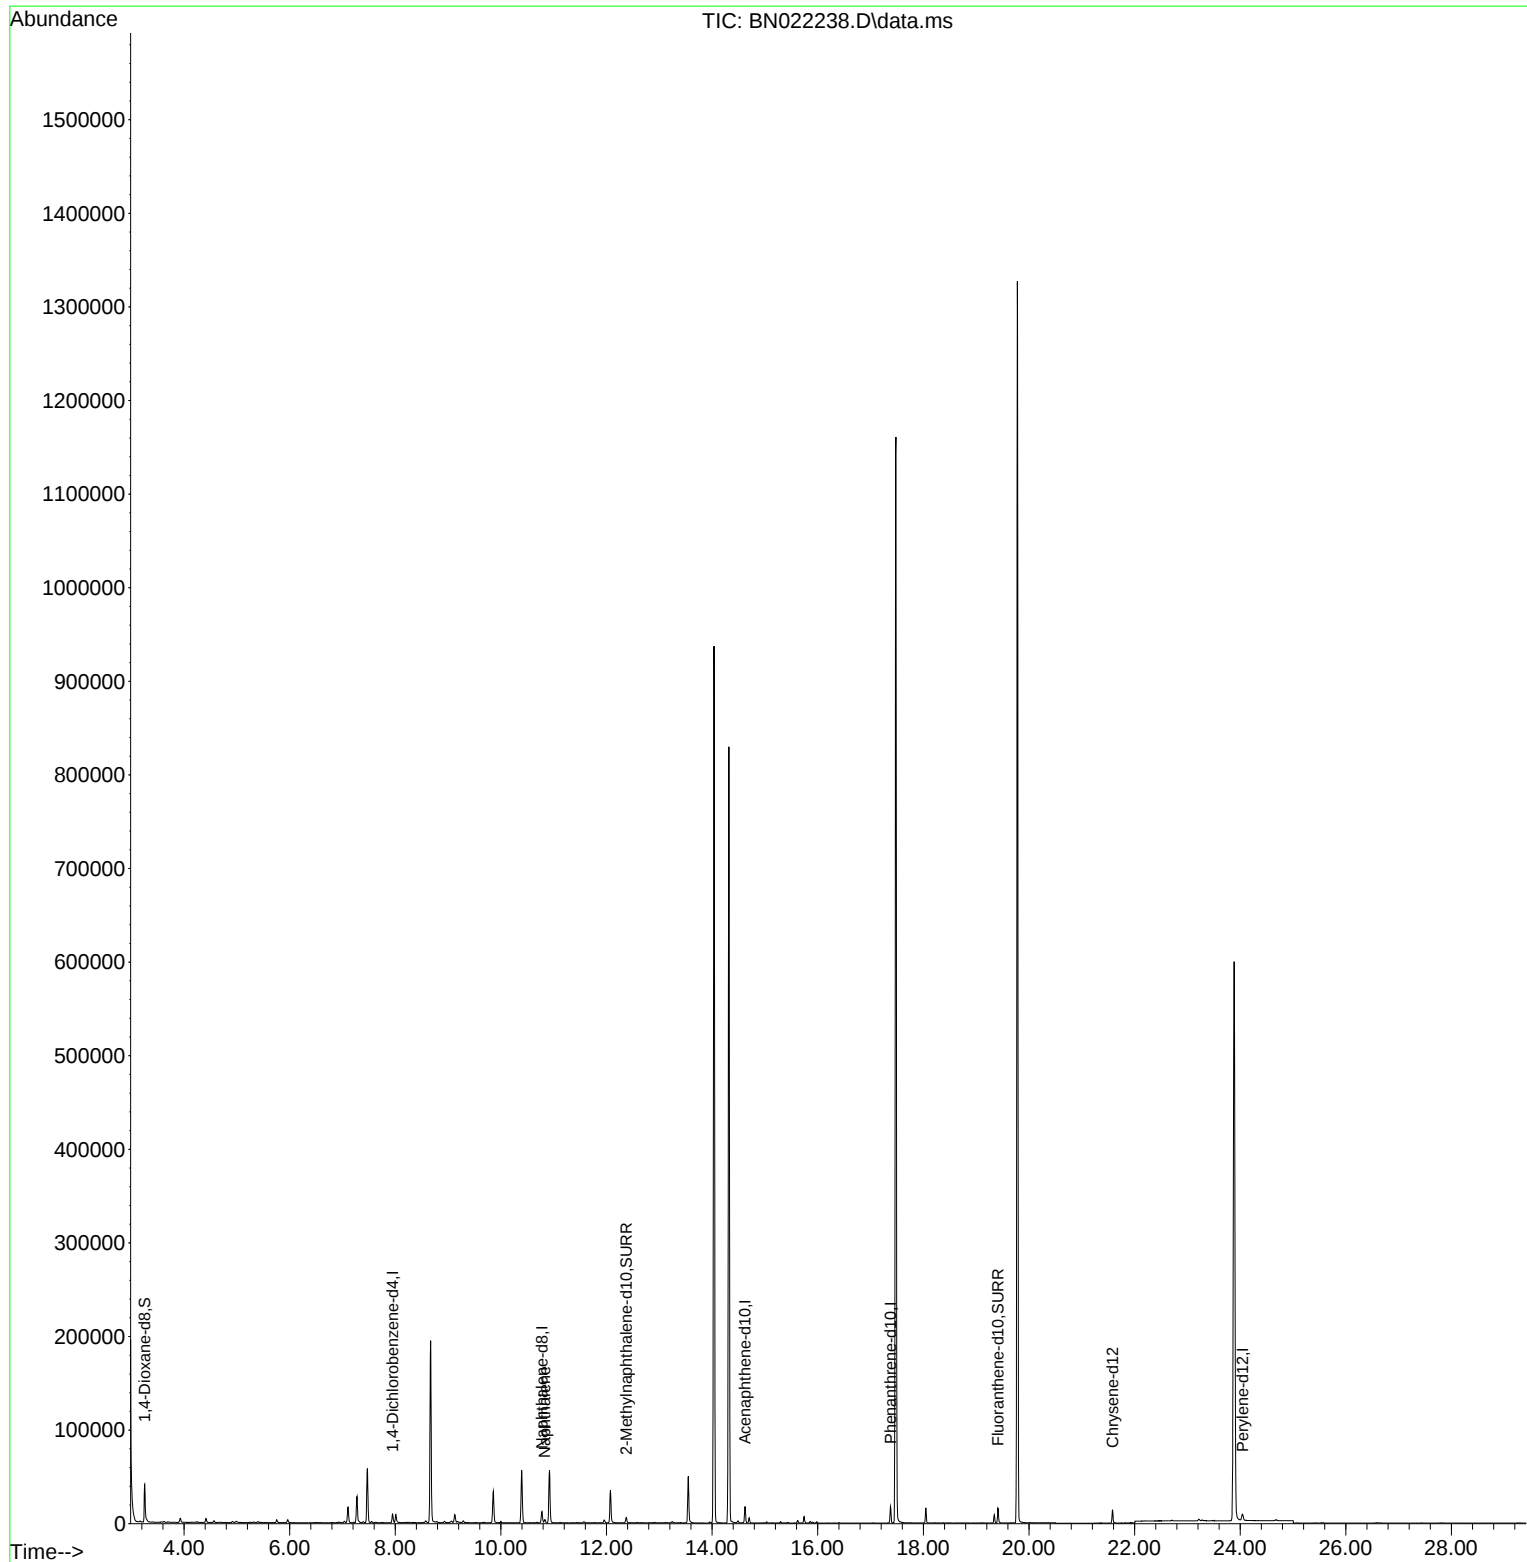

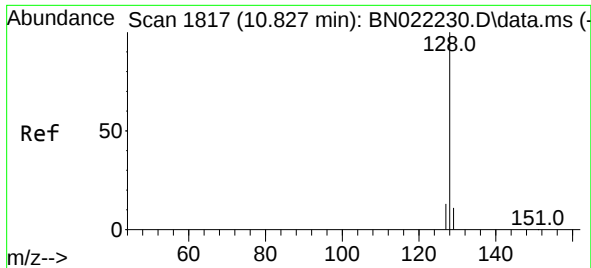

#5
Naphthalene
Concen: 0.024 ng/ul
RT: 10.827 min Scan# 1817
Delta R.T. -0.004 min
Lab File: BN022238.D
Acq: 20 Oct 2022 17:54

Instrument :
BNA_N
ClientSampleId :
C1BD7

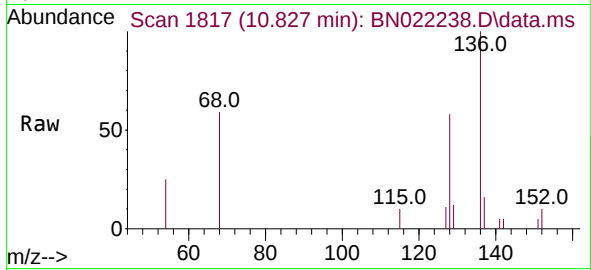

Tgt Ion:128 Resp: 1112
Ion Ratio Lower Upper
128 100
129 20.7 9.3 13.9#
127 19.4 10.7 16.1#

