

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
 Data File : BN022241.D
 Acq On : 20 Oct 2022 19:46
 Operator : CG/JU
 Sample : N5060-13
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BD6

Quant Time: Oct 21 01:52:27 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.948	152	4313	0.400	ng/ul	0.00
4) Naphthalene-d8	10.778	136	14647	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.623	164	8677	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.378	188	17827	0.400	ng/ul	0.00
17) Chrysene-d12	21.579	240	11433	0.400	ng/ul	0.00
23) Perylene-d12	24.043	264	8614	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.253	96	22224	3.965	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.372	152	8380	0.378	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	17850	0.465	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.827	128	898	0.021	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102022\
 Data File : BN022241.D
 Acq On : 20 Oct 2022 19:46
 Operator : CG/JU
 Sample : N5060-13
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BD6


Quant Time: Oct 21 01:52:27 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

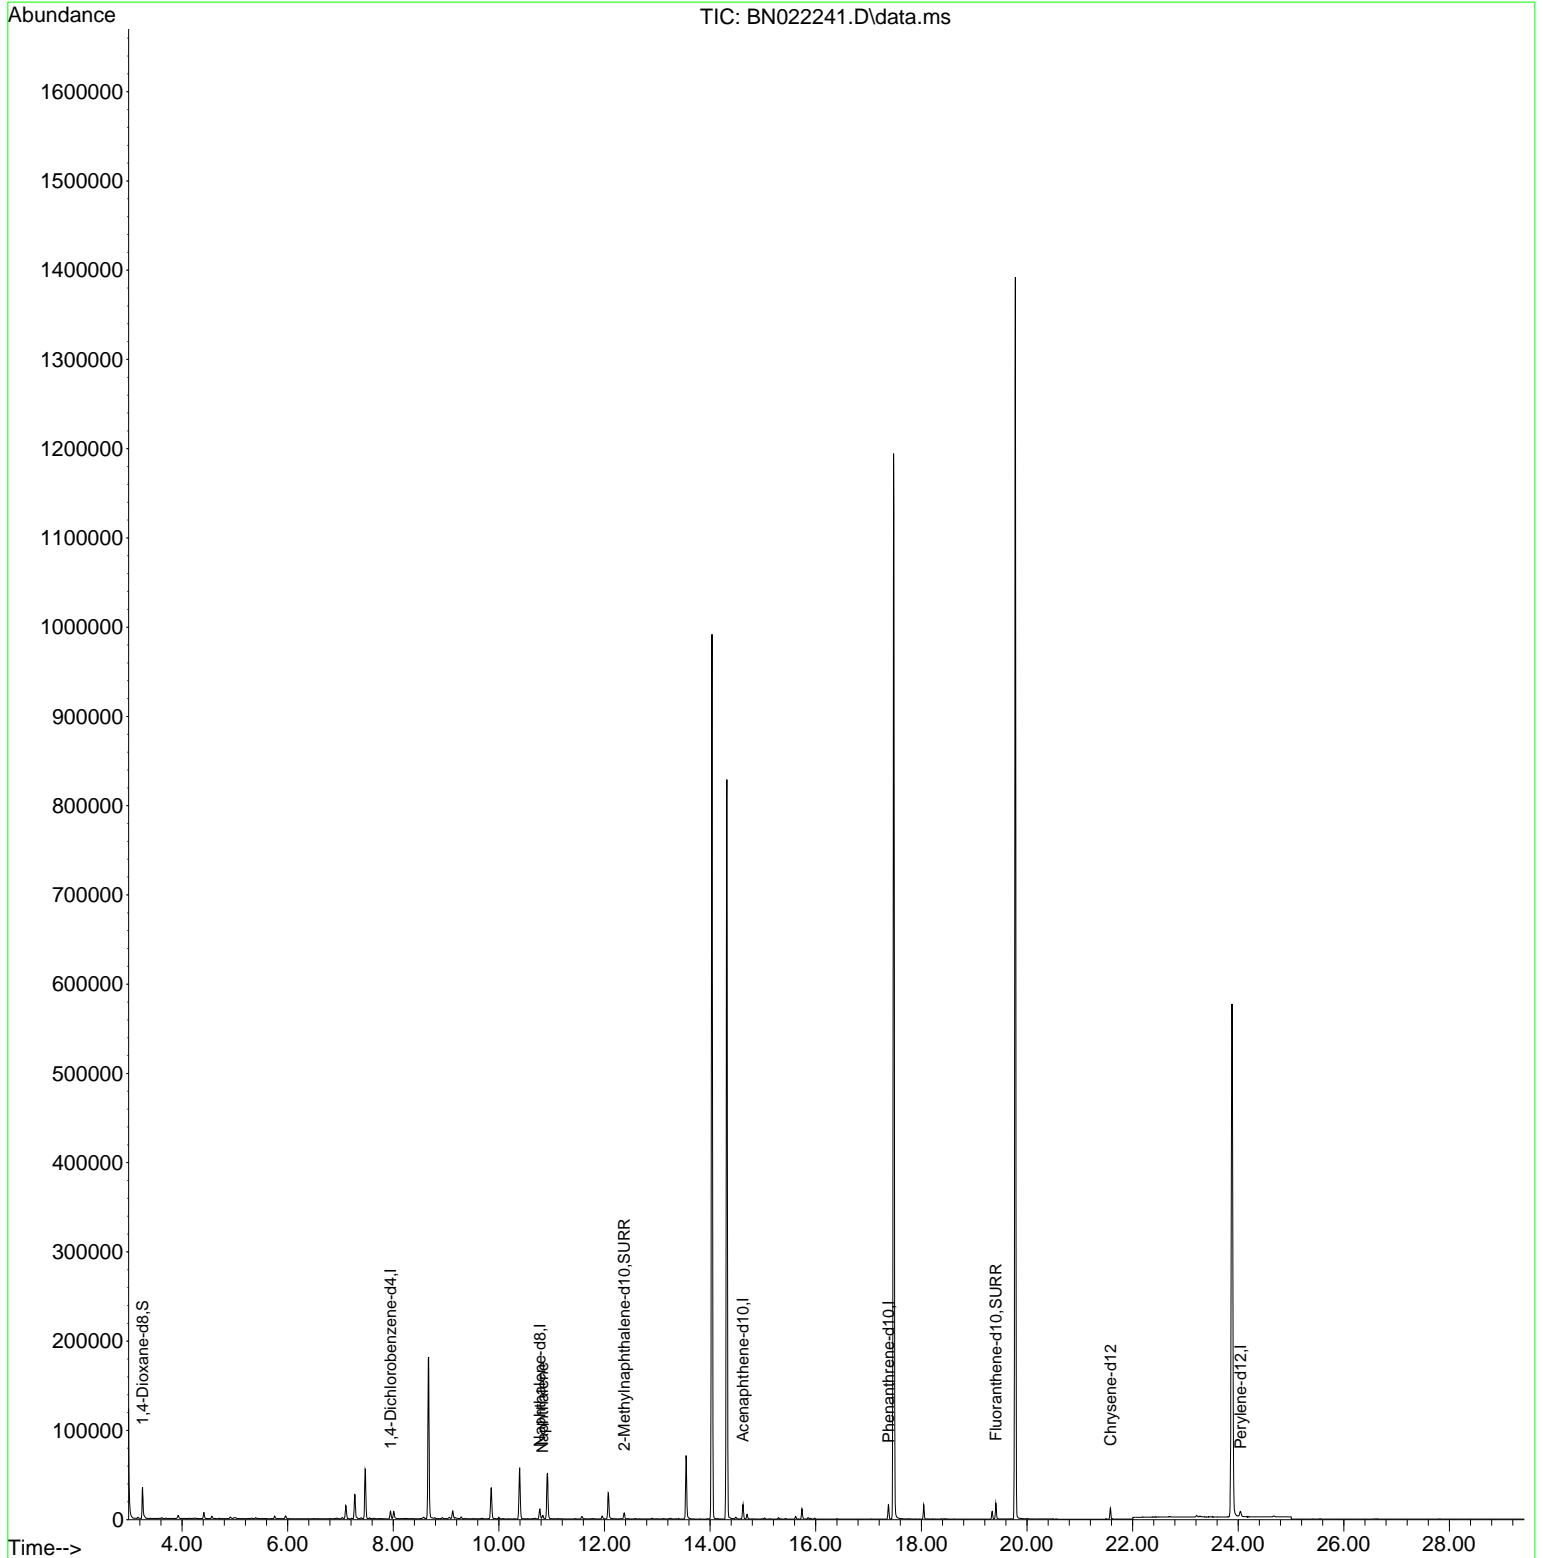

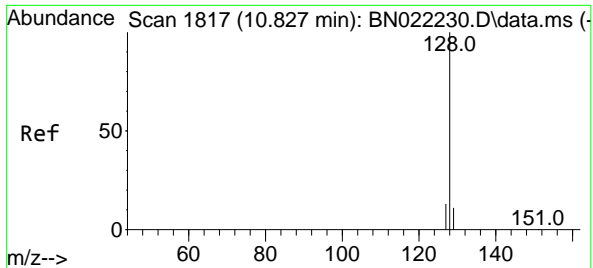

#5
 Naphthalene
 Concen: 0.021 ng/ul
 RT: 10.827 min Scan# 1817
 Delta R.T. -0.004 min
 Lab File: BN022241.D
 Acq: 20 Oct 2022 19:46

Instrument :
 BNA_N
 ClientSampleId :
 C1BD6

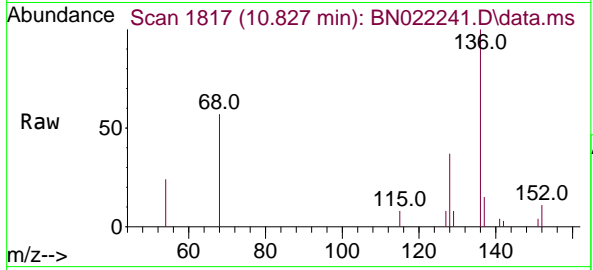

Tgt Ion:128 Resp: 898

Ion	Ratio	Lower	Upper
128	100		
129	22.6	9.3	13.9#
127	21.1	10.7	16.1#

