

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102122\
 Data File : BM037169.D
 Acq On : 21 Oct 2022 11:01
 Operator : CG/JU
 Sample : N5015-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BF8

Quant Time: Oct 22 02:31:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 20 02:11:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	3193	0.400	ng/ul	0.00
4) Naphthalene-d8	10.704	136	10256	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.533	164	6244	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.275	188	13284	0.400	ng/ul	0.00
17) Chrysene-d12	21.453	240	11039	0.400	ng/ul	0.00
23) Perylene-d12	23.824	264	10982	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	21733	5.582	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.294	152	5185	0.356	ng/ul	0.00
18) Fluoranthene-d10	19.299	212	12292	0.368	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.348	88	88	0.022	ng/ul#	34
20) Pyrene	19.661	202	2780	0.057	ng/ul#	1
26) Benzo(a)pyrene	23.674	252	4626	0.099	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102122\
Data File : BM037169.D
Acq On : 21 Oct 2022 11:01
Operator : CG/JU
Sample : N5015-09
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BF8

Quant Time: Oct 22 02:31:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 20 02:11:25 2022
Response via : Initial Calibration




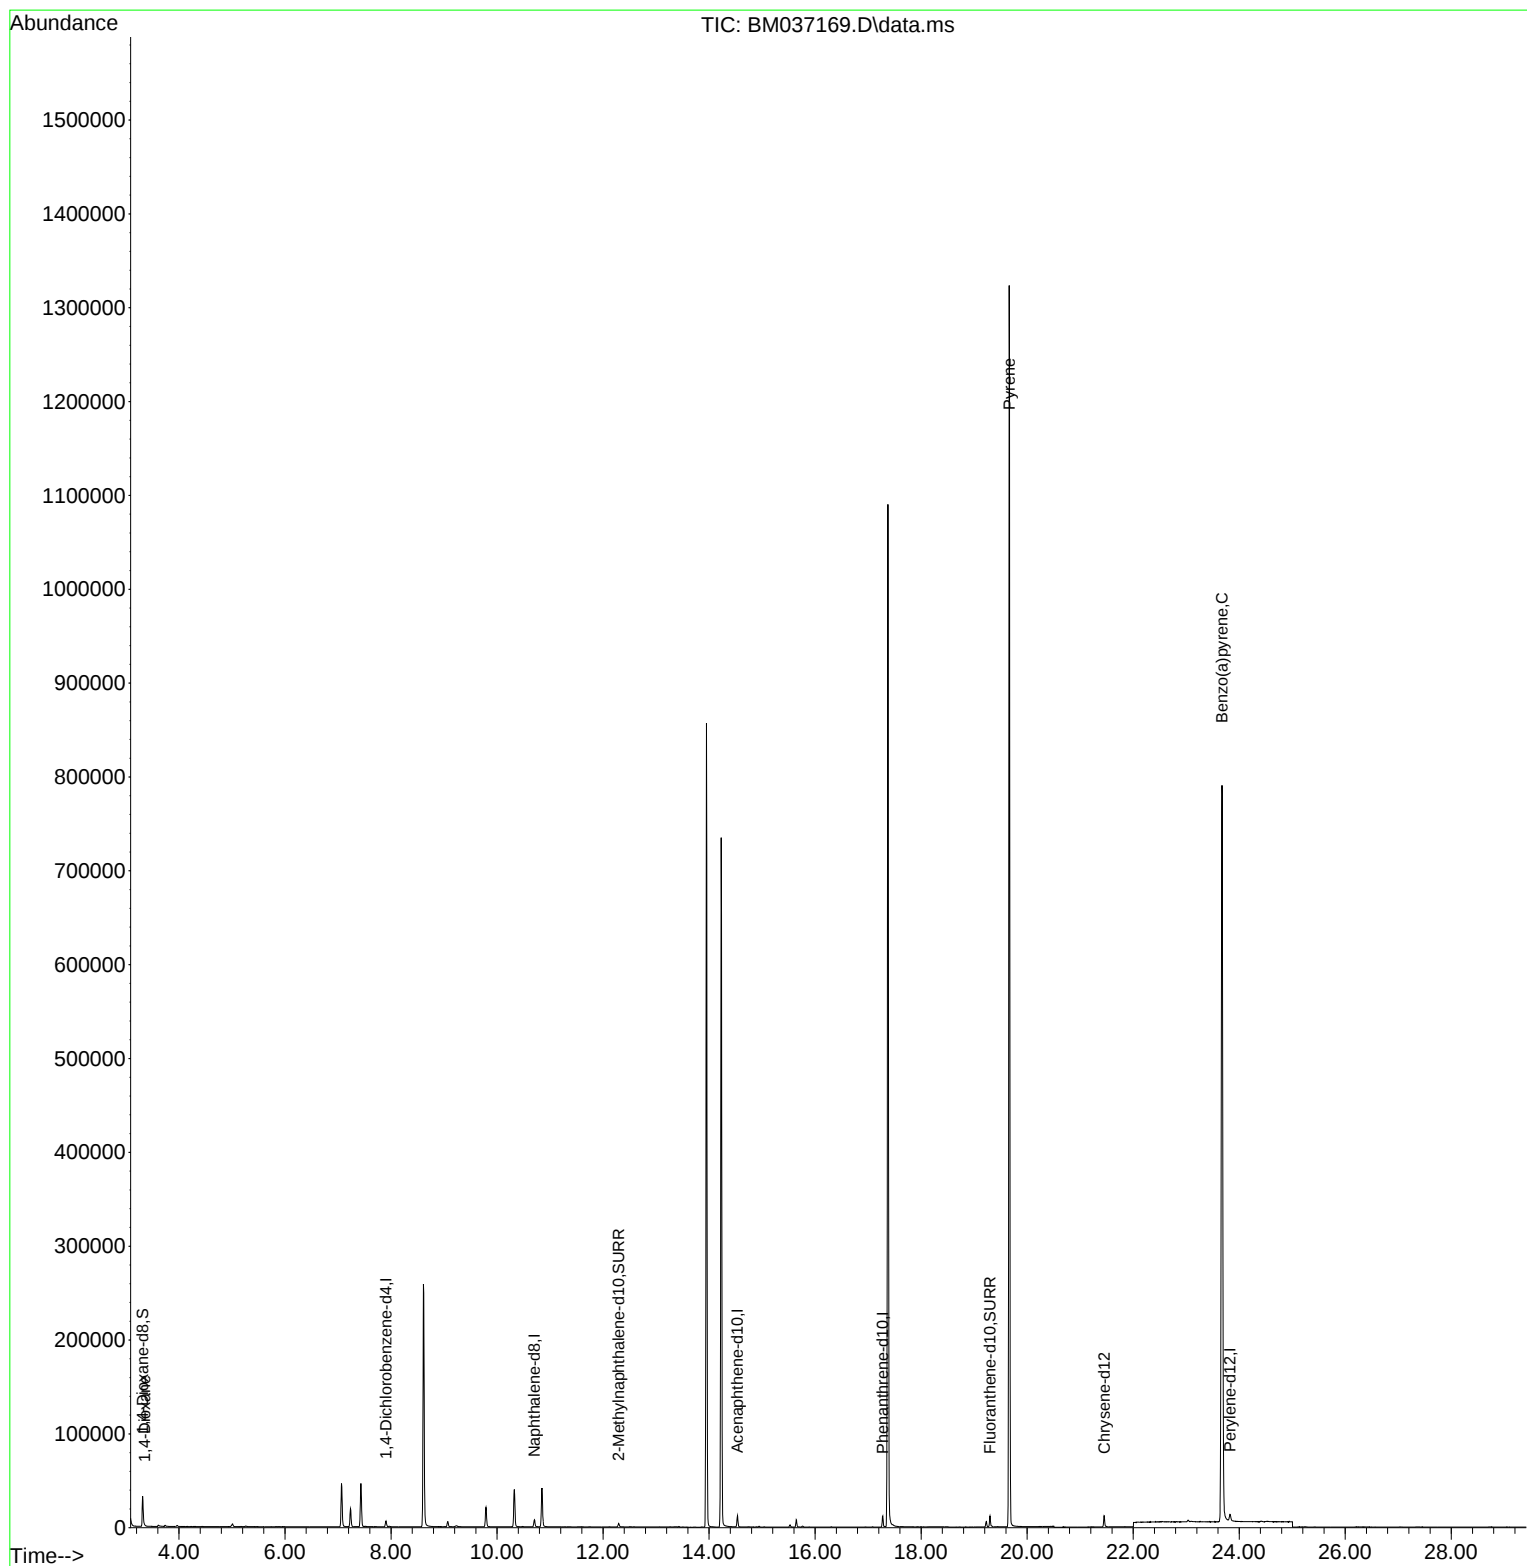


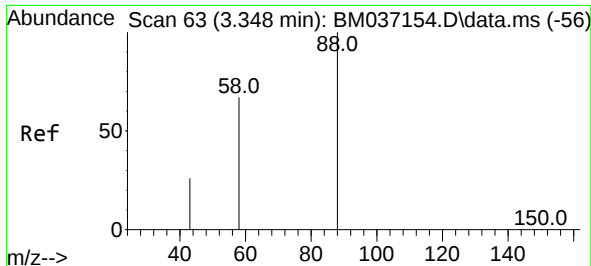

#2
1,4-Dioxane
Concen: 0.022 ng/ul
RT: 3.348 min Scan# 61
Delta R.T. -0.008 min
Lab File: BM037169.D
Acq: 21 Oct 2022 11:01




Instrument :
BNA_N
ClientSampleId :
C1BF8


Tgt Ion: 88 Resp: 88
Ion Ratio Lower Upper
88 100
43 98.6 25.5 38.3#
58 30.5 45.8 68.6#

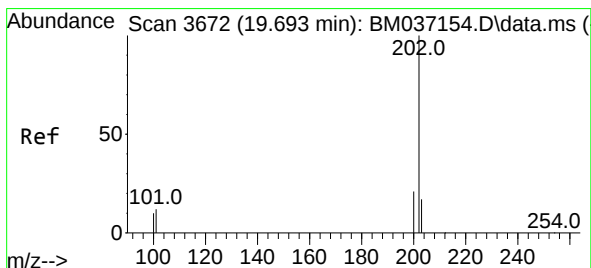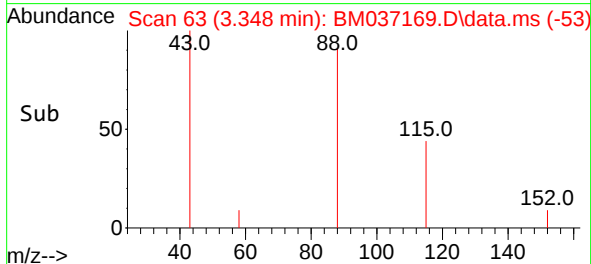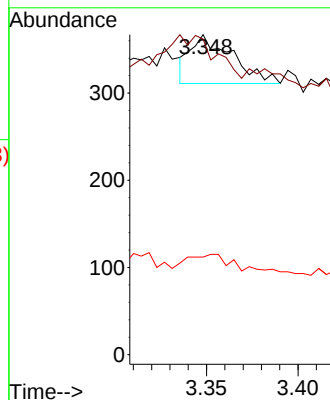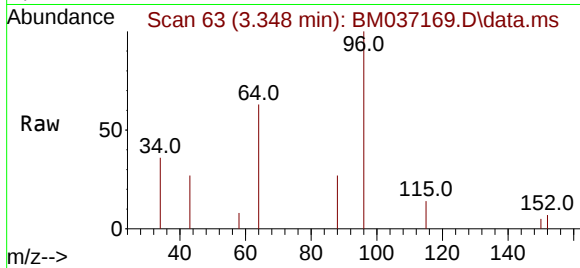

#20
Pyrene
Concen: 0.057 ng/ul
RT: 19.661 min Scan# 3665
Delta R.T. -0.037 min
Lab File: BM037169.D
Acq: 21 Oct 2022 11:01


Tgt Ion: 202 Resp: 2780
Ion Ratio Lower Upper
202 100
101 143.3 9.7 14.5#
100 1084.5 7.8 11.8#

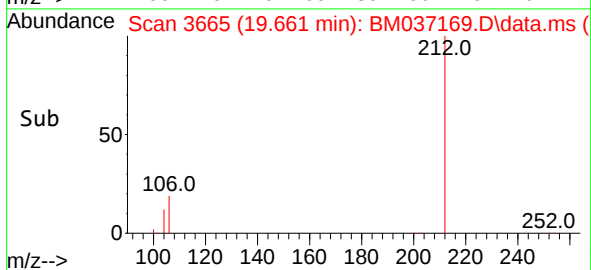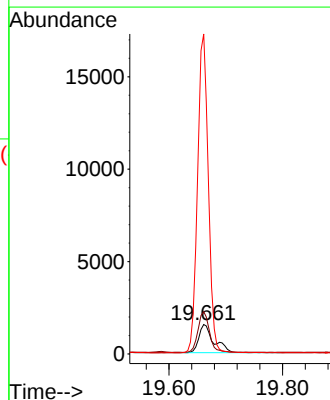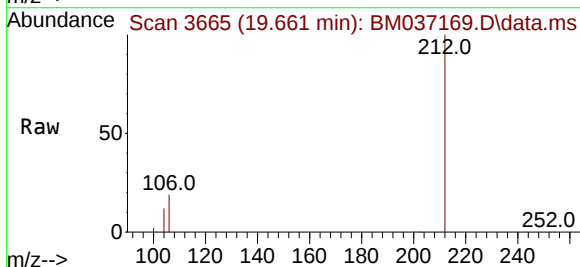

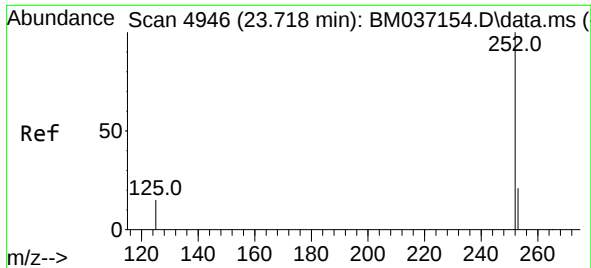

#26
 Benzo(a)pyrene
 Concen: 0.099 ng/ul
 RT: 23.674 min Scan# 4946
 Delta R.T. -0.055 min
 Lab File: BM037169.D
 Acq: 21 Oct 2022 11:01

Instrument :
 BNA_N
 ClientSampleId :
 C1BF8

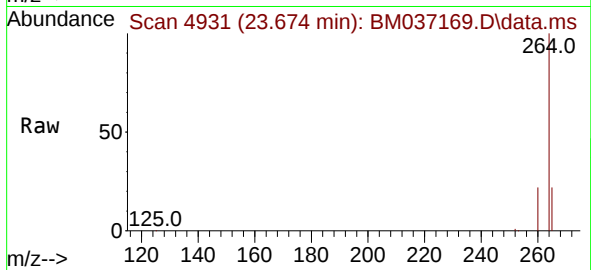

Tgt Ion:252 Resp: 4626
 Ion Ratio Lower Upper
 252 100
 253 50.3 22.1 33.1#
 125 45.5 17.6 26.4#

