

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102122\
 Data File : BM037170.D
 Acq On : 21 Oct 2022 11:37
 Operator : CG/JU
 Sample : N5015-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BE7

Quant Time: Oct 22 02:31:57 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 20 02:11:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	4787	0.400	ng/ul	0.00
4) Naphthalene-d8	10.704	136	15843	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.534	164	9608	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.276	188	20446	0.400	ng/ul	0.00
17) Chrysene-d12	21.452	240	18253	0.400	ng/ul	# 0.00
23) Perylene-d12	23.826	264	16114	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	33274	5.701	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.294	152	8168	0.363	ng/ul	0.00
18) Fluoranthene-d10	19.299	212	19021	0.344	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.662	202	4219	0.052	ng/ul#	1
21) Benzo(a)anthracene	21.455	228	2229	0.031	ng/ul#	67
26) Benzo(a)pyrene	23.674	252	6735	0.098	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102122\
Data File : BM037170.D
Acq On : 21 Oct 2022 11:37
Operator : CG/JU
Sample : N5015-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BE7

Quant Time: Oct 22 02:31:57 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 20 02:11:25 2022
Response via : Initial Calibration

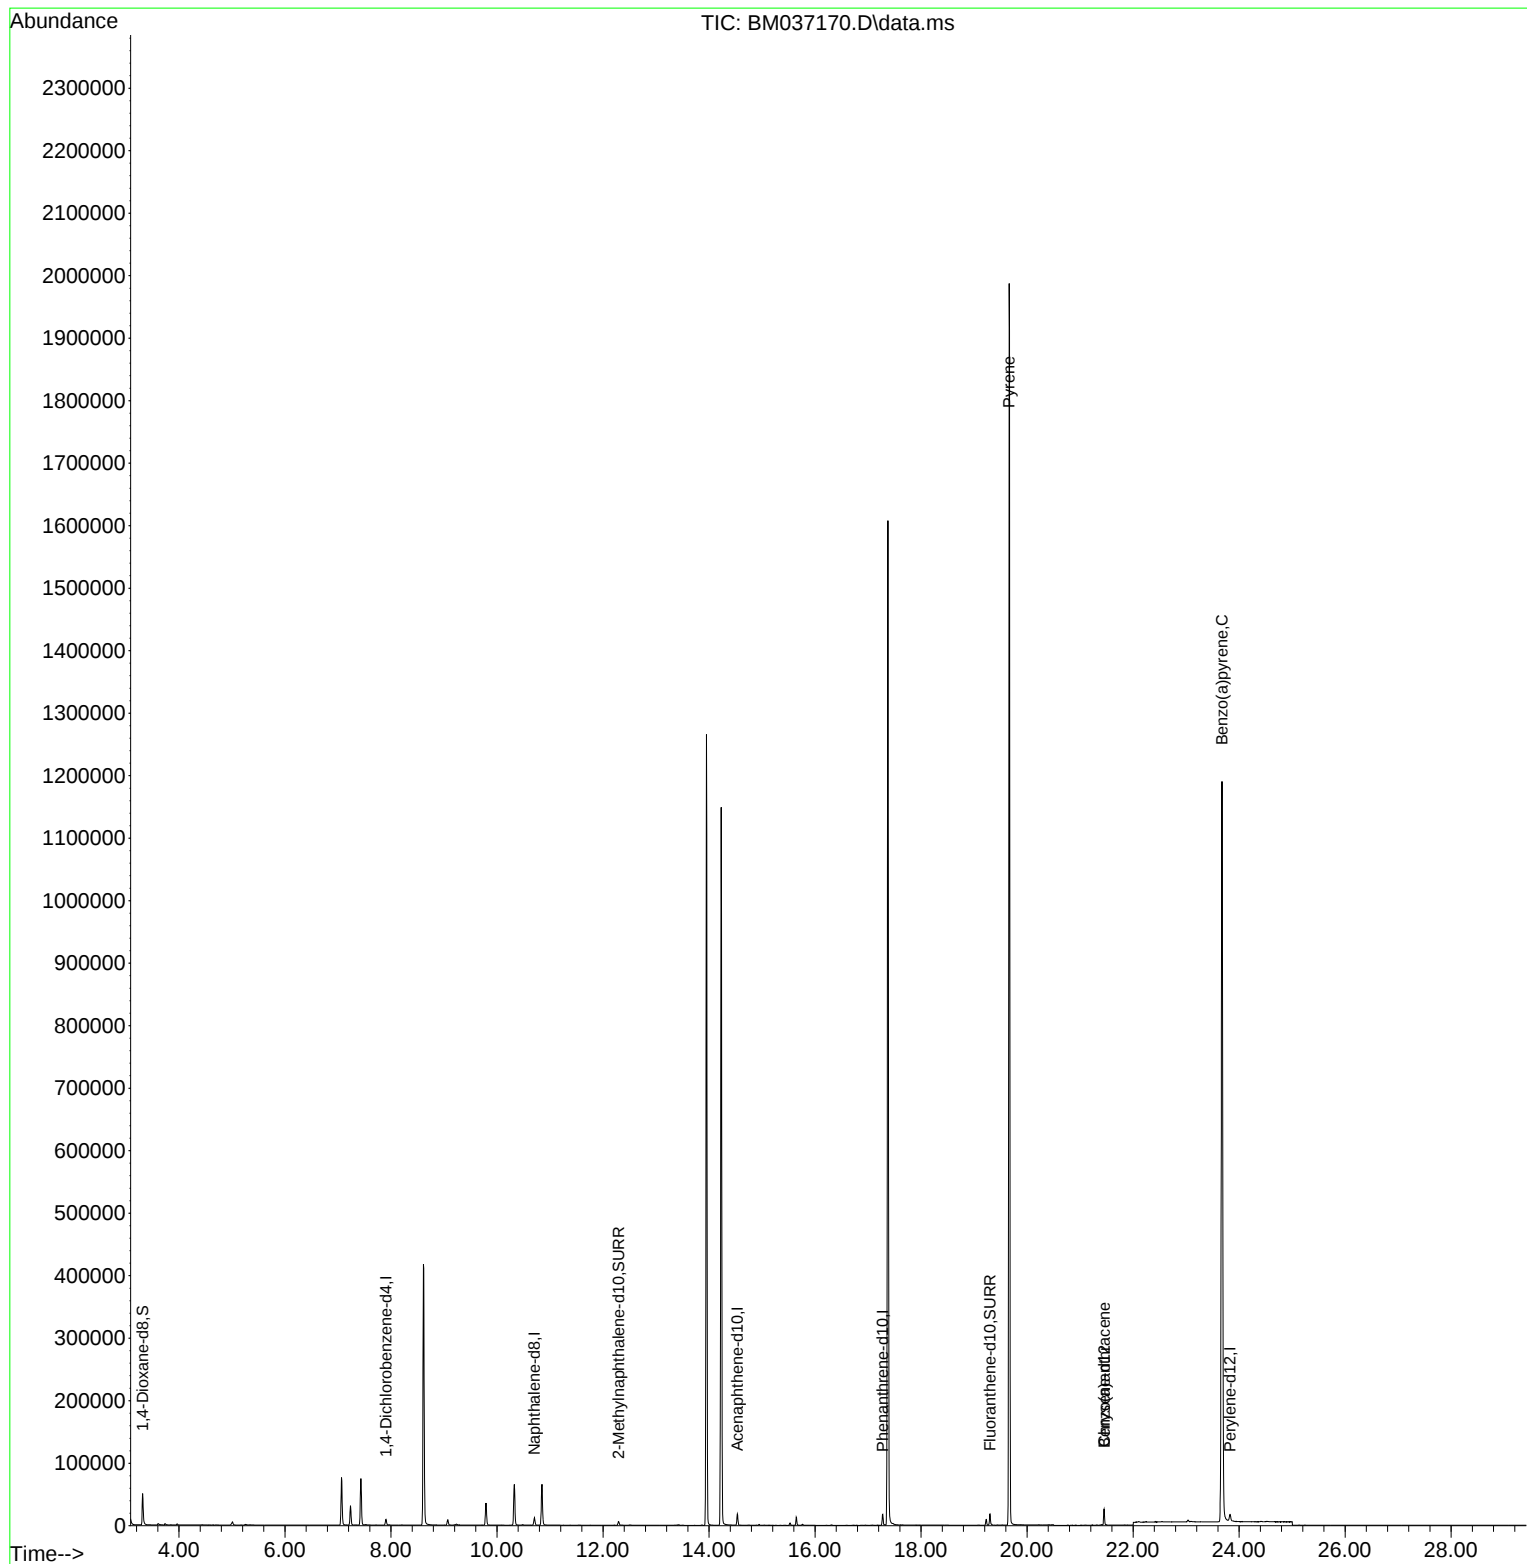

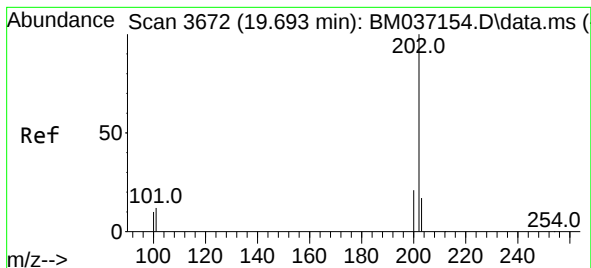

#20

Pyrene

Concen: 0.052 ng/ul

RT: 19.662 min Scan# 3

Delta R.T. -0.036 min

Lab File: BM037170.D

Acq: 21 Oct 2022 11:37

Instrument :





BNA_N

ClientSampleId :

C1BE7

Tgt Ion:202 Resp: 4219

Ion	Ratio	Lower	Upper
202	100		
101	144.2	9.7	14.5#
100	1101.5	7.8	11.8#

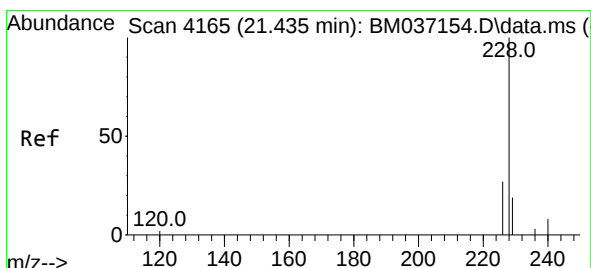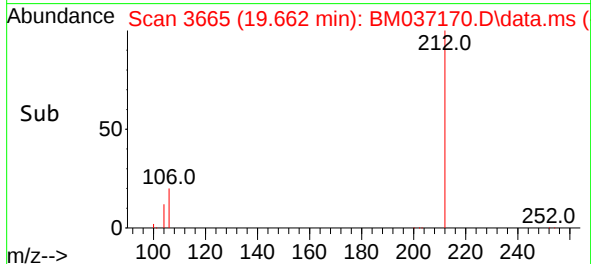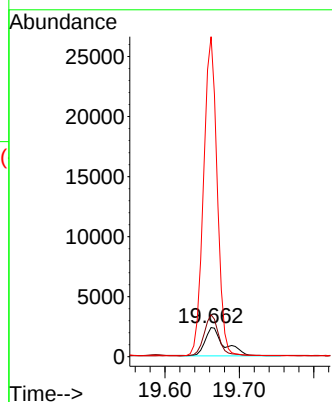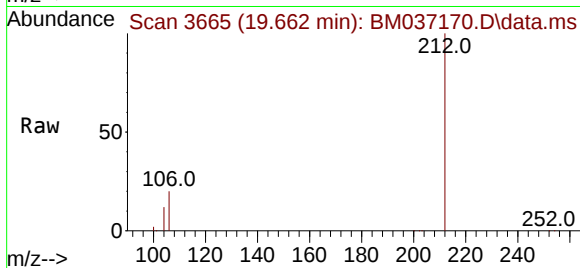

#21

Benzo(a)anthracene

Concen: 0.031 ng/ul

RT: 21.455 min Scan# 4172




Delta R.T. 0.014 min


Lab File: BM037170.D

Acq: 21 Oct 2022 11:37

Tgt Ion:228 Resp: 2229


Ion	Ratio	Lower	Upper
228	100		
229	32.5	15.8	23.6#
226	8.6	21.8	32.8#

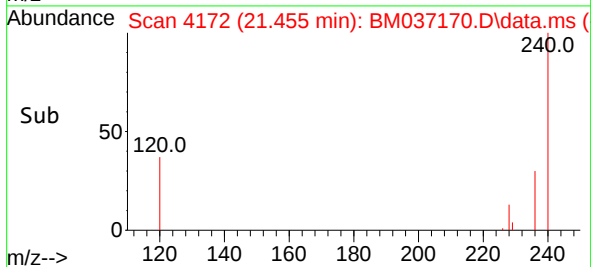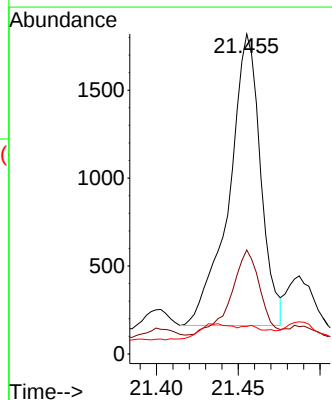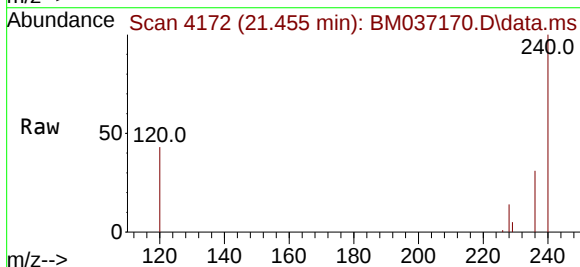

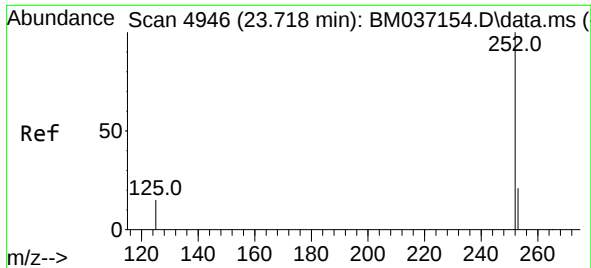

#26
 Benzo(a)pyrene
 Concen: 0.098 ng/ul
 RT: 23.674 min Scan# 4946
 Delta R.T. -0.056 min
 Lab File: BM037170.D
 Acq: 21 Oct 2022 11:37

Instrument :
 BNA_N
 ClientSampleId :
 C1BE7

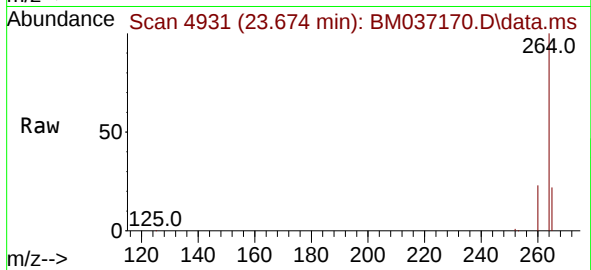

Tgt Ion:252 Resp: 6735
 Ion Ratio Lower Upper
 252 100
 253 44.1 22.1 33.1#
 125 38.3 17.6 26.4#

