

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102122\
 Data File : BM037172.D
 Acq On : 21 Oct 2022 13:59
 Operator : CG/JU
 Sample : PB148368BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK368

Quant Time: Oct 22 02:32:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 20 02:11:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	6222	0.400	ng/ul	0.00
4) Naphthalene-d8	10.704	136	19458	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.534	164	11186	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.276	188	22700	0.400	ng/ul	0.00
17) Chrysene-d12	21.452	240	16123	0.400	ng/ul	0.00
23) Perylene-d12	23.828	264	13349	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.318	96	36136	4.763	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.299	152	7241	0.262	ng/ul	0.00
18) Fluoranthene-d10	19.299	212	15218	0.312	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.524	166	2855	0.056	ng/ul#	14
20) Pyrene	19.662	202	2823	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.674	252	4552	0.080	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102122\
Data File : BM037172.D
Acq On : 21 Oct 2022 13:59
Operator : CG/JU
Sample : PB148368BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK368

Quant Time: Oct 22 02:32:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 20 02:11:25 2022
Response via : Initial Calibration




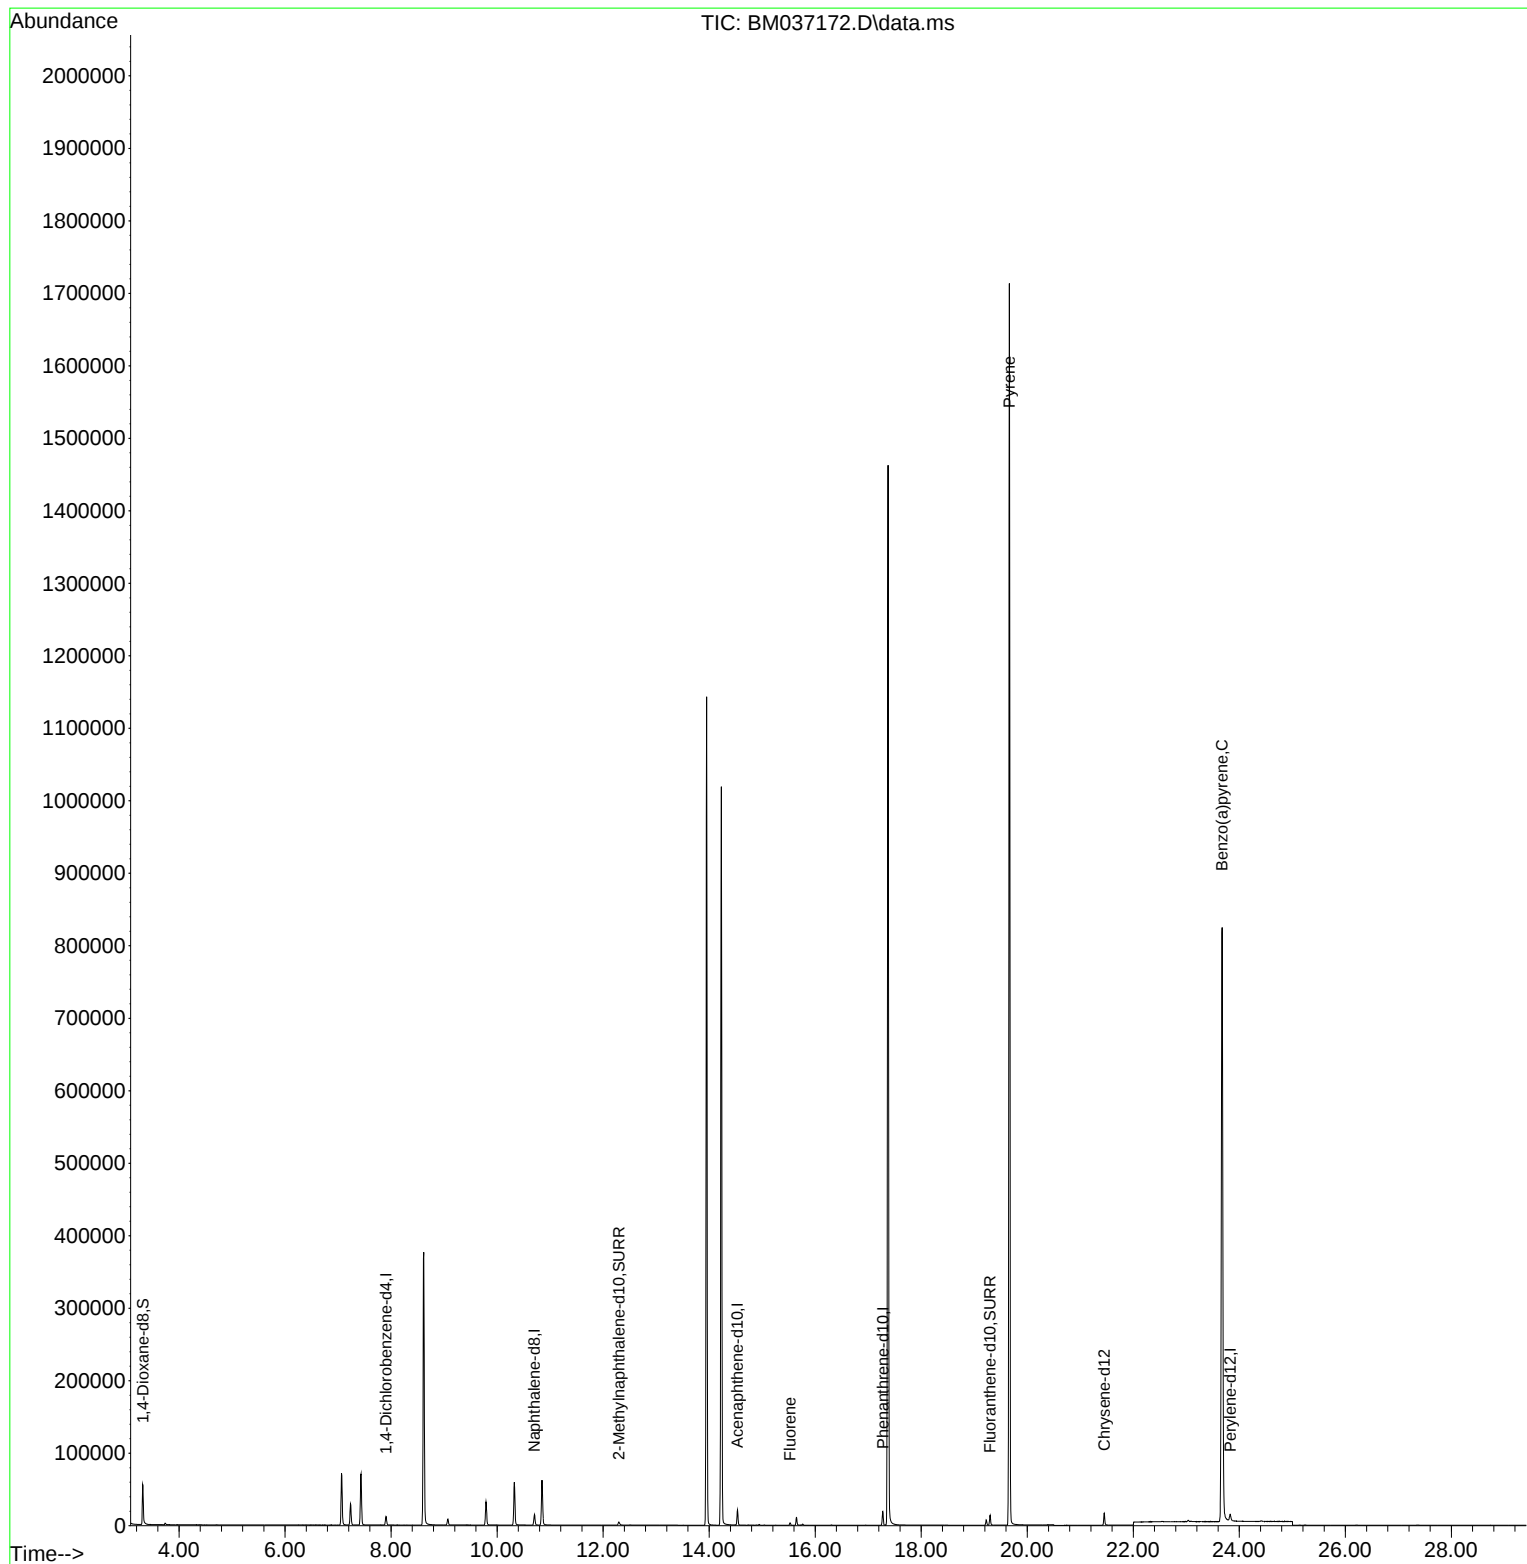


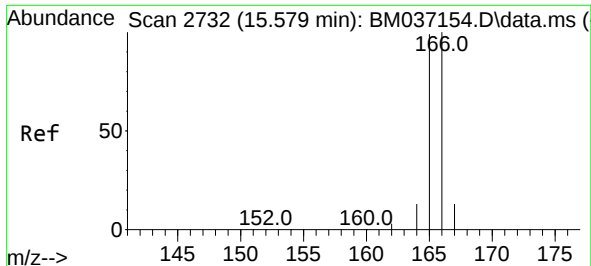

#12
Fluorene
Concen: 0.056 ng/ul
RT: 15.524 min Scan# 21
Delta R.T. -0.059 min
Lab File: BM037172.D
Acq: 21 Oct 2022 13:59




Instrument :
BNA_N
ClientSampleId :
SBLK368


Tgt Ion:166 Resp: 2855
Ion Ratio Lower Upper
166 100
165 7.1 79.4 119.2#
167 31.1 11.3 16.9#

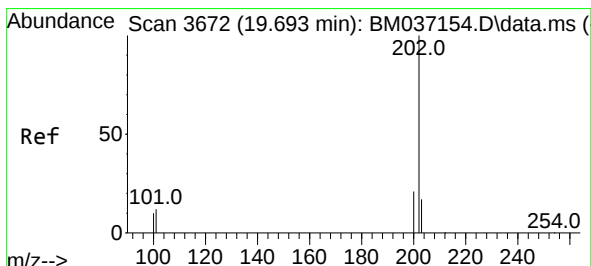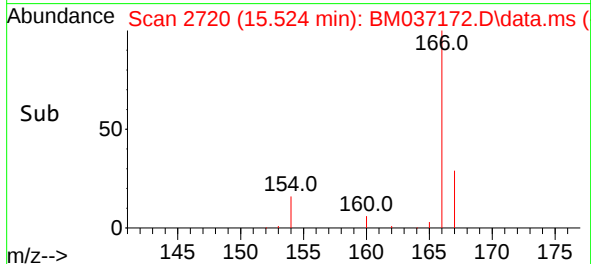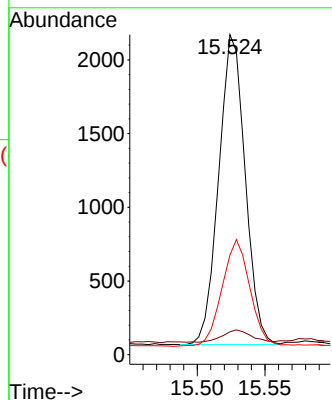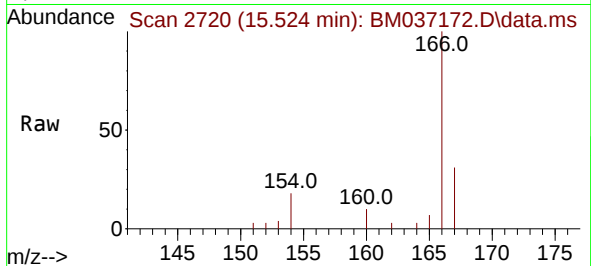

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.662 min Scan# 3665
Delta R.T. -0.036 min
Lab File: BM037172.D
Acq: 21 Oct 2022 13:59


Tgt Ion:202 Resp: 2823
Ion Ratio Lower Upper
202 100
101 148.4 9.7 14.5#
100 1118.2 7.8 11.8#

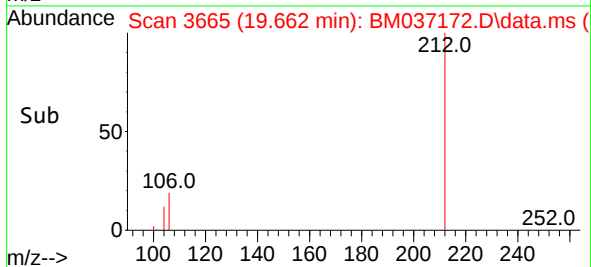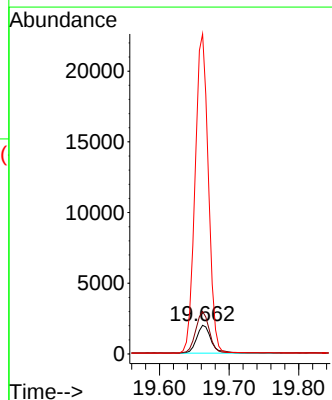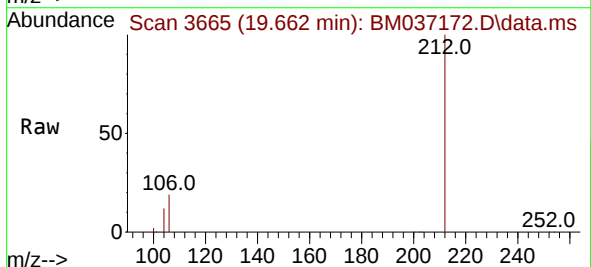

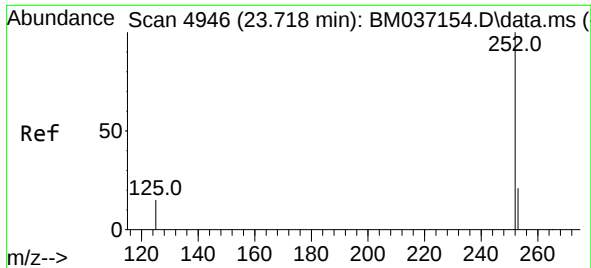

#26
 Benzo(a)pyrene
 Concen: 0.080 ng/ul
 RT: 23.674 min Scan# 4946
 Delta R.T. -0.056 min
 Lab File: BM037172.D
 Acq: 21 Oct 2022 13:59

Instrument :
 BNA_N
 ClientSampleId :
 SBLK368

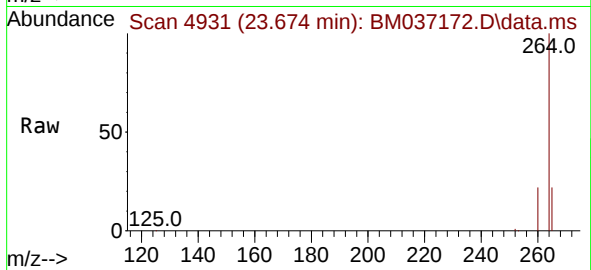

Tgt Ion:252 Resp: 4552
 Ion Ratio Lower Upper
 252 100
 253 47.4 22.1 33.1#
 125 43.3 17.6 26.4#

