

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102122\
 Data File : BM037178.D
 Acq On : 21 Oct 2022 17:36
 Operator : CG/JU
 Sample : N5103-05
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COBX2

Quant Time: Oct 22 02:34:03 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 20 02:11:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	4679	0.400	ng/ul	0.00
4) Naphthalene-d8	10.704	136	14862	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.533	164	9086	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.275	188	18486	0.400	ng/ul	0.00
17) Chrysene-d12	21.450	240	14988	0.400	ng/ul	0.00
23) Perylene-d12	23.826	264	13773	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	18550	3.252	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.294	152	5907	0.280	ng/ul	0.00
18) Fluoranthene-d10	19.298	212	17294	0.381	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.352	88	1074	0.181	ng/ul#	78
20) Pyrene	19.661	202	3374	0.051	ng/ul#	1
26) Benzo(a)pyrene	23.672	252	6046	0.103	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102122\
Data File : BM037178.D
Acq On : 21 Oct 2022 17:36
Operator : CG/JU
Sample : N5103-05
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BX2

Quant Time: Oct 22 02:34:03 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 20 02:11:25 2022
Response via : Initial Calibration




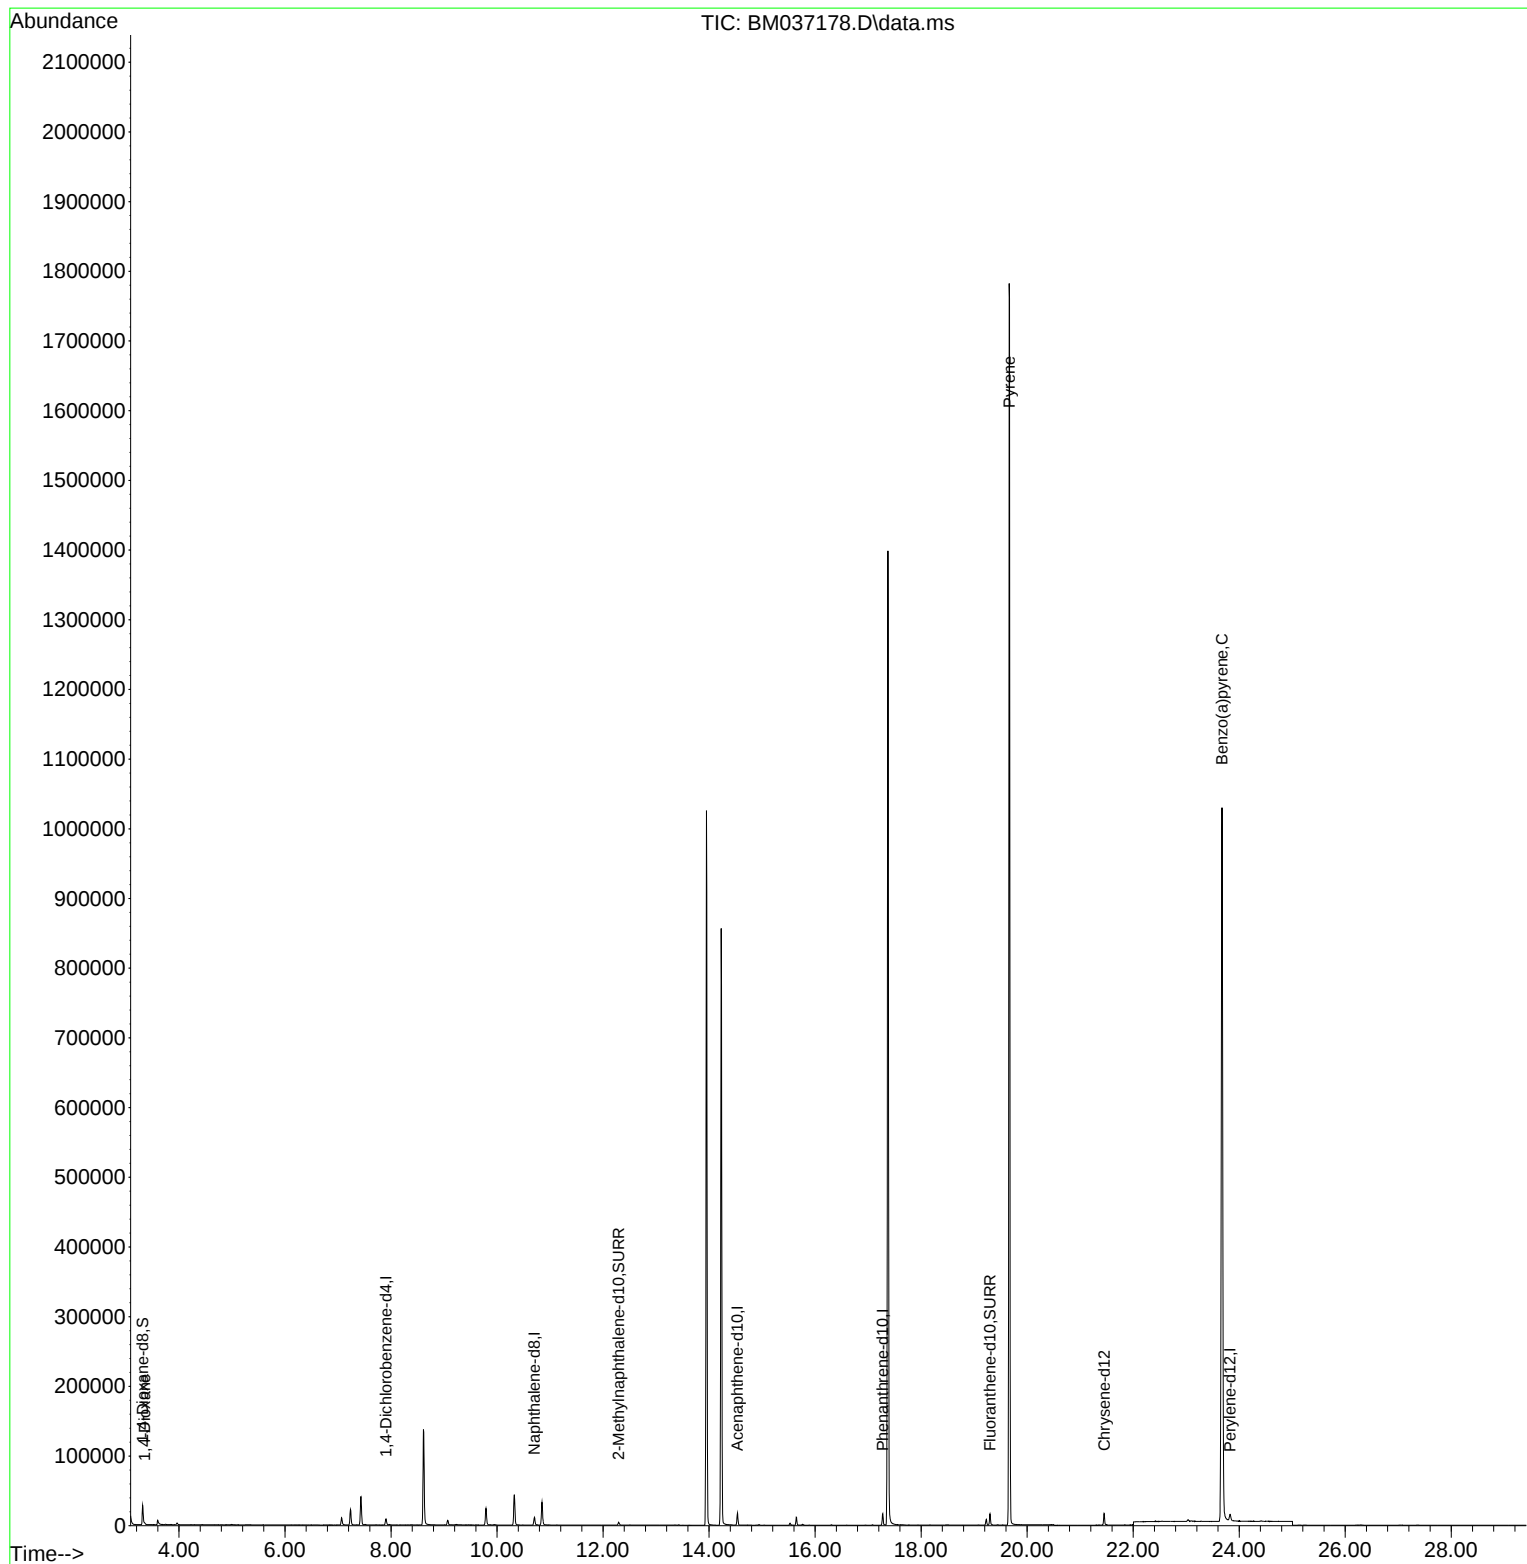


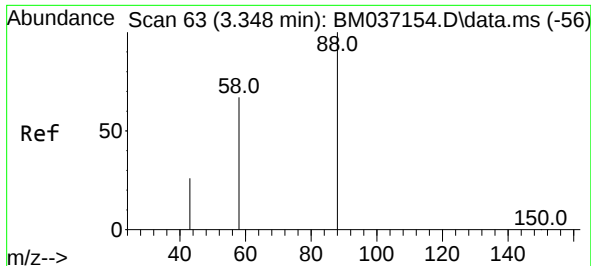

#2
1,4-Dioxane
Concen: 0.181 ng/ul
RT: 3.352 min Scan# 64
Delta R.T. -0.004 min
Lab File: BM037178.D
Acq: 21 Oct 2022 17:36




Instrument :
BNA_N
ClientSampleId :
C0BX2


Tgt Ion: 88 Resp: 1074
Ion Ratio Lower Upper
88 100
43 62.4 25.5 38.3#
58 60.0 45.8 68.6

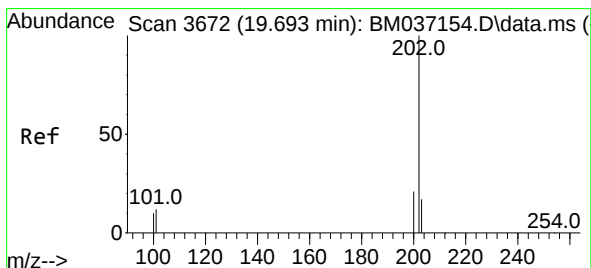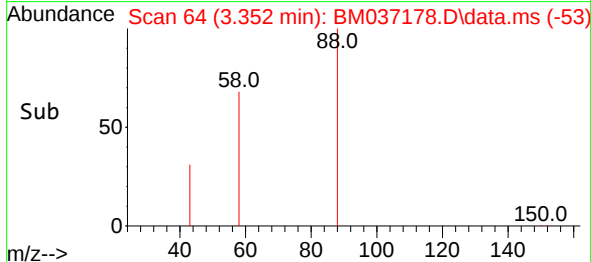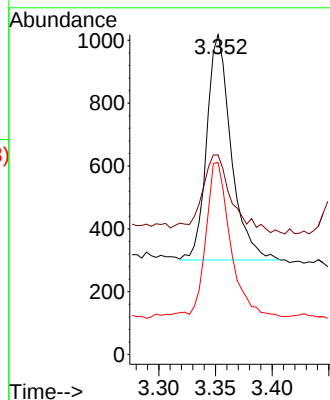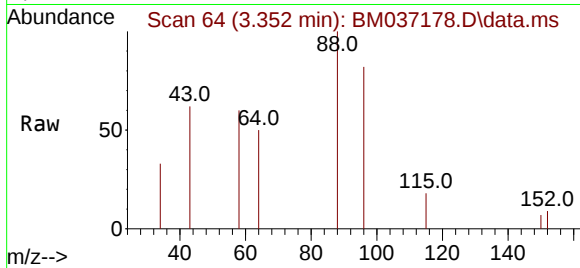

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.661 min Scan# 3665
Delta R.T. -0.037 min
Lab File: BM037178.D
Acq: 21 Oct 2022 17:36


Tgt Ion: 202 Resp: 3374
Ion Ratio Lower Upper
202 100
101 145.8 9.7 14.5#
100 1108.4 7.8 11.8#

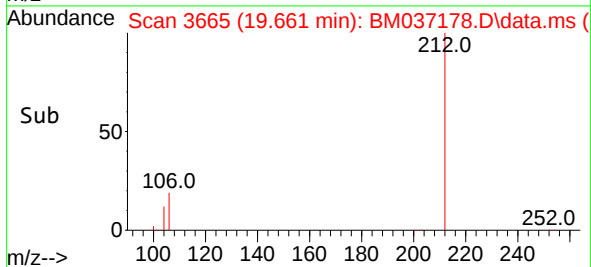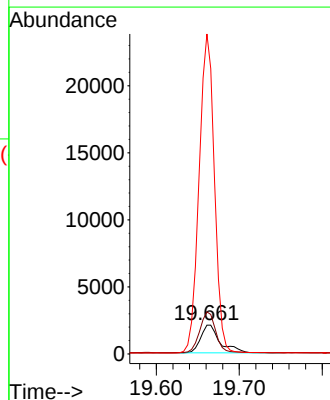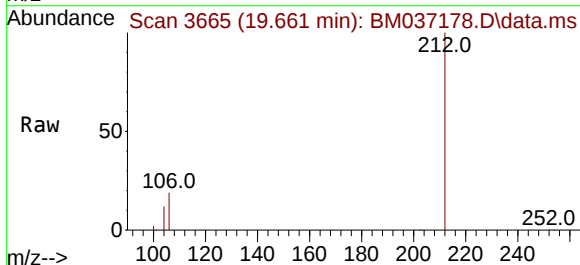

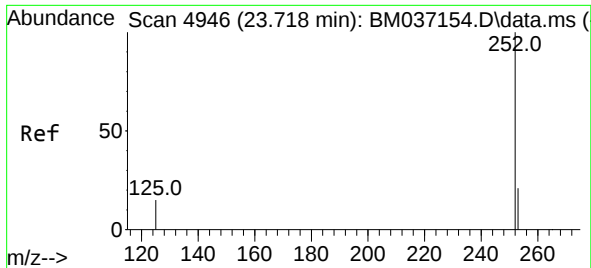

#26
Benzo(a)pyrene
Concen: 0.103 ng/ul
RT: 23.672 min Scan# 4946
Delta R.T. -0.058 min
Lab File: BM037178.D
Acq: 21 Oct 2022 17:36

Instrument :
BNA_N
ClientSampleId :
C0BX2

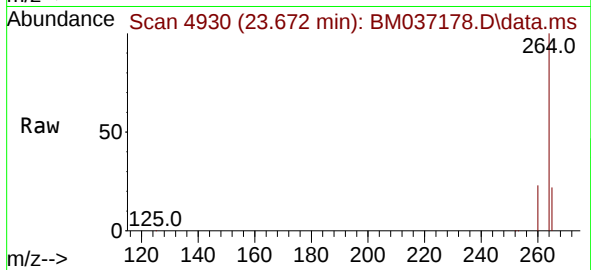

Tgt Ion:252 Resp: 6046
Ion Ratio Lower Upper
252 100
253 46.1 22.1 33.1#
125 42.9 17.6 26.4#

