

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
 Data File : BN022247.D
 Acq On : 21 Oct 2022 10:42
 Operator : CG/JU
 Sample : PB148368BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK368

Quant Time: Oct 21 22:37:50 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.944	152	4150	0.400	ng/ul	0.00
4) Naphthalene-d8	10.772	136	13656	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.619	164	7897	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.374	188	16632	0.400	ng/ul	0.00
17) Chrysene-d12	21.576	240	12587	0.400	ng/ul	0.00
23) Perylene-d12	24.035	264	11189	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.253	96	30428	5.642	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.367	152	6489	0.314	ng/ul	0.00
18) Fluoranthene-d10	19.407	212	13600	0.322	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.613	166	2078	0.060	ng/ul#	15
20) Pyrene	19.775	202	1885	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.877	252	3678	0.082	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
Data File : BN022247.D
Acq On : 21 Oct 2022 10:42
Operator : CG/JU
Sample : PB148368BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK368

Quant Time: Oct 21 22:37:50 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration




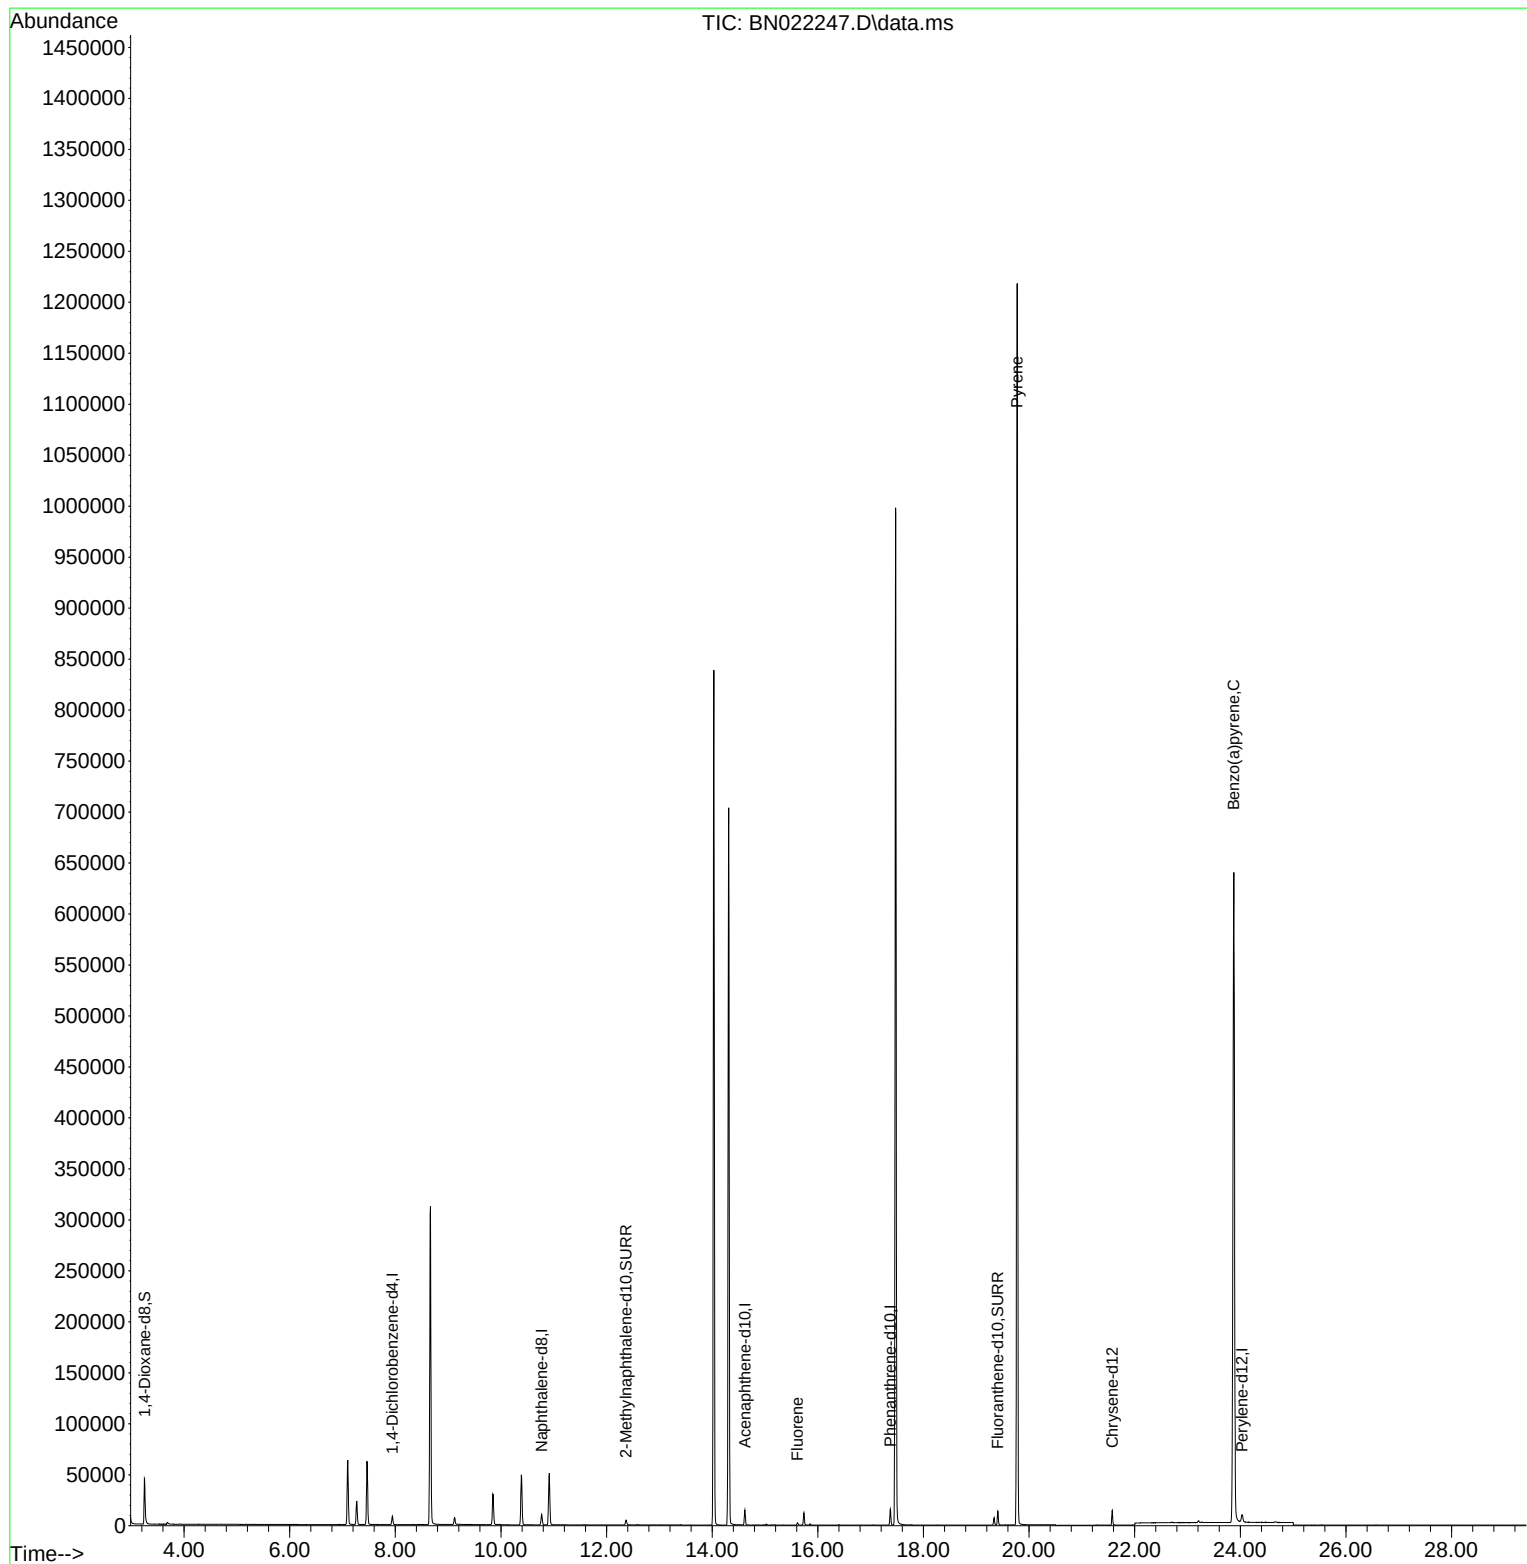


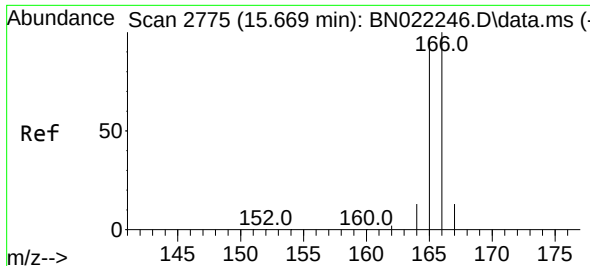

#12
Fluorene
Concen: 0.060 ng/ul
RT: 15.613 min Scan# 21
Delta R.T. -0.063 min
Lab File: BN022247.D
Acq: 21 Oct 2022 10:42




Instrument :
BNA_N
ClientSampleId :
SBLK368


Tgt Ion:166 Resp: 2078
Ion Ratio Lower Upper
166 100
165 8.3 78.2 117.2#
167 32.8 11.0 16.4#

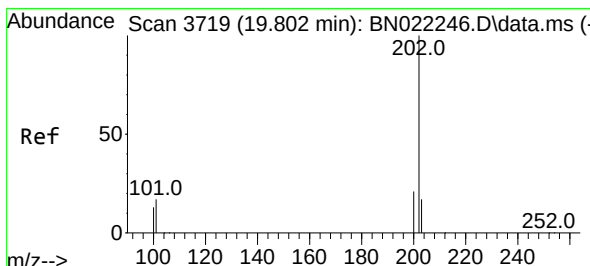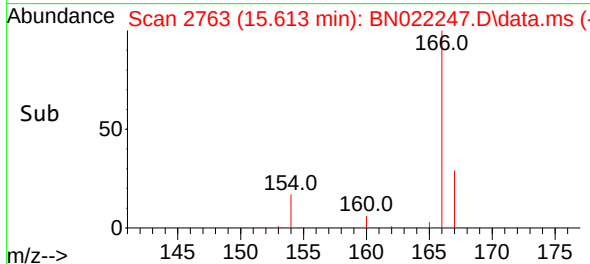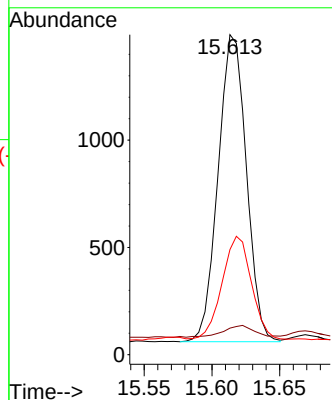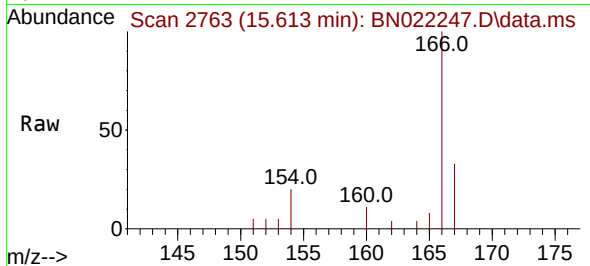

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.775 min Scan# 3713
Delta R.T. -0.036 min
Lab File: BN022247.D
Acq: 21 Oct 2022 10:42


Tgt Ion:202 Resp: 1885
Ion Ratio Lower Upper
202 100
101 178.1 13.1 19.7#
100 1319.7 10.6 16.0#

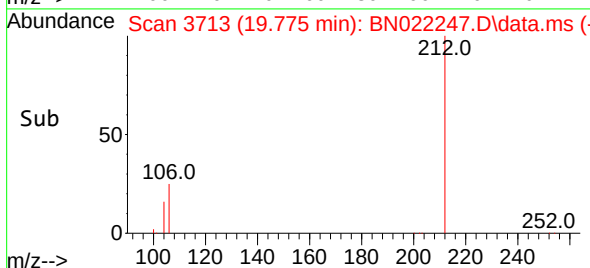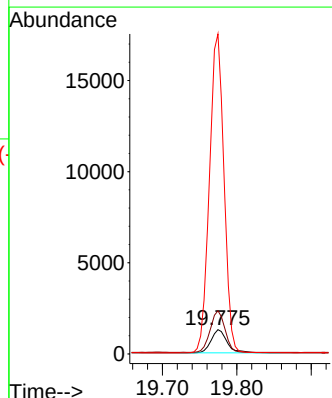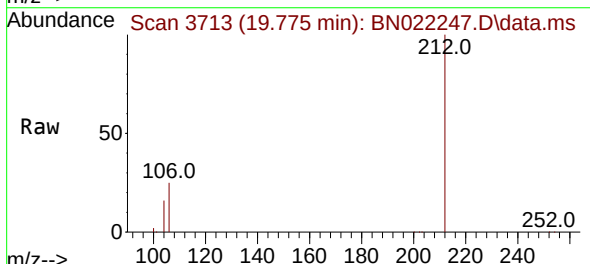

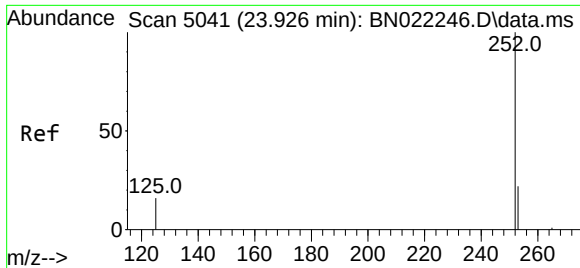

#26
 Benzo(a)pyrene
 Concen: 0.082 ng/ul
 RT: 23.877 min Scan# 50
 Delta R.T. -0.059 min
 Lab File: BN022247.D
 Acq: 21 Oct 2022 10:42

Instrument :
 BNA_N
 ClientSampleId :
 SBLK368

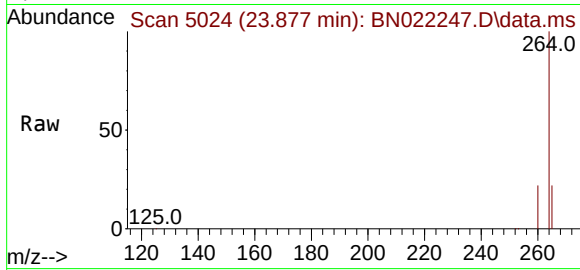

Tgt Ion:252 Resp: 3678

Ion	Ratio	Lower	Upper
252	100		
253	44.4	21.0	31.6#
125	45.1	17.9	26.9#

