

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
 Data File : BN022250.D
 Acq On : 21 Oct 2022 12:33
 Operator : CG/JU
 Sample : N5015-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BG2

Quant Time: Oct 21 22:38:38 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.944	152	3941	0.400	ng/ul	0.00
4) Naphthalene-d8	10.772	136	13857	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.619	164	8109	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.374	188	16944	0.400	ng/ul	0.00
17) Chrysene-d12	21.576	240	11349	0.400	ng/ul	0.00
23) Perylene-d12	24.037	264	8526	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.249	96	32211	6.289	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.373	152	8609	0.411	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	17875	0.469	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.287	88	412	0.078	ng/ul#	8
19) Fluoranthene	19.440	202	1349	0.026	ng/ul#	77
26) Benzo(a)pyrene	23.880	252	3375	0.099	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
Data File : BN022250.D
Acq On : 21 Oct 2022 12:33
Operator : CG/JU
Sample : N5015-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BG2

Quant Time: Oct 21 22:38:38 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration




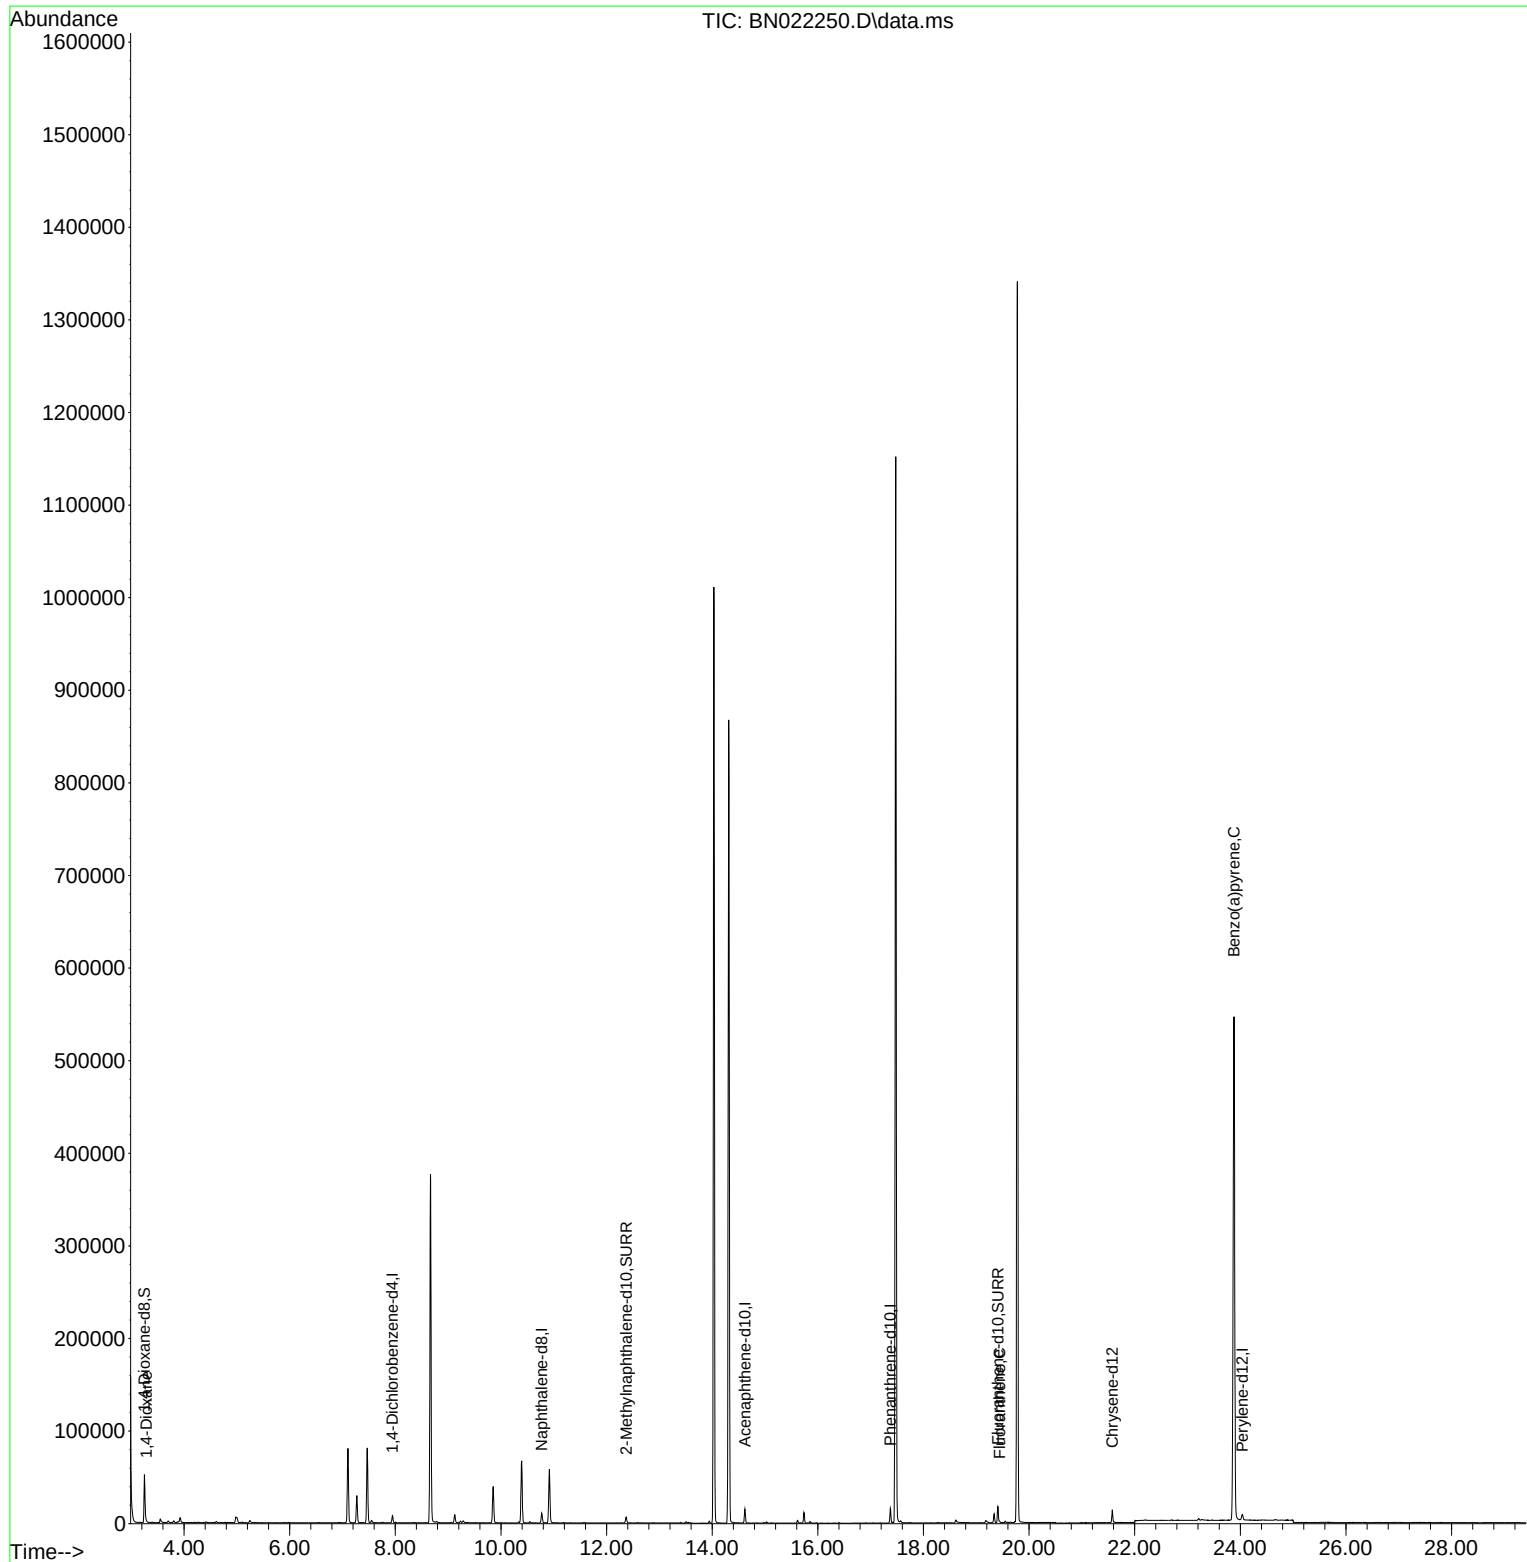


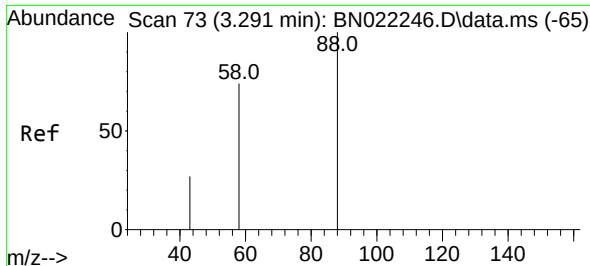

#2
 1,4-Dioxane
 Concen: 0.078 ng/ul
 RT: 3.287 min Scan# 71
 Delta R.T. -0.008 min
 Lab File: BN022250.D
 Acq: 21 Oct 2022 12:33




Instrument :
 BNA_N
 ClientSampleId :
 C1BG2


Tgt Ion: 88 Resp: 412
 Ion Ratio Lower Upper
 88 100
 43 167.2 27.4 41.2#
 58 51.1 48.2 72.2

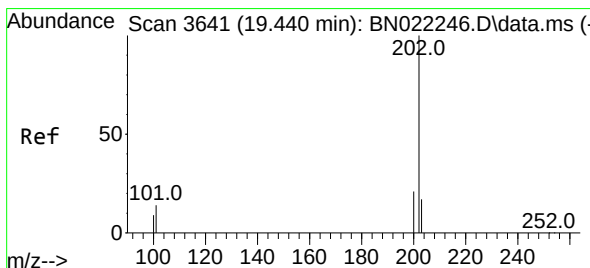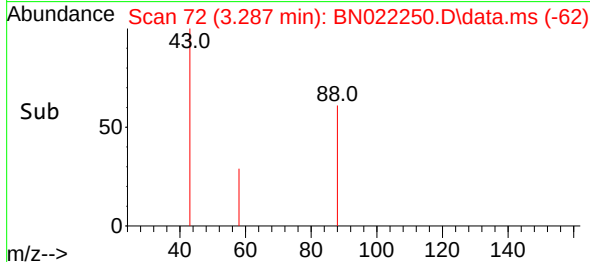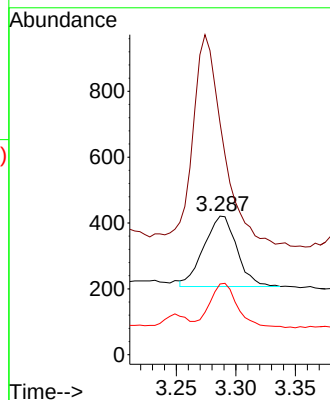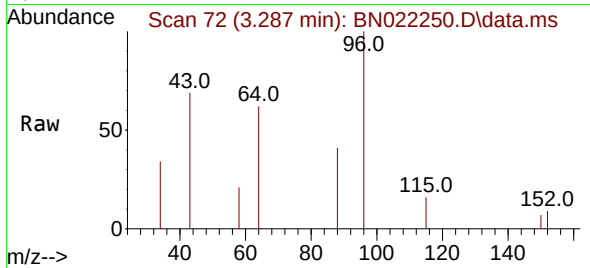

#19
 Fluoranthene
 Concen: 0.026 ng/ul
 RT: 19.440 min Scan# 3641
 Delta R.T. -0.003 min
 Lab File: BN022250.D
 Acq: 21 Oct 2022 12:33

Tgt Ion: 202 Resp: 1349
 Ion Ratio Lower Upper
 202 100
 101 24.6 11.8 17.6#
 100 19.1 8.7 13.1#

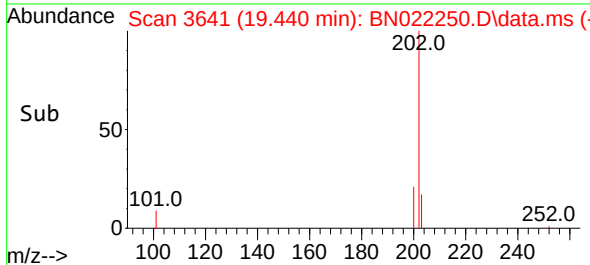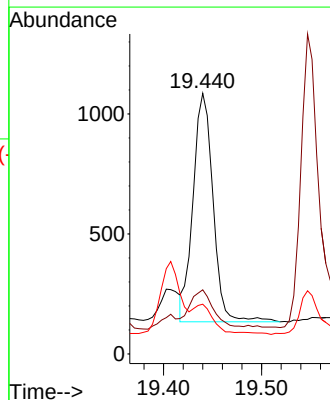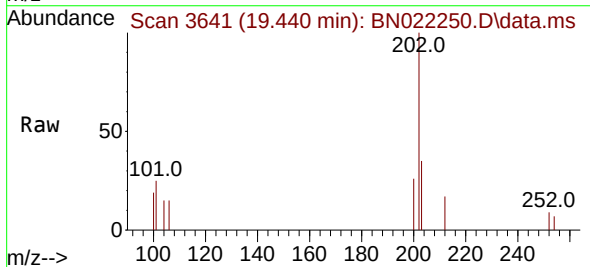

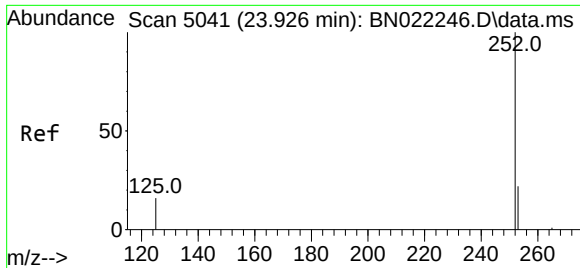

#26

Benzo(a)pyrene

Concen: 0.099 ng/ul

RT: 23.880 min Scan# 50

Delta R.T. -0.056 min

Lab File: BN022250.D


Acq: 21 Oct 2022 12:33

Instrument :

BNA_N

ClientSampleId :

C1BG2

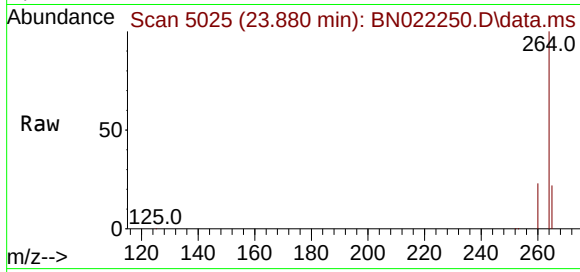

Tgt Ion:252 Resp: 3375

Ion Ratio Lower Upper

252 100

253 49.9 21.0 31.6#

125 65.7 17.9 26.9#

