

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
 Data File : BN022252.D
 Acq On : 21 Oct 2022 13:47
 Operator : CG/JU
 Sample : N5015-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1BF9

Quant Time: Oct 21 22:39:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.949	152	3995	0.400	ng/ul	0.00
4) Naphthalene-d8	10.772	136	13893	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.623	164	8134	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.378	188	17009	0.400	ng/ul	0.00
17) Chrysene-d12	21.576	240	11757	0.400	ng/ul	# 0.00
23) Perylene-d12	24.034	264	8691	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.249	96	29870	5.753	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.373	152	7889	0.375	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	16658	0.422	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.287	88	215	0.040	ng/ul#	1
20) Pyrene	19.779	202	2428	0.045	ng/ul#	1
26) Benzo(a)pyrene	23.877	252	3129	0.090	ng/ul#	37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
Data File : BN022252.D
Acq On : 21 Oct 2022 13:47
Operator : CG/JU
Sample : N5015-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1BF9


Quant Time: Oct 21 22:39:10 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration

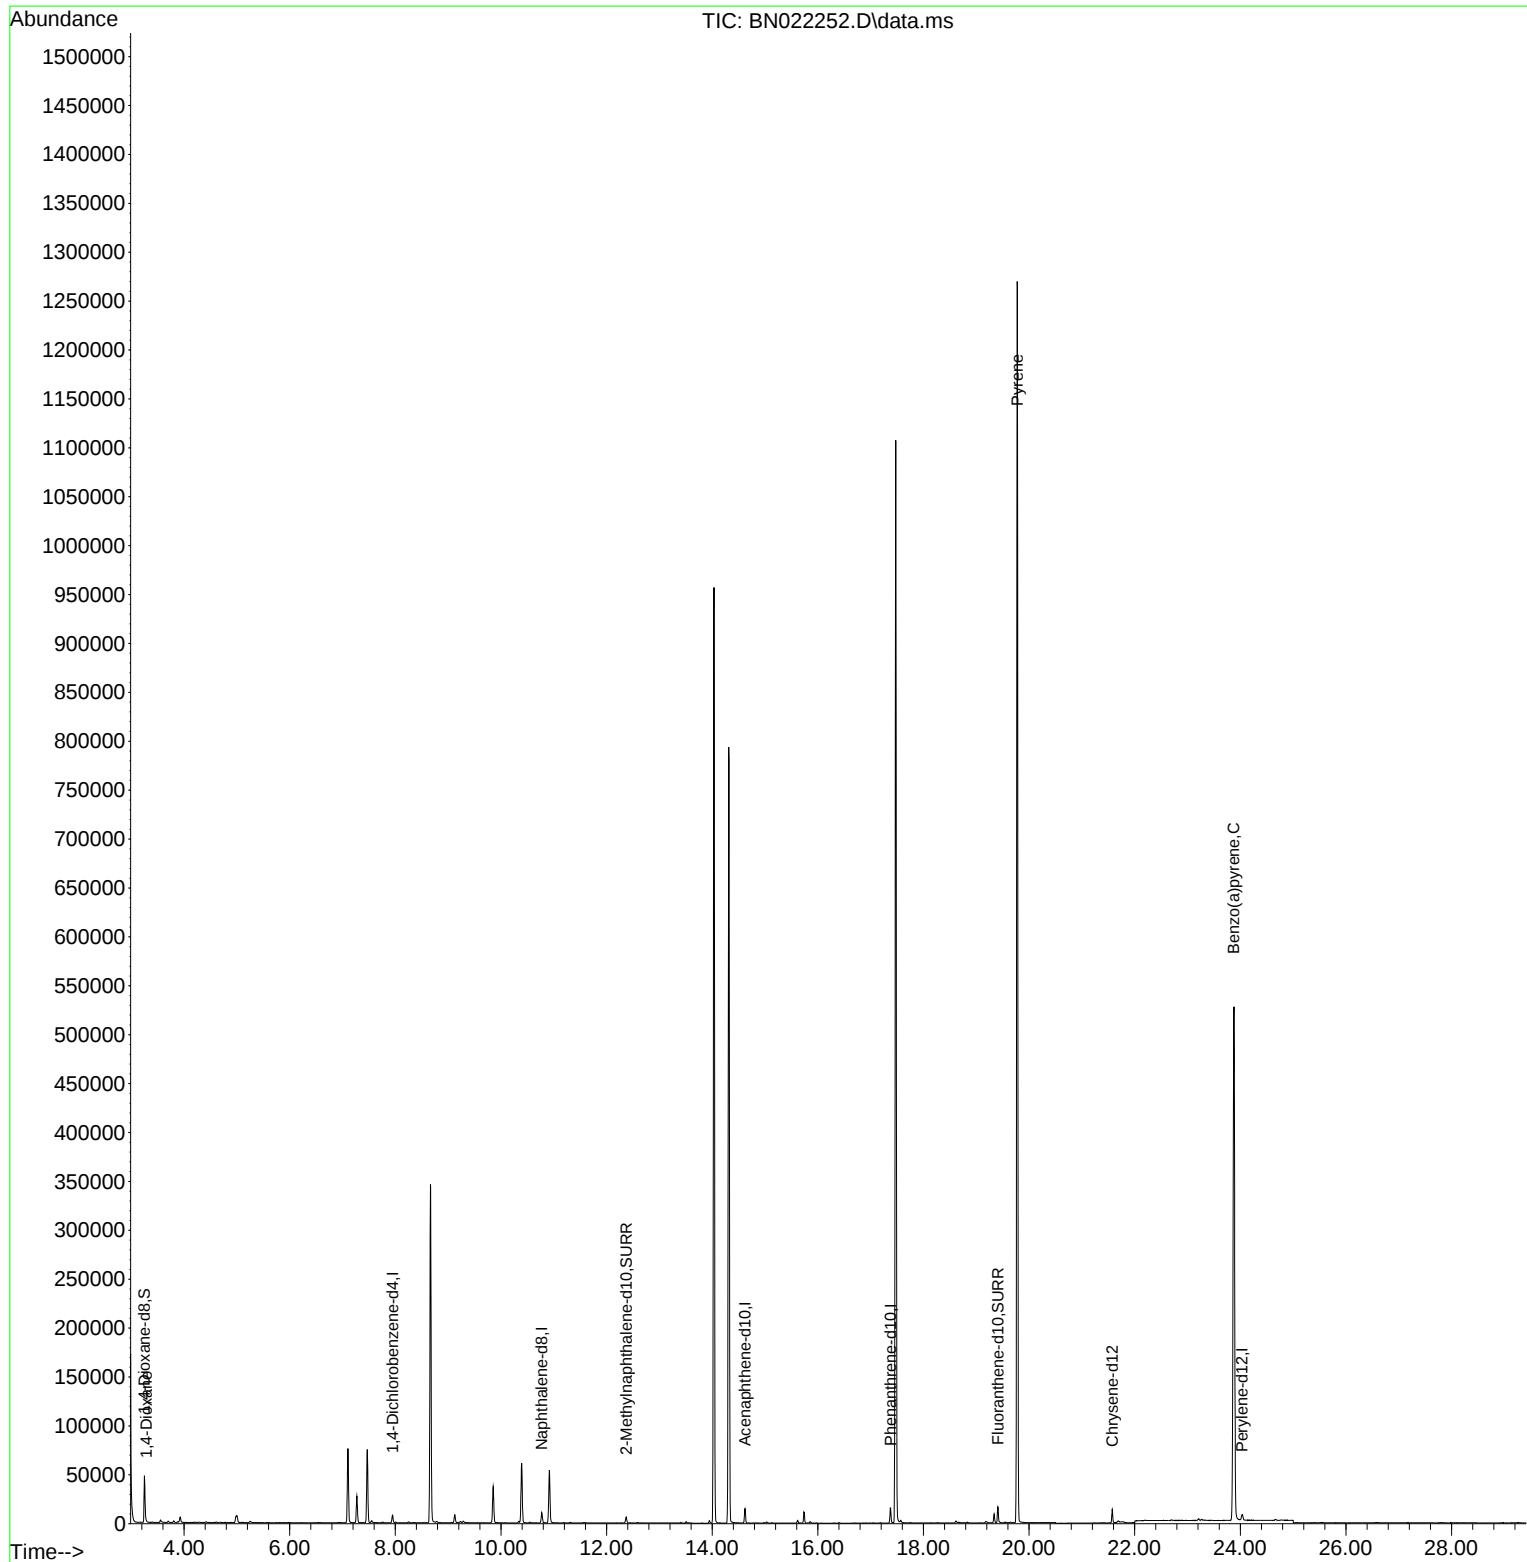



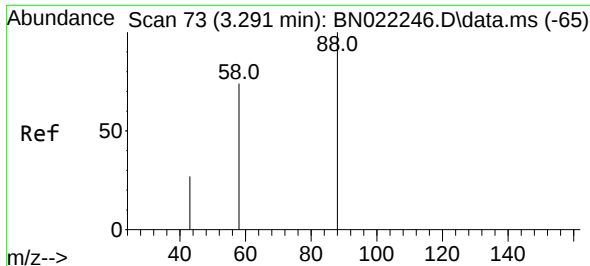


#2
1,4-Dioxane
Concen: 0.040 ng/ul
RT: 3.287 min Scan# 71
Delta R.T. -0.009 min
Lab File: BN022252.D
Acq: 21 Oct 2022 13:47

Instrument :
BNA_N
ClientSampleId :
C1BF9



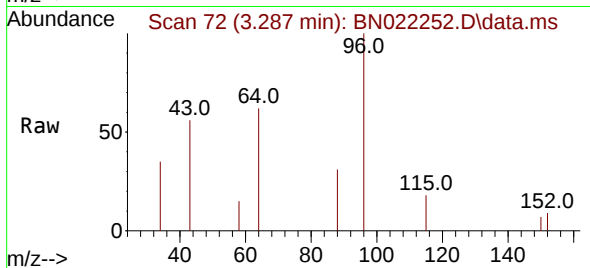



Tgt Ion: 88 Resp: 215
Ion Ratio Lower Upper
88 100
43 183.4 27.4 41.2#
58 47.8 48.2 72.2#

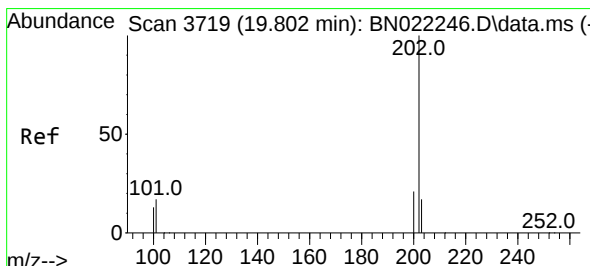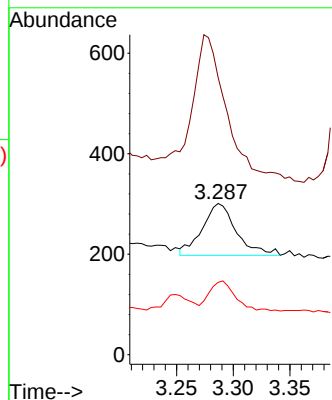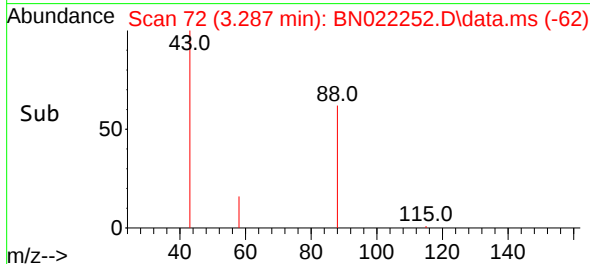

#20
Pyrene
Concen: 0.045 ng/ul
RT: 19.779 min Scan# 3714
Delta R.T. -0.031 min
Lab File: BN022252.D
Acq: 21 Oct 2022 13:47


Tgt Ion: 202 Resp: 2428
Ion Ratio Lower Upper
202 100
101 168.0 13.1 19.7#
100 1171.2 10.6 16.0#

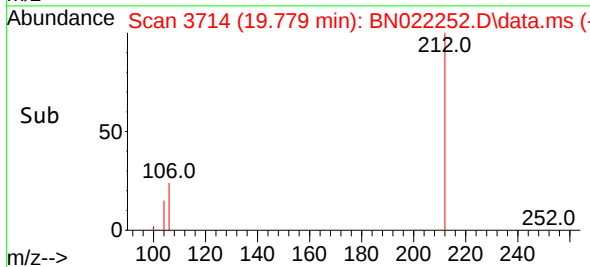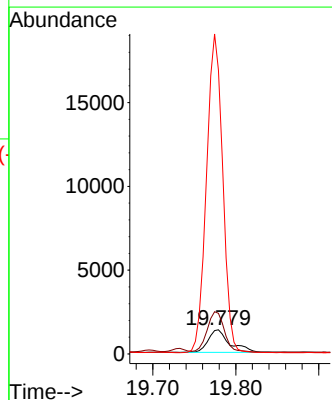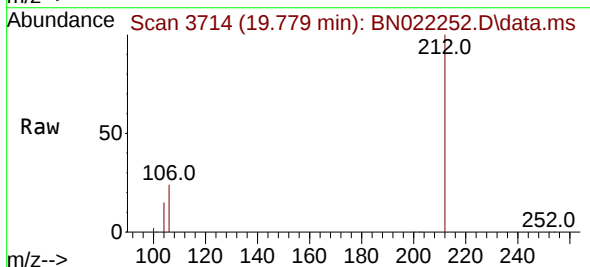

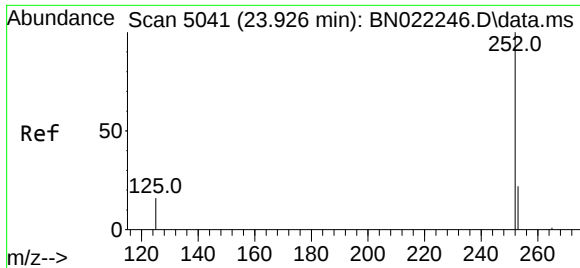

#26
Benzo(a)pyrene
Concen: 0.090 ng/ul
RT: 23.877 min Scan# 50
Delta R.T. -0.059 min
Lab File: BN022252.D
Acq: 21 Oct 2022 13:47

Instrument :
BNA_N
ClientSampleId :
C1BF9

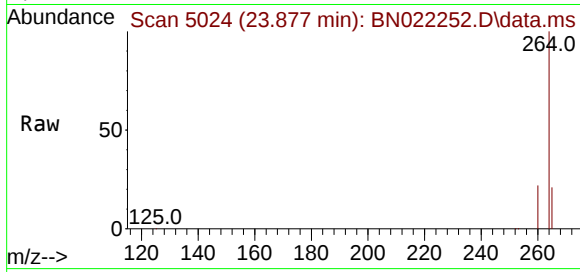

Tgt Ion:	252	Resp:	3129
Ion Ratio	Lower	Upper	
252	100		
253	49.6	21.0	31.6#
125	62.3	17.9	26.9#

