

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
 Data File : BN022257.D
 Acq On : 21 Oct 2022 16:54
 Operator : CG/JU
 Sample : PB148372BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK372

Quant Time: Oct 21 22:40:32 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.948	152	4797	0.400	ng/ul	0.00
4) Naphthalene-d8	10.778	136	15380	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.623	164	7915	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.378	188	14216	0.400	ng/ul	0.00
17) Chrysene-d12	21.582	240	9191	0.400	ng/ul	0.00
23) Perylene-d12	24.040	264	9069	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.253	96	32522	5.217	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.372	152	6553	0.282	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	9989	0.324	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.618	166	1900	0.055	ng/ul#	15
20) Pyrene	19.779	202	1422	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.879	252	2760	0.076	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
Data File : BN022257.D
Acq On : 21 Oct 2022 16:54
Operator : CG/JU
Sample : PB148372BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK372

Quant Time: Oct 21 22:40:32 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration




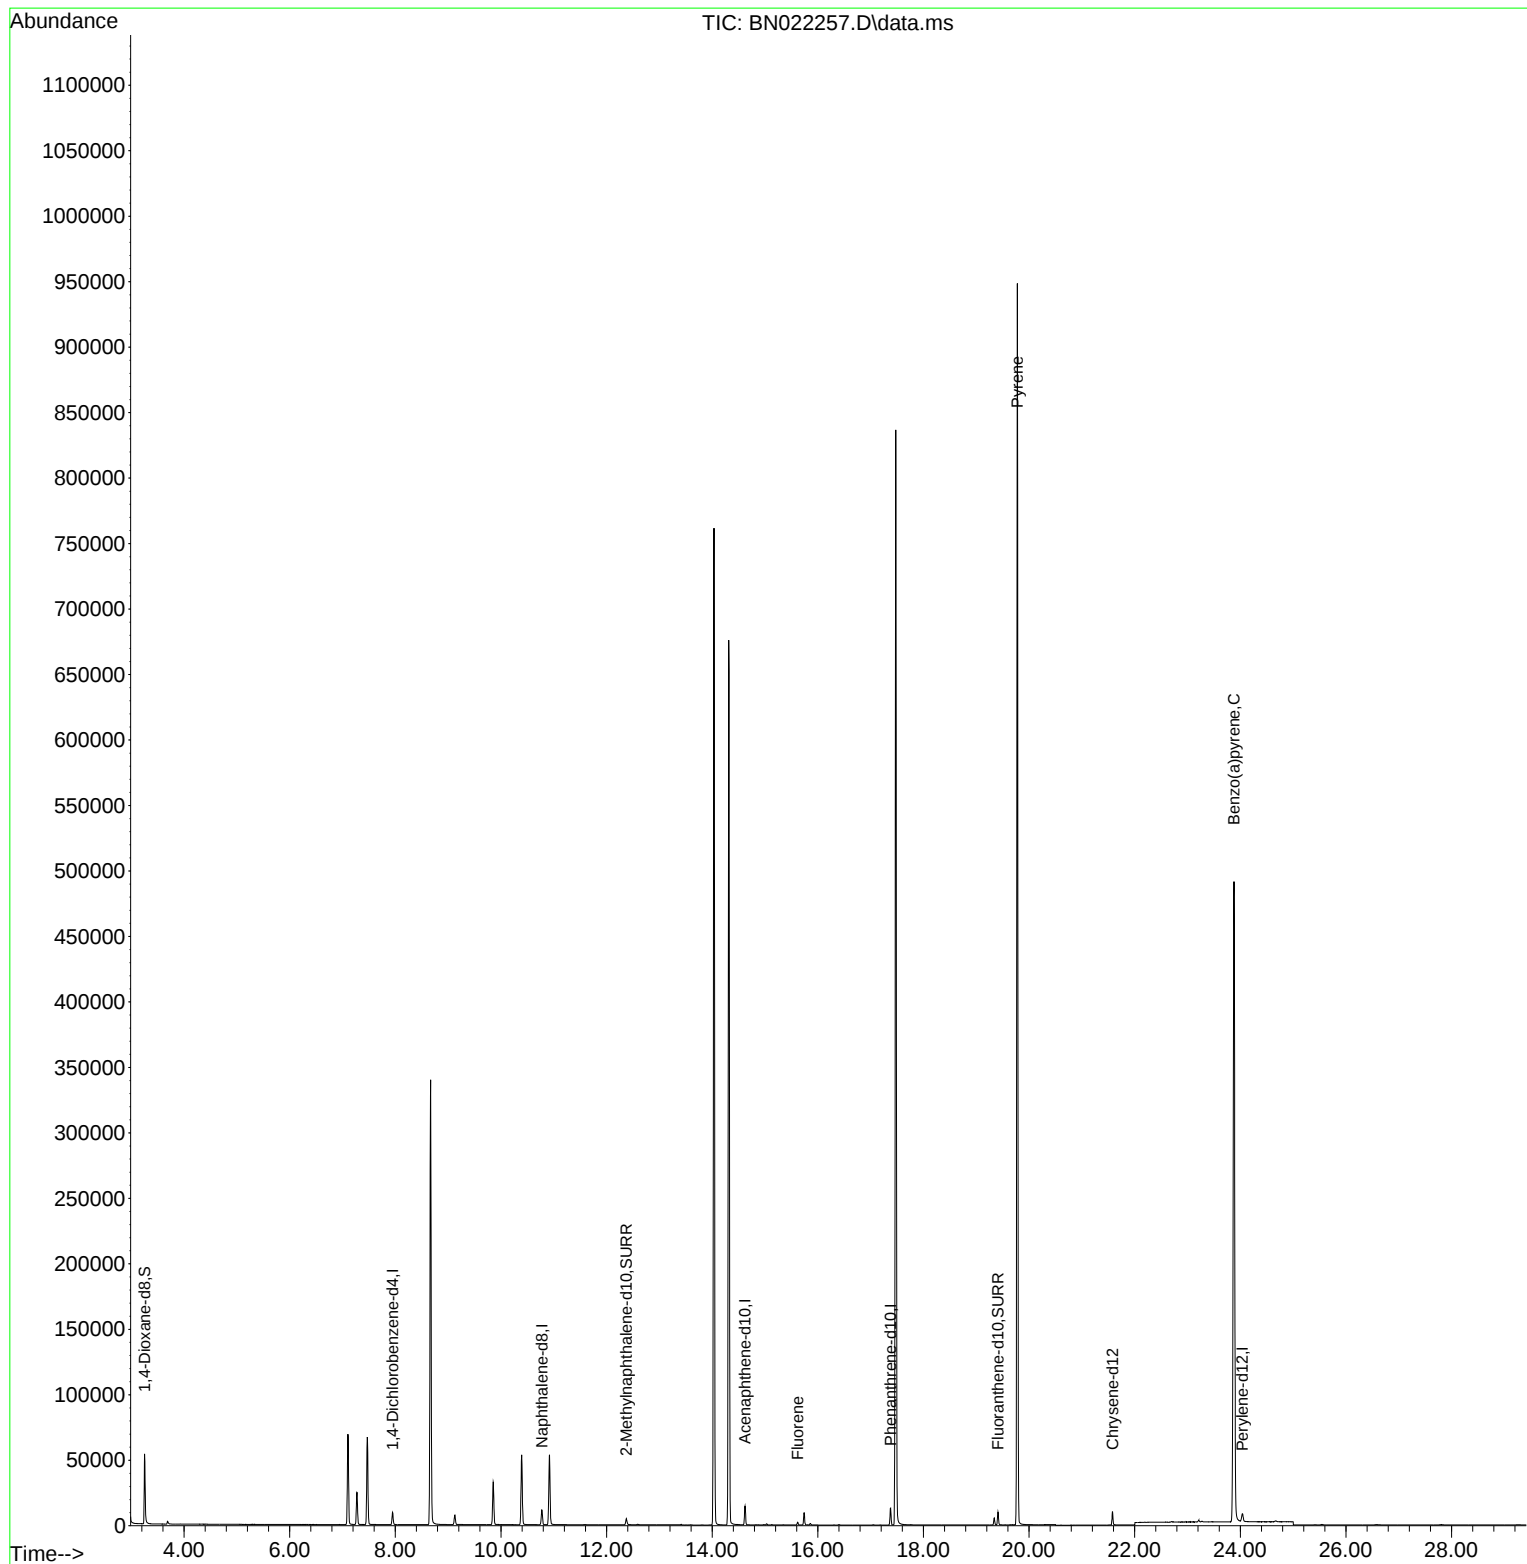


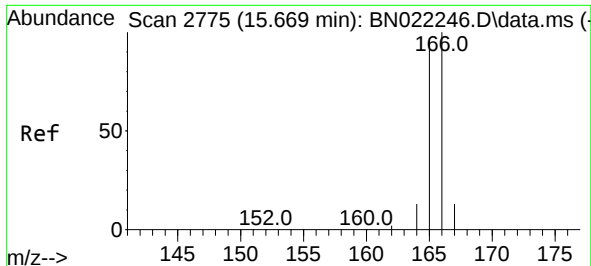

#12
Fluorene
Concen: 0.055 ng/ul
RT: 15.618 min Scan# 21
Delta R.T. -0.059 min
Lab File: BN022257.D
Acq: 21 Oct 2022 16:54




Instrument :
BNA_N
ClientSampleId :
SBLK372


Tgt Ion:166 Resp: 1900
Ion Ratio Lower Upper
166 100
165 8.3 78.2 117.2#
167 32.8 11.0 16.4#

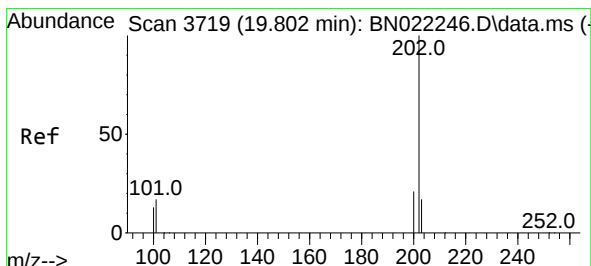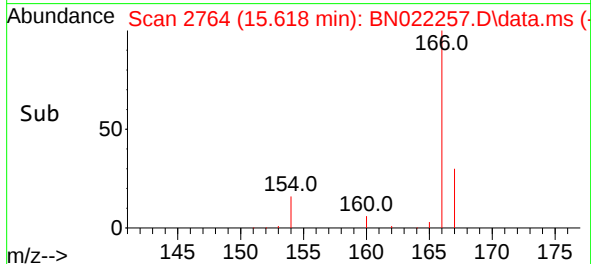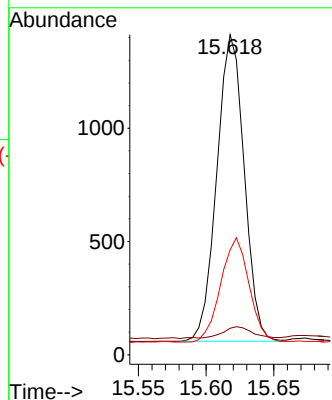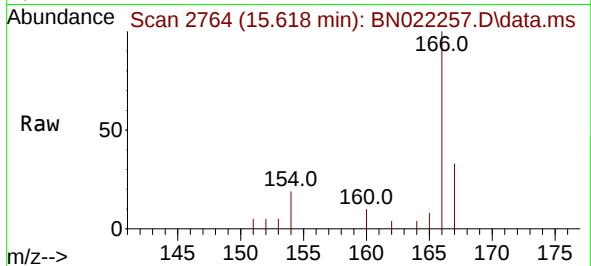

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.779 min Scan# 3714
Delta R.T. -0.032 min
Lab File: BN022257.D
Acq: 21 Oct 2022 16:54


Tgt Ion:202 Resp: 1422
Ion Ratio Lower Upper
202 100
101 177.1 13.1 19.7#
100 1265.1 10.6 16.0#

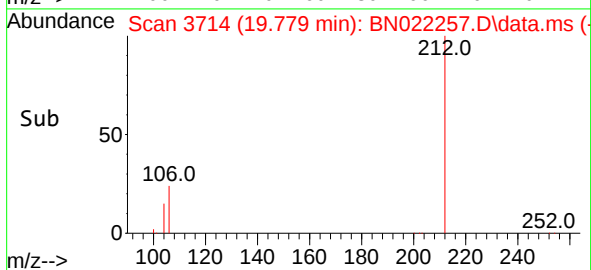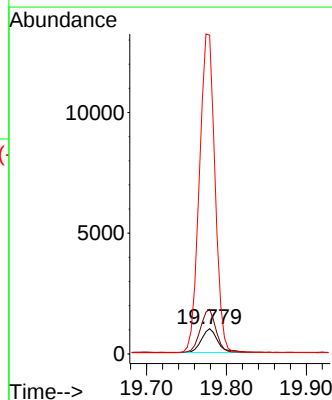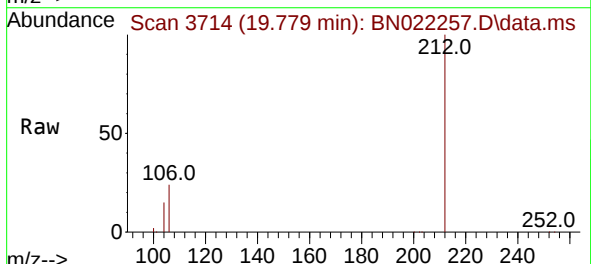

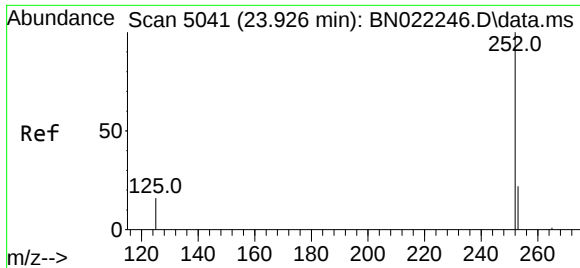

#26
 Benzo(a)pyrene
 Concen: 0.076 ng/ul
 RT: 23.879 min Scan# 50
 Delta R.T. -0.056 min
 Lab File: BN022257.D
 Acq: 21 Oct 2022 16:54

Instrument :
 BNA_N
 ClientSampleId :
 SBLK372

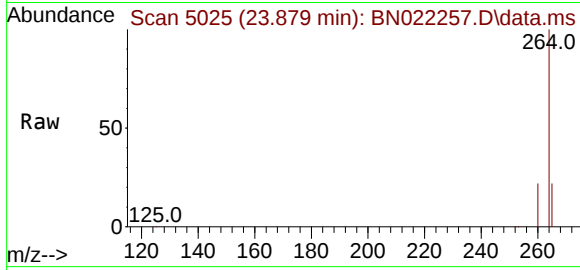

Tgt Ion:252	Resp:	2760
Ion Ratio	Lower	Upper
252	100	
253	47.6	21.0 31.6#
125	52.2	17.9 26.9#

