




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
 Data File : BN022284.D
 Acq On : 22 Oct 2022 10:03
 Operator : CG/JU
 Sample : N5064-10DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BP6DL

Manual IntegrationsAPPROVED

Quant Time: Oct 22 12:15:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 22 03:40:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

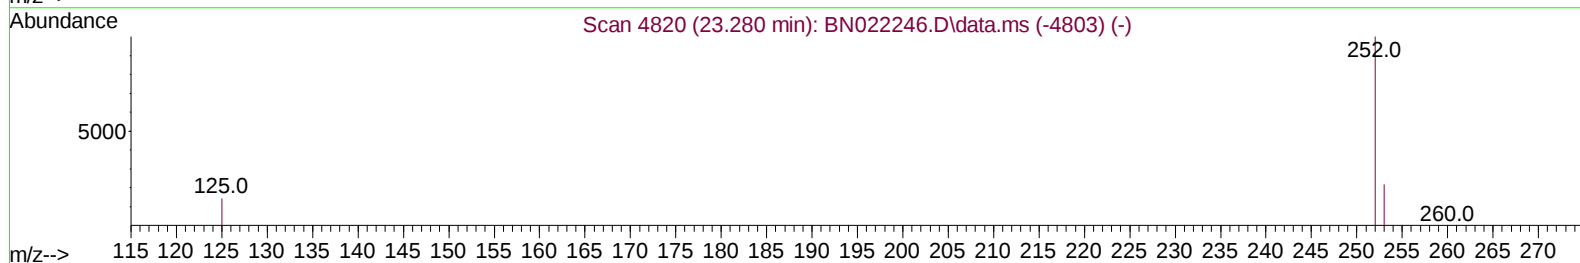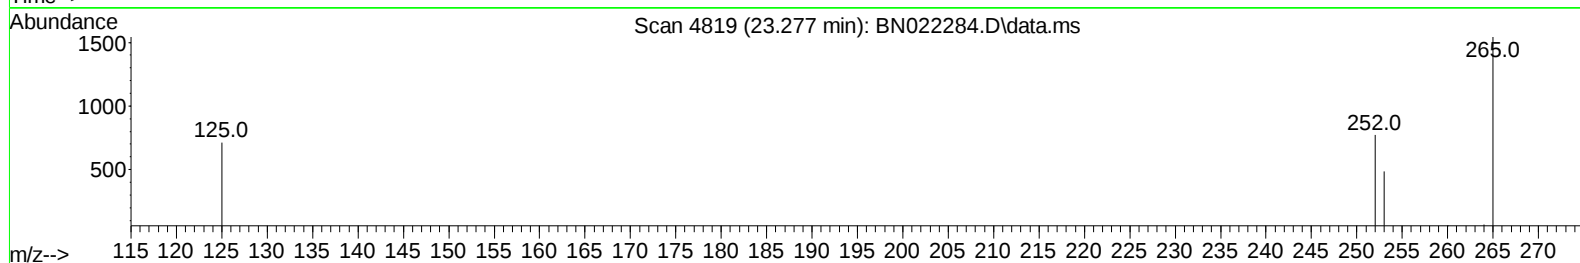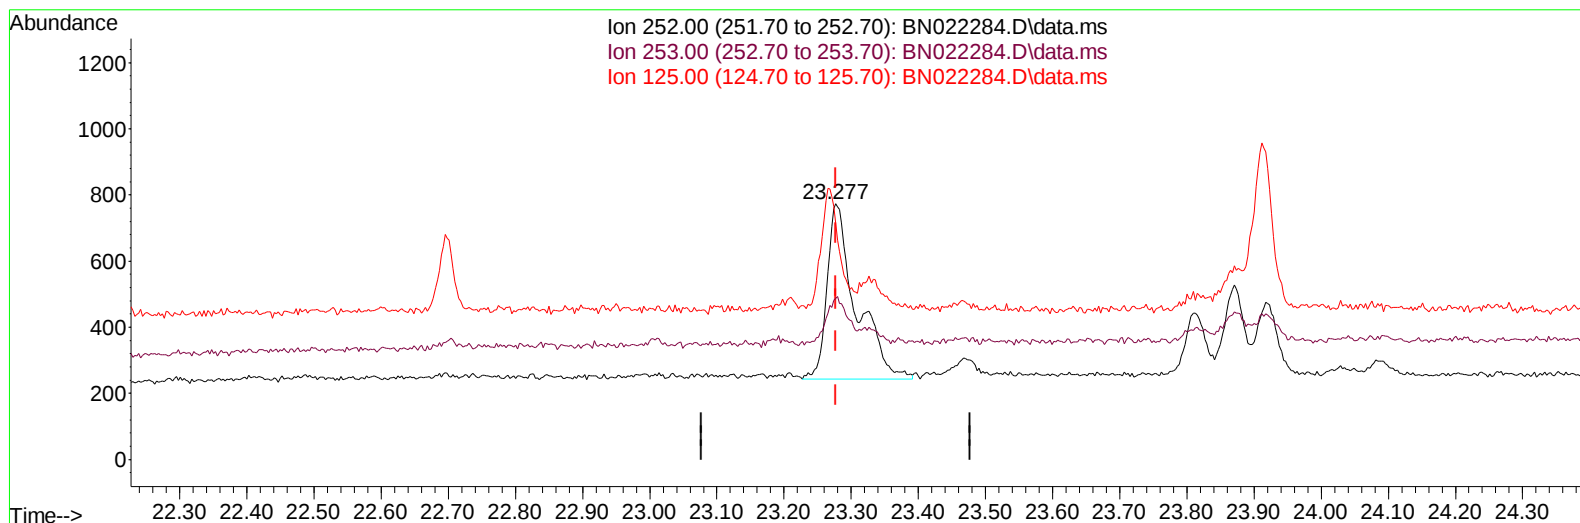

TIC: BN022284.D\data.ms

(24) Benzo(b)fluoranthene

23.277min (-0.000) 0.04 ng/u1

response 1603

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	24.50	62.92#
125.00	17.60	92.38#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
 Data File : BN022284.D
 Acq On : 22 Oct 2022 10:03
 Operator : CG/JU
 Sample : N5064-10DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BP6DL

Manual IntegrationsAPPROVED

Quant Time: Oct 22 12:15:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 22 03:40:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

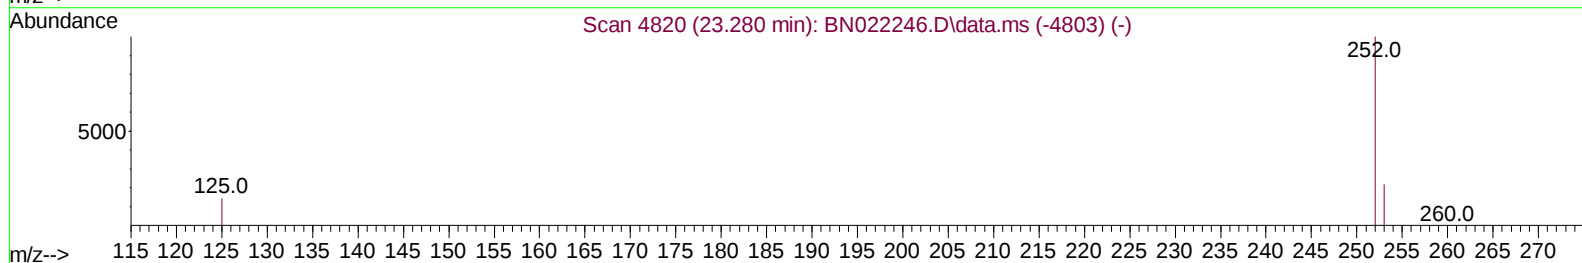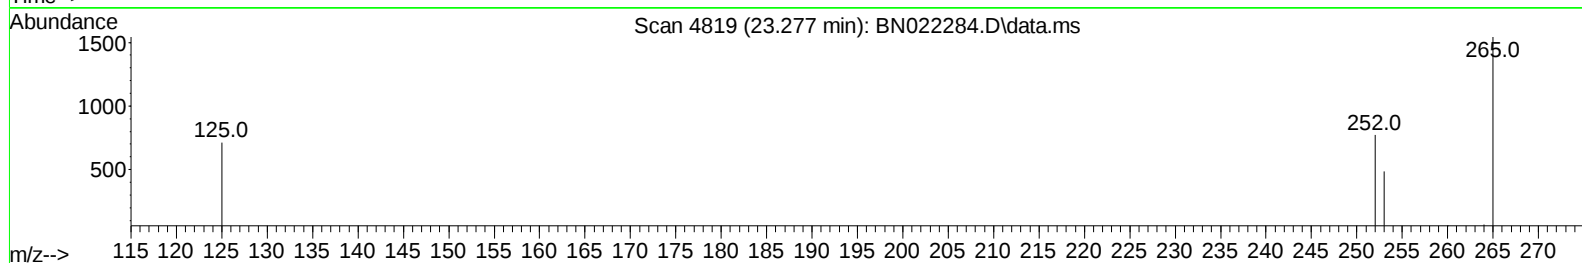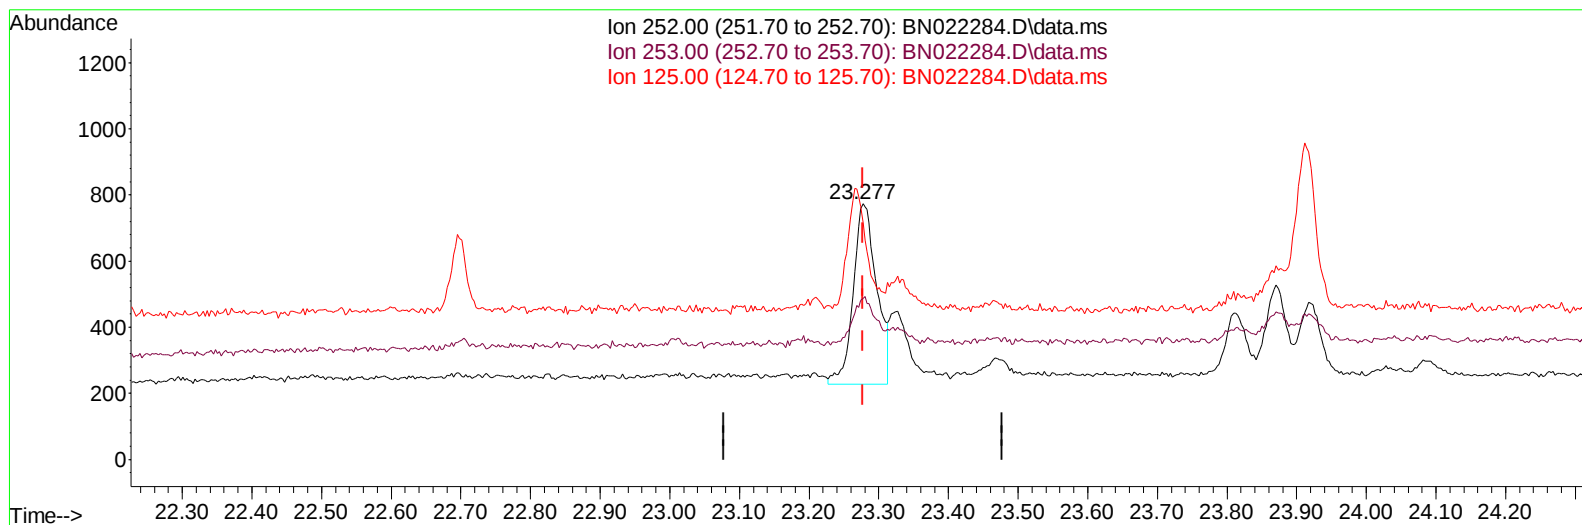

TIC: BN022284.D\data.ms

(24) Benzo(b)fluoranthene

23.277min (-0.000) 0.03 ng/u1 m

response 1278

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	24.50	62.92#
125.00	17.60	92.38#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
 Data File : BN022284.D
 Acq On : 22 Oct 2022 10:03
 Operator : CG/JU
 Sample : N5064-10DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BP6DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

Quant Time: Oct 22 12:15:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 22 03:40:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.944	152	5219	0.400	ng/ul	0.00
4) Naphthalene-d8	10.772	136	17167	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.618	164	8667	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.374	188	14855	0.400	ng/ul	0.00
17) Chrysene-d12	21.576	240	9608	0.400	ng/ul	0.00
23) Perylene-d12	24.031	264	8885	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.253	96	5978	0.881	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.373	152	1367	0.053	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	1955	0.061	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.416	178	2270	0.046	ng/ul#	93
19) Fluoranthene	19.440	202	2235	0.051	ng/ul	95
22) Chrysene	21.614	228	1033	0.027	ng/ul#	83
24) Benzo(b)fluoranthene	23.277	252	1278m	0.029	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
Data File : BN022284.D
Acq On : 22 Oct 2022 10:03
Operator : CG/JU
Sample : N5064-10DL 5X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BP6DL

Manual IntegrationsAPPROVED

Quant Time: Oct 22 12:15:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 22 03:40:14 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

