

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
 Data File : BN022265.D
 Acq On : 21 Oct 2022 21:54
 Operator : CG/JU
 Sample : N5064-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COBM3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

Quant Time: Oct 21 22:42:50 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 23:32:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.948	152	4329	0.400	ng/ul	0.00
4) Naphthalene-d8	10.771	136	14790	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.622	164	8405	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.377	188	16714	0.400	ng/ul	0.00
17) Chrysene-d12	21.576	240	9549	0.400	ng/ul	0.00
23) Perylene-d12	24.035	264	7694	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.253	96	23304	4.142	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.371	152	6221	0.278	ng/ul	0.00
18) Fluoranthene-d10	19.411	212	11550	0.360	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.820	128	13034	0.298	ng/ul	99
7) 2-Methylnaphthalene	12.443	142	10604	0.385	ng/ul	100
8) 1-Methylnaphthalene	12.663	142	9162	0.324	ng/ul	100
10) Acenaphthylene	14.340	152	3063	0.081	ng/ul#	83
11) Acenaphthene	14.682	153	2807	0.088	ng/ul	98
12) Fluorene	15.672	166	2739	0.074	ng/ul#	95
15) Phenanthrene	17.415	178	59355	1.058	ng/ul	99
16) Anthracene	17.508	178	10516	0.222	ng/ul	98
19) Fluoranthene	19.438	202	81355	1.860	ng/ul	100
20) Pyrene	19.806	202	62498m	1.422	ng/ul	
21) Benzo(a)anthracene	21.559	228	27583	0.771	ng/ul	95
22) Chrysene	21.611	228	28854	0.761	ng/ul	96
24) Benzo(b)fluoranthene	23.280	252	32659m	0.845	ng/ul	
25) Benzo(k)fluoranthene	23.324	252	9923m	0.264	ng/ul	
26) Benzo(a)pyrene	23.924	252	19784	0.642	ng/ul	95
27) Indeno(1,2,3-cd)pyrene	26.612	276	15200	0.397	ng/ul#	93
28) Dibenzo(a,h)anthracene	26.625	278	3942	0.129	ng/ul#	62
29) Benzo(g,h,i)perylene	27.413	276	14326	0.459	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102122\
Data File : BN022265.D
Acq On : 21 Oct 2022 21:54
Operator : CG/JU
Sample : N5064-15
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0BM3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022


Quant Time: Oct 21 22:42:50 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 23:32:34 2022
Response via : Initial Calibration

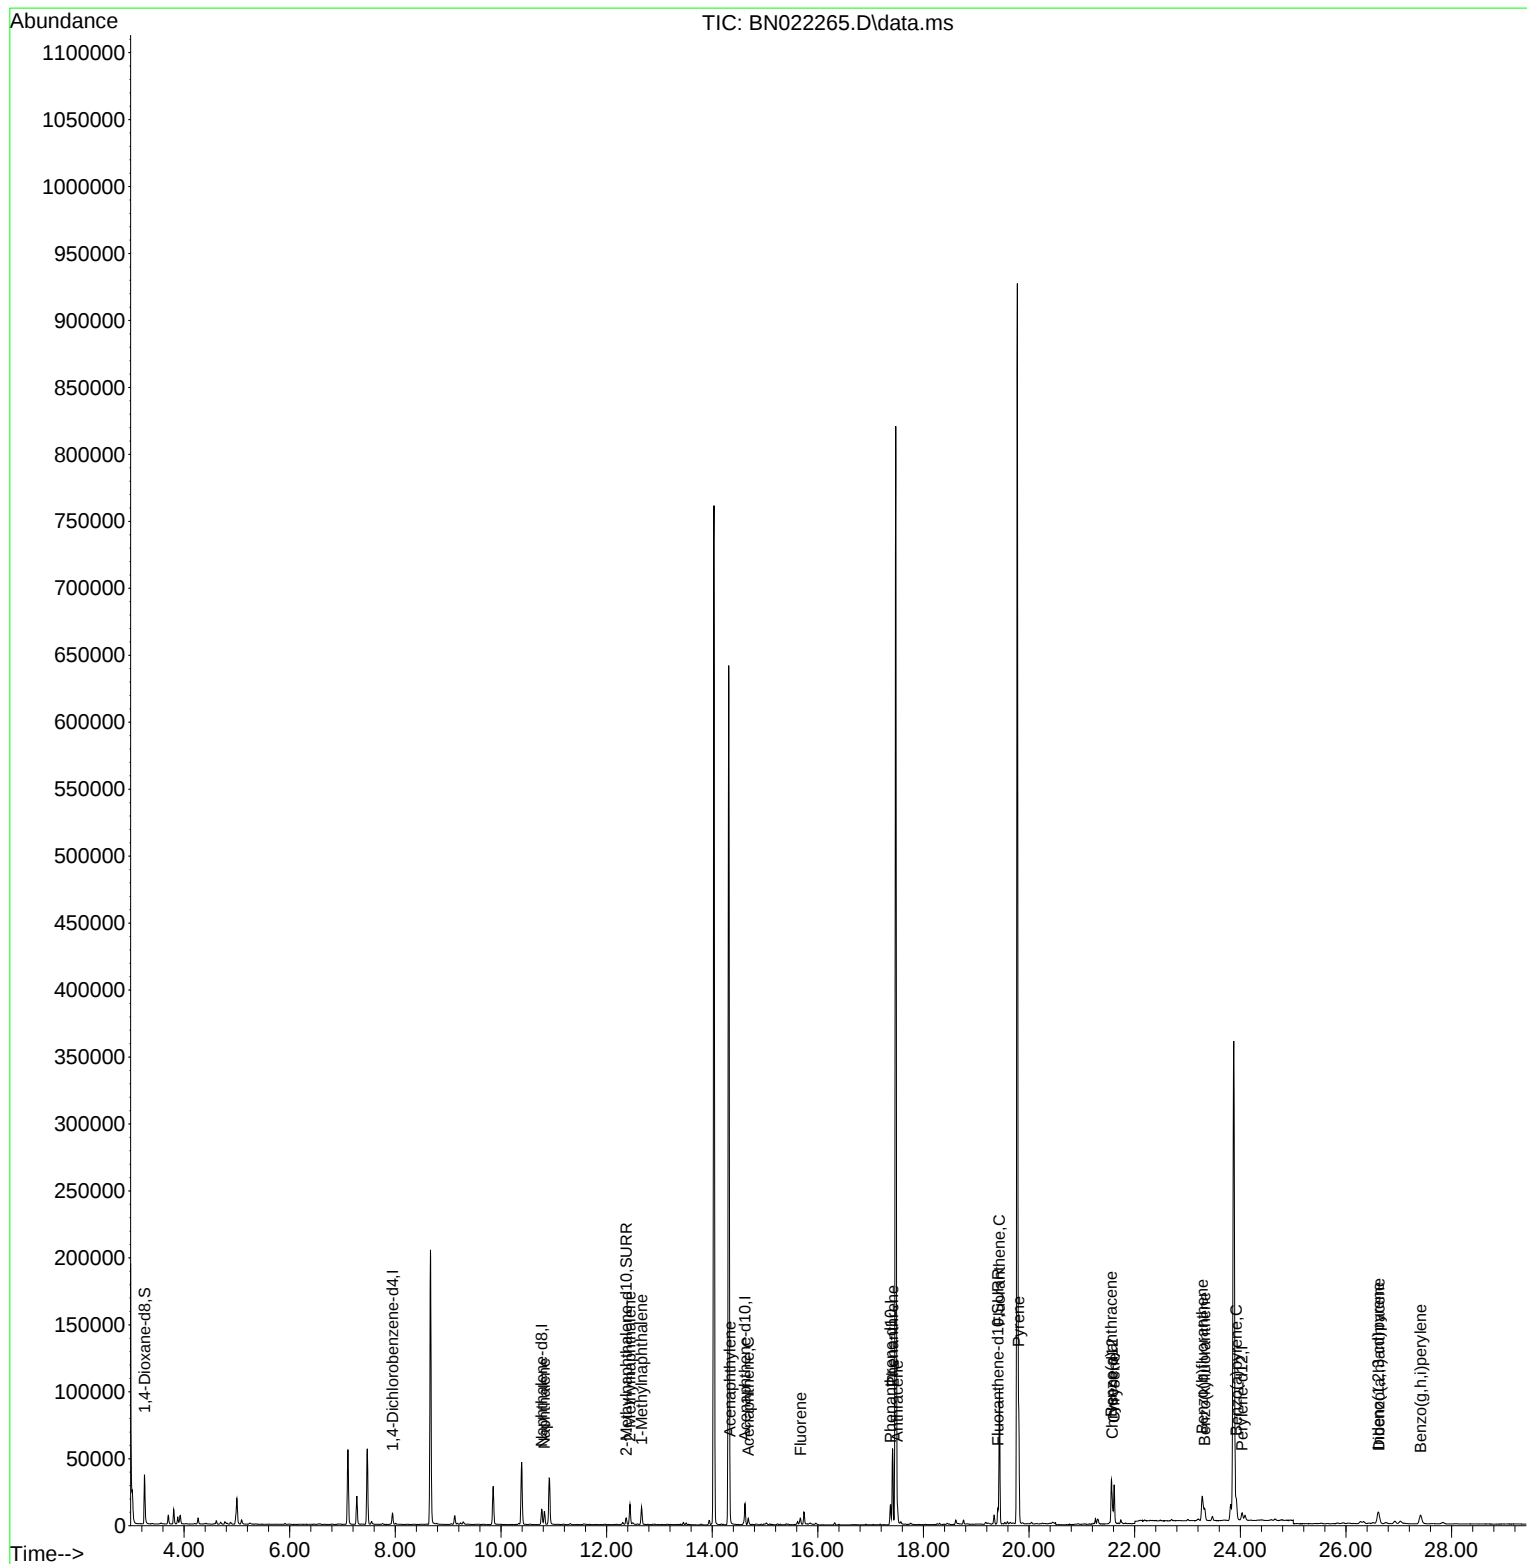

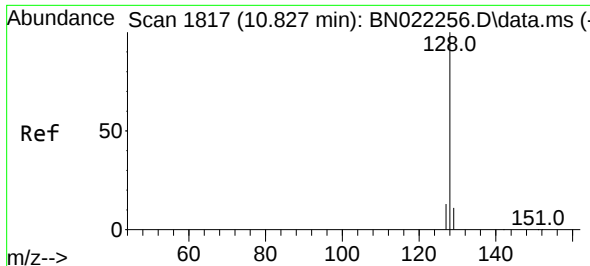

#5
Naphthalene
Concen: 0.298 ng/ul
RT: 10.820 min Scan# 1817
Delta R.T. -0.011 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54




Instrument :
BNA_N
ClientSampleId :
COBM3




Tgt Ion:128 Resp: 13034
Ion Ratio Lower Upper
128 100
129 11.8 9.3 13.9
127 13.6 10.7 16.1

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

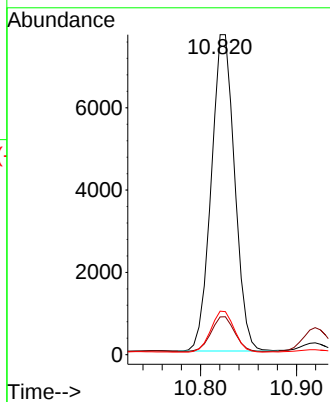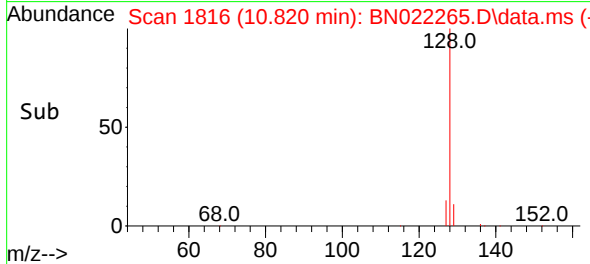


#7
2-Methylnaphthalene
Concen: 0.385 ng/ul
RT: 12.443 min Scan# 2111
Delta R.T. -0.006 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54

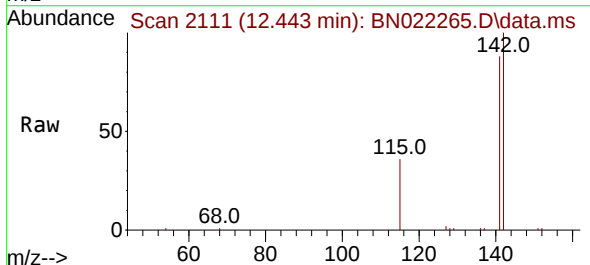

Tgt Ion:142 Resp: 10604
Ion Ratio Lower Upper
142 100
141 88.8 71.1 106.7

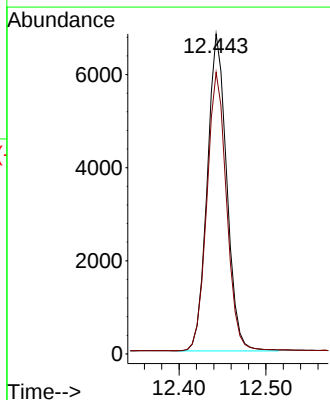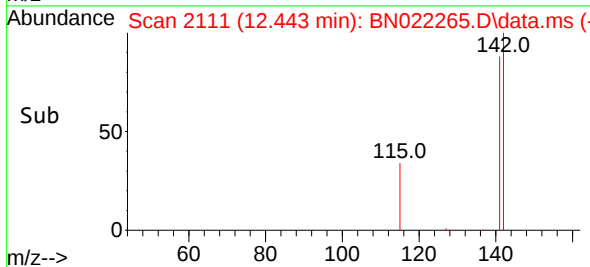

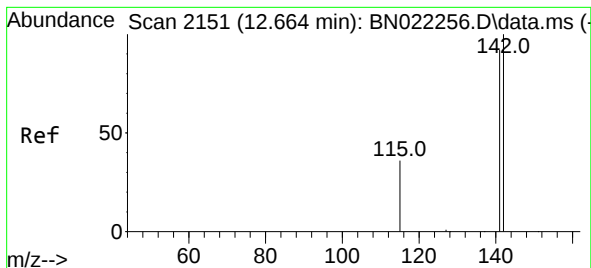

#8

1-Methylnaphthalene

Concen: 0.324 ng/ul

RT: 12.663 min Scan# 2151

Delta R.T. -0.006 min

Lab File: BN022265.D


Acq: 21 Oct 2022 21:54

Instrument :

BNA_N

ClientSampleId :

COBM3

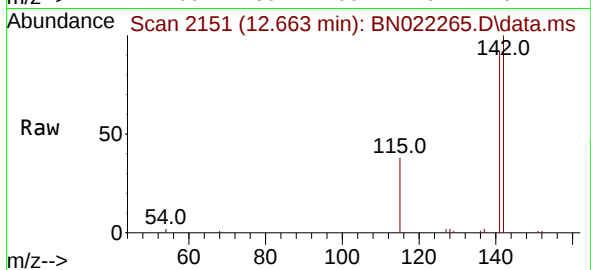

Tgt Ion:142 Resp: 916

Ion Ratio Lower Upper




142 100

141 91.7 73.3 109.9

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

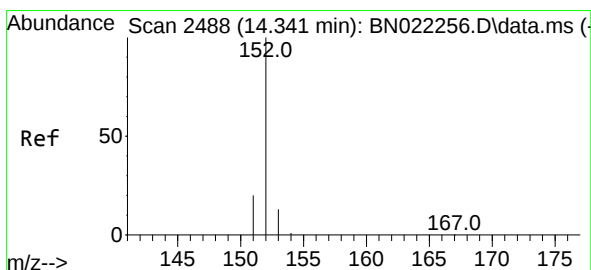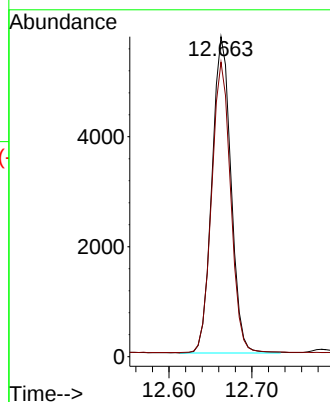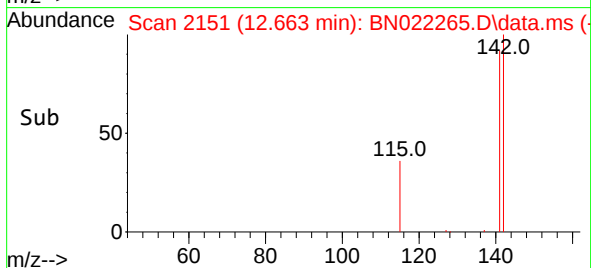

#10

Acenaphthylene

Concen: 0.081 ng/ul

RT: 14.340 min Scan# 2488

Delta R.T. -0.009 min

Lab File: BN022265.D

Acq: 21 Oct 2022 21:54




Tgt Ion:152 Resp: 3063


Ion Ratio Lower Upper

152 100

151 24.5 15.9 23.9#


153 24.0 10.8 16.2#

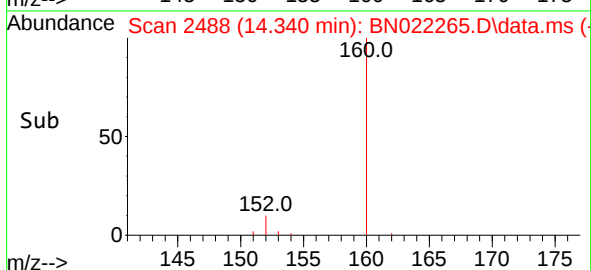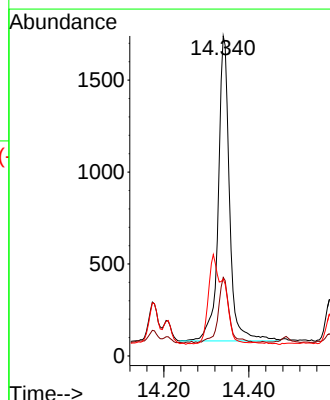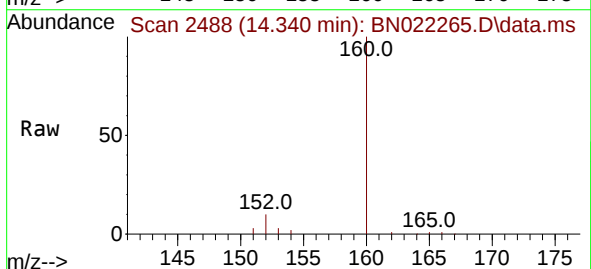

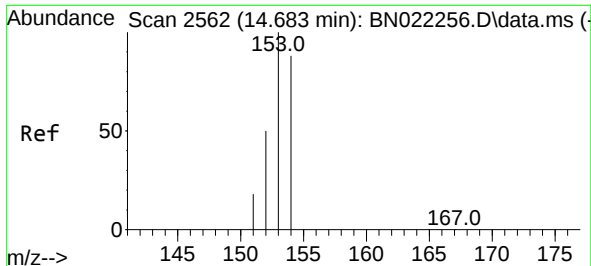

#11
Acenaphthene
Concen: 0.088 ng/u1
RT: 14.682 min Scan# 21
Delta R.T. -0.005 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54




Instrument :
BNA_N
ClientSampleId :
COBM3

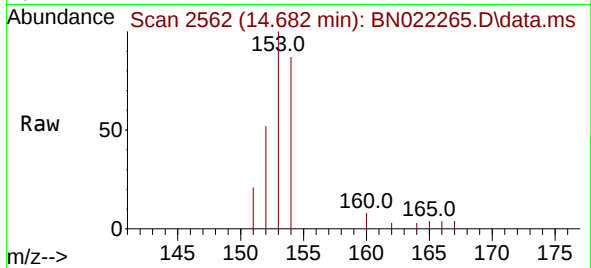


Tgt Ion:153 Resp: 280
Ion Ratio Lower Upper
153 100
152 52.3 40.6 61.0
154 87.1 70.6 106.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

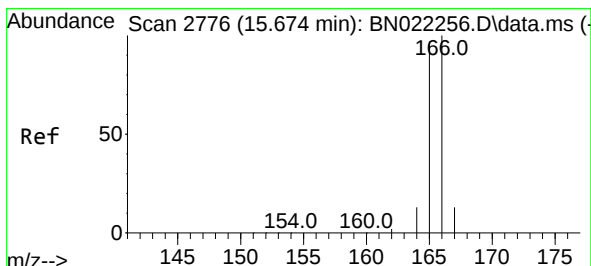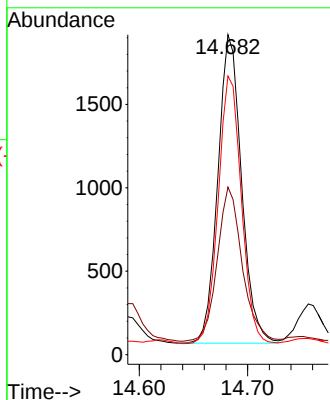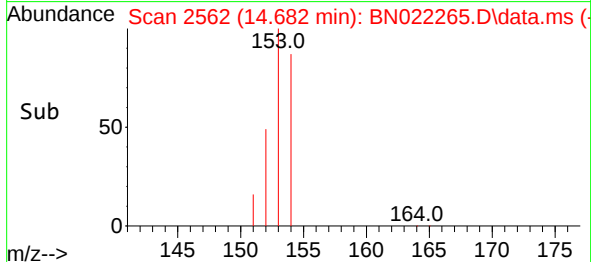


#12
Fluorene
Concen: 0.074 ng/u1
RT: 15.672 min Scan# 2776
Delta R.T. -0.005 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54

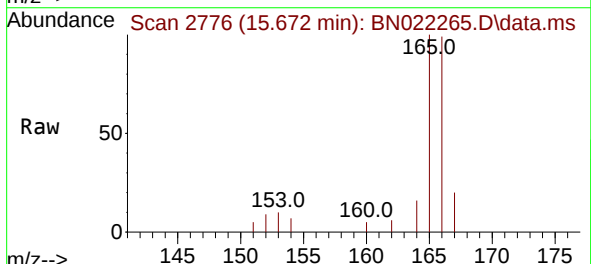


Tgt Ion:166 Resp: 2739
Ion Ratio Lower Upper
166 100
165 100.8 78.2 117.2
167 19.9 11.0 16.4#

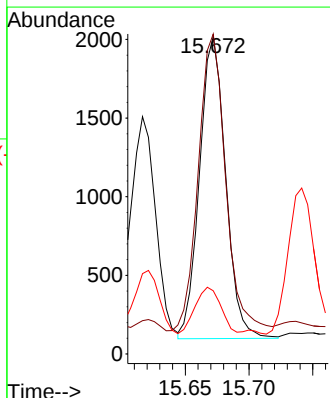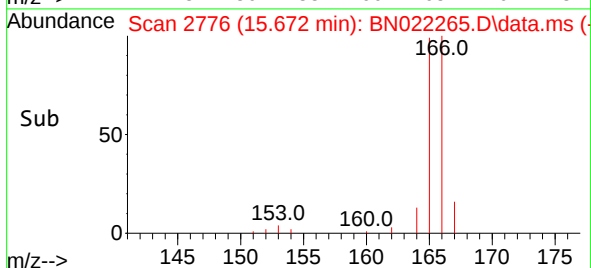

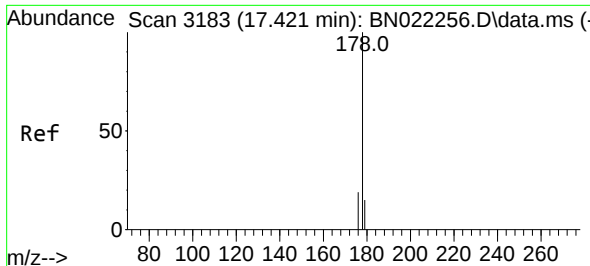

#15
Phenanthrene
Concen: 1.058 ng/u1
RT: 17.415 min Scan# 3182
Delta R.T. -0.009 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54




Instrument :
BNA_N
ClientSampleId :
COBM3




Tgt Ion:178 Resp: 5935
Ion Ratio Lower Upper
178 100
179 15.2 12.7 19.1
176 19.6 15.4 23.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

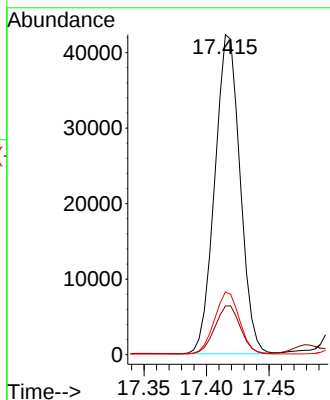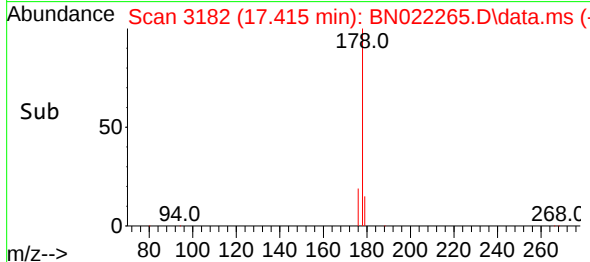


#16
Anthracene
Concen: 0.222 ng/u1
RT: 17.508 min Scan# 3204
Delta R.T. -0.009 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54

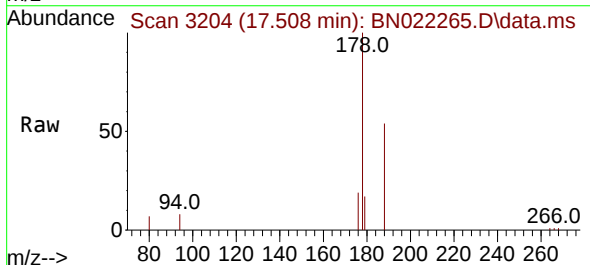


Tgt Ion:178 Resp: 10516
Ion Ratio Lower Upper
178 100
179 16.6 12.6 18.8
176 19.3 15.0 22.6

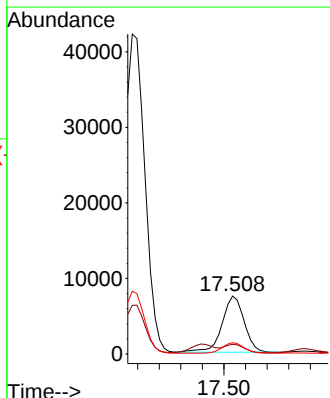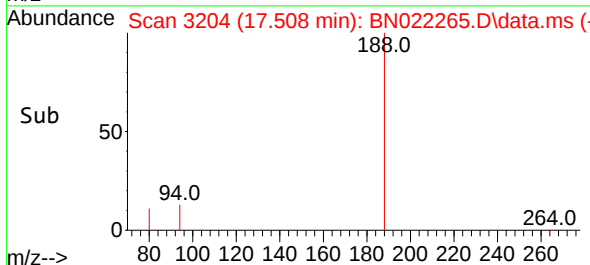

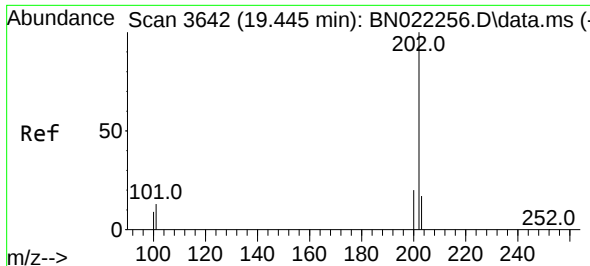

#19
Fluoranthene
Concen: 1.860 ng/ul
RT: 19.438 min Scan# 3641
Delta R.T. -0.005 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54




Instrument :
BNA_N
ClientSampleId :
COBM3




Tgt Ion:202 Resp: 8135
Ion Ratio Lower Upper
202 100
101 14.8 11.8 17.6
100 11.1 8.7 13.1

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

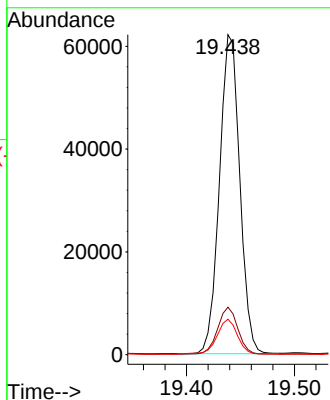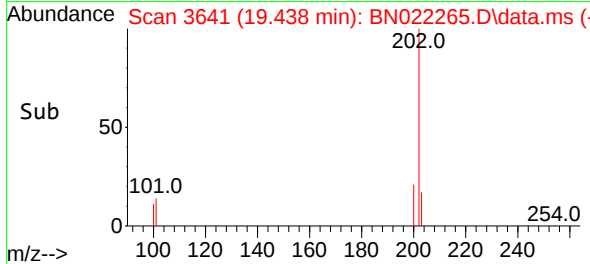


#20
Pyrene
Concen: 1.422 ng/ul m
RT: 19.806 min Scan# 3720
Delta R.T. -0.005 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54

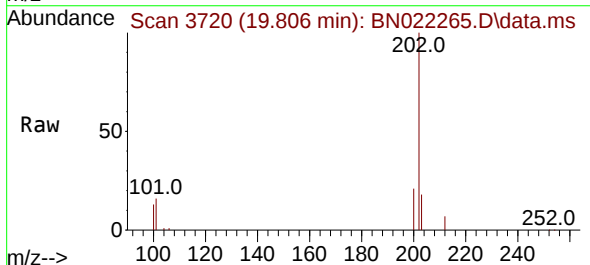


Tgt Ion:202 Resp: 62498
Ion Ratio Lower Upper
202 100
101 16.2 13.1 19.7
100 12.6 10.6 16.0

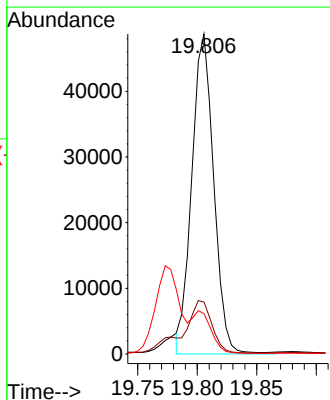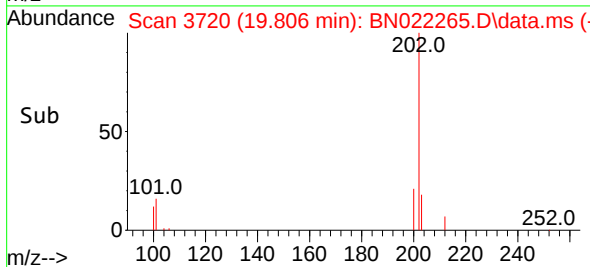

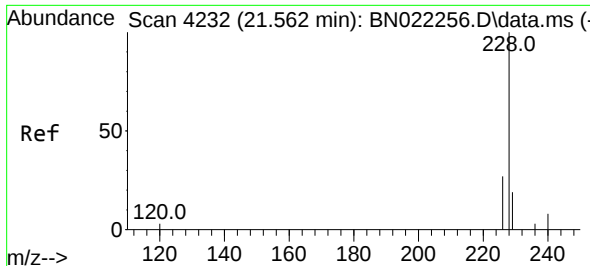

#21
Benzo(a)anthracene
Concen: 0.771 ng/ul
RT: 21.559 min Scan# 41
Delta R.T. -0.009 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54




Instrument :
BNA_N
ClientSampleId :
COBM3




Tgt Ion:228 Resp: 2758
Ion Ratio Lower Upper
228 100
229 21.9 15.7 23.5
226 29.2 21.5 32.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

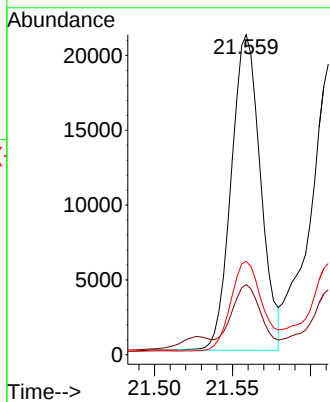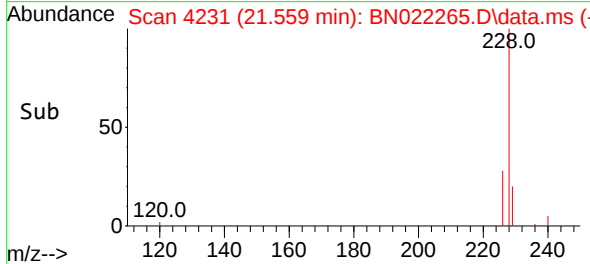


#22
Chrysene
Concen: 0.761 ng/ul
RT: 21.611 min Scan# 4249
Delta R.T. -0.009 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54

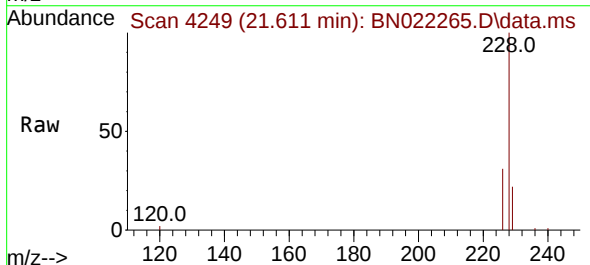


Tgt Ion:228 Resp: 28854
Ion Ratio Lower Upper
228 100
226 31.4 23.9 35.9
229 22.3 15.9 23.9

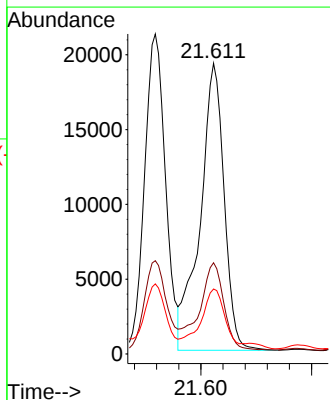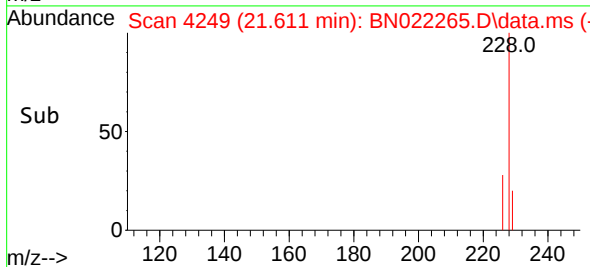



#24
Benzo(b)fluoranthene
Concen: 0.845 ng/ul m
RT: 23.280 min Scan# 4820
Delta R.T. -0.009 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54




Instrument :
BNA_N
ClientSampleId :
COBM3




Tgt Ion:252 Resp: 3265
Ion Ratio Lower Upper
252 100
253 25.9 0.0 49.0
125 22.0 0.0 35.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

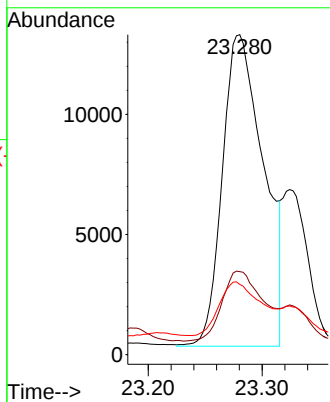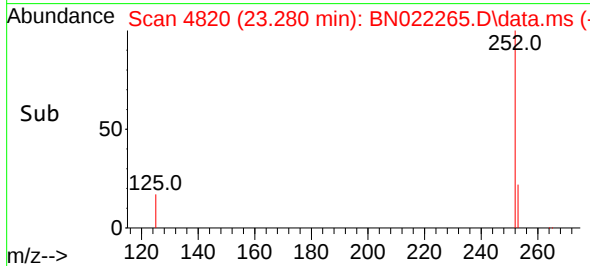


#25
Benzo(k)fluoranthene
Concen: 0.264 ng/ul m
RT: 23.324 min Scan# 4835
Delta R.T. -0.015 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54

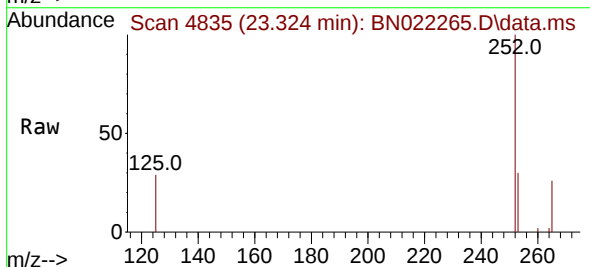


Tgt Ion:252 Resp: 9923
Ion Ratio Lower Upper
252 100
253 30.1 19.7 29.5#
125 29.5 14.0 21.0#

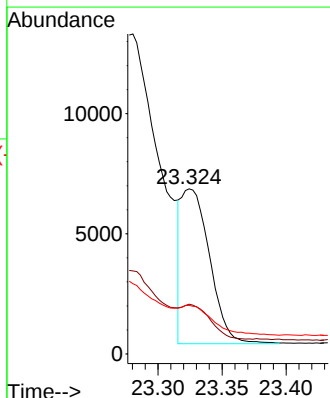

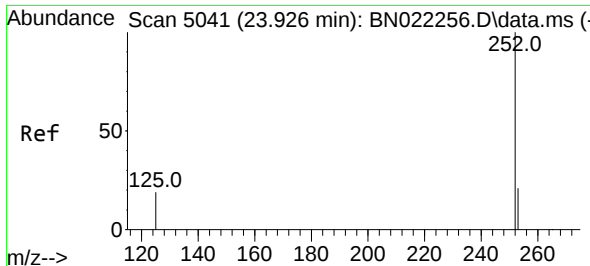

#26
Benzo(a)pyrene
Concen: 0.642 ng/ul
RT: 23.924 min Scan# 5041
Delta R.T. -0.012 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54




Instrument :
BNA_N
ClientSampleId :
COBM3




Tgt Ion:252 Resp: 19784
Ion Ratio Lower Upper
252 100
253 26.8 21.0 31.6
125 26.6 17.9 26.9

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

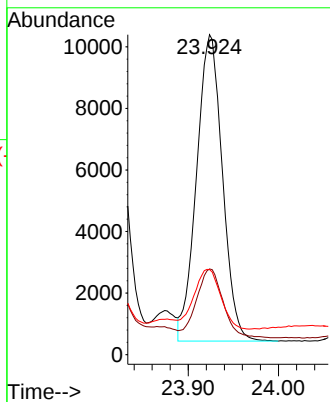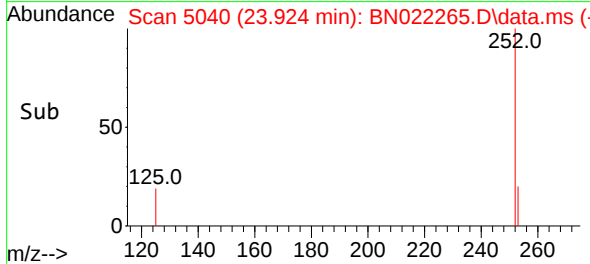


#27
Indeno(1,2,3-cd)pyrene
Concen: 0.397 ng/ul
RT: 26.612 min Scan# 5889
Delta R.T. -0.024 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54

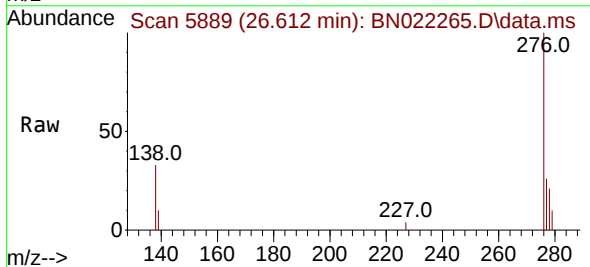


Tgt Ion:276 Resp: 15200
Ion Ratio Lower Upper
276 100
138 30.6 27.7 41.5
227 0.0 0.2 0.2#

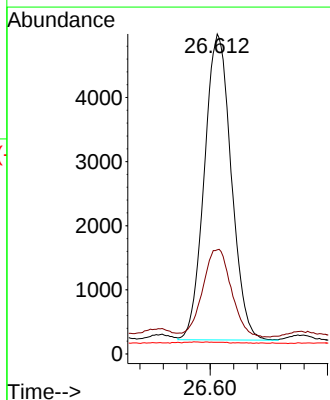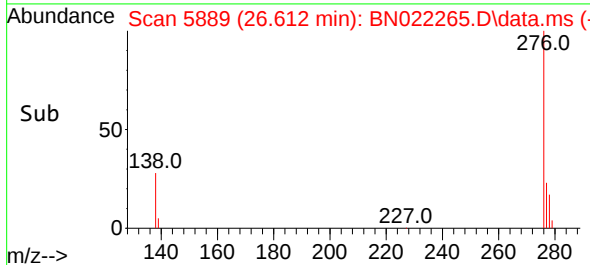

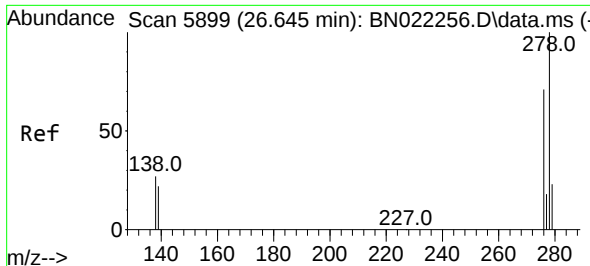

#28
Dibenzo(a,h)anthracene
Concen: 0.129 ng/ul
RT: 26.625 min Scan# 5893
Delta R.T. -0.030 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54




Instrument :
BNA_N
ClientSampleId :
COBM3




Tgt Ion: 278 Resp: 394
Ion Ratio Lower Upper
278 100
139 44.2 19.6 29.4
279 43.8 20.6 30.8

Manual Integrations
APPROVED

Reviewed By : Jagrut Upadhyay 10/24/2022
Supervised By : mohammad ahmed 10/24/2022

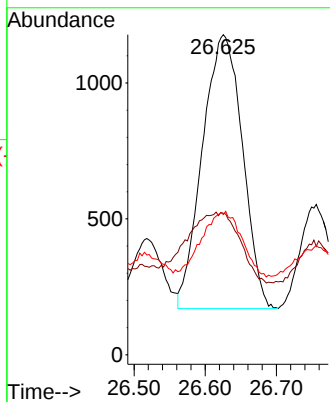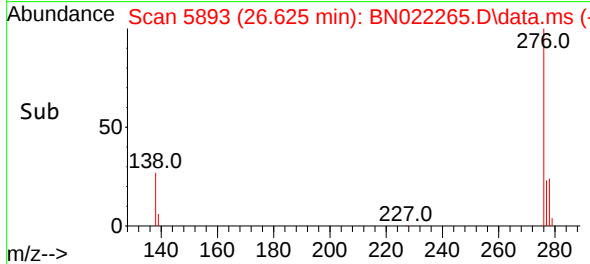

#29
Benzo(g,h,i)perylene
Concen: 0.459 ng/ul
RT: 27.413 min Scan# 6128
Delta R.T. -0.017 min
Lab File: BN022265.D
Acq: 21 Oct 2022 21:54

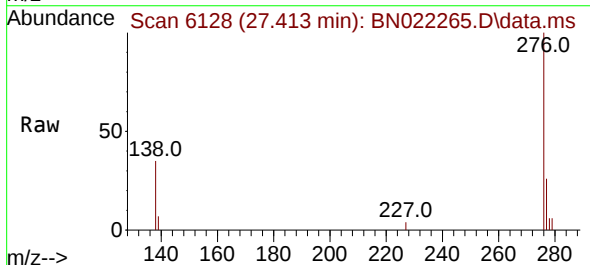

Tgt Ion: 276 Resp: 14326
Ion Ratio Lower Upper
276 100
138 34.7 25.2 37.8
277 26.3 19.9 29.9

