
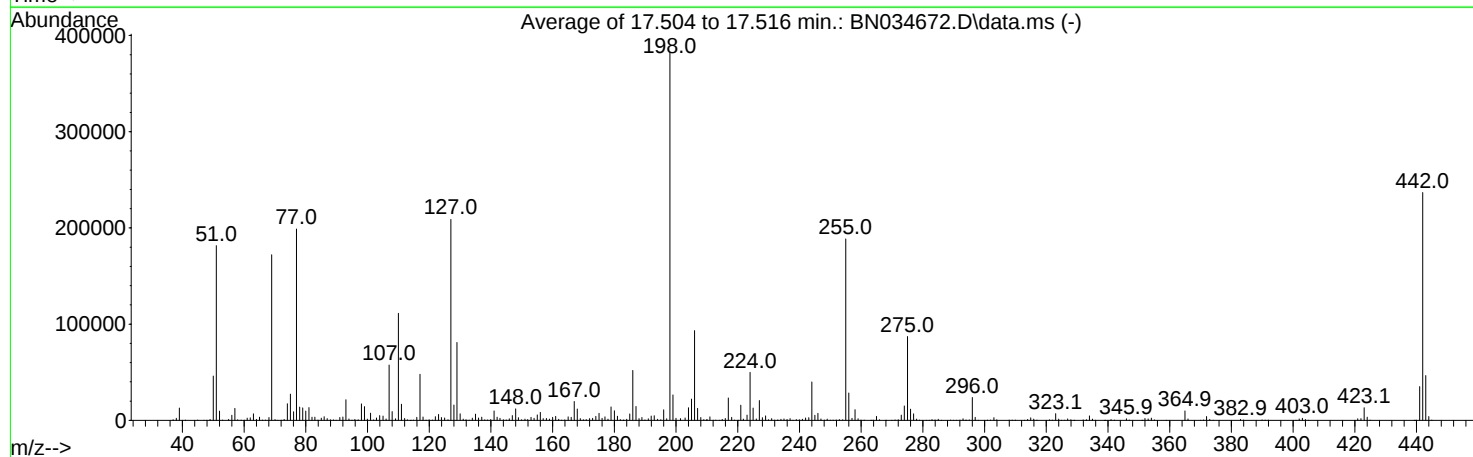


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102224\
Data File : BN034672.D
Acq On : 22 Oct 2024 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 22 16:43:19 2024

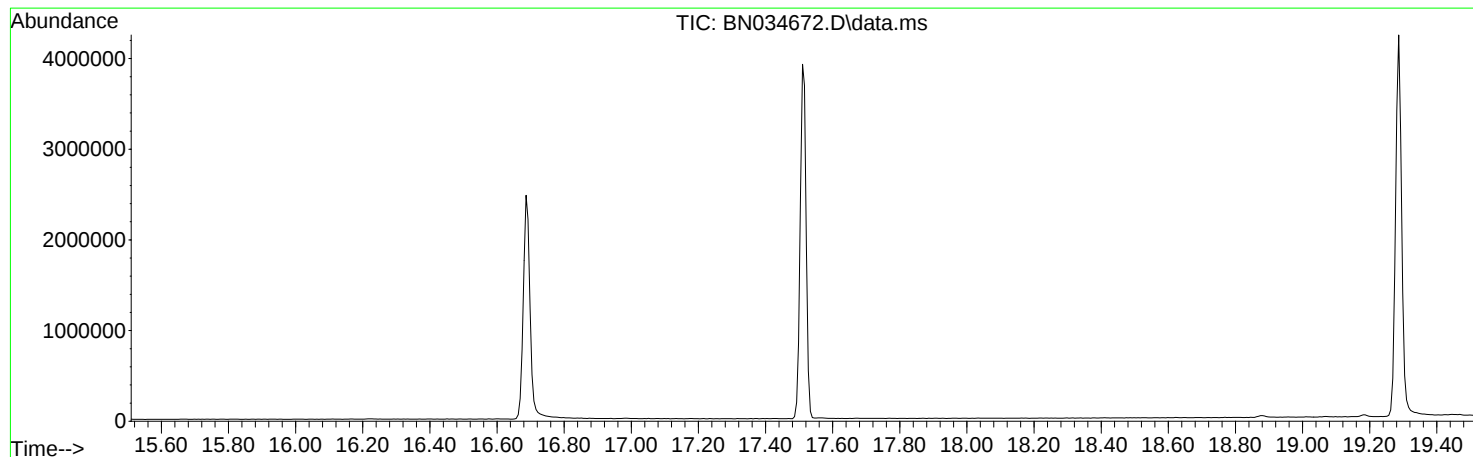




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.5	181584	PASS
68	69	0.00	2	1.7	2930	PASS
69	198	0.00	100	45.0	172173	PASS
70	69	0.00	2	0.5	780	PASS
127	198	10	80	54.6	208896	PASS
197	198	0.00	2	0.4	1640	PASS
198	198	100	100	100.0	382293	PASS
199	198	5	9	6.9	26389	PASS
275	198	10	60	22.8	87227	PASS
365	198	1	100	2.6	9770	PASS
441	198	0.01	100	9.2	35043	PASS
442	442	50	100	100.0	236811	PASS
443	442	15	24	19.7	46611	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102224\
Data File : BN034672.D
Acq On : 22 Oct 2024 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 23 02:40:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 02:40:52 2024
Response via : Initial Calibration

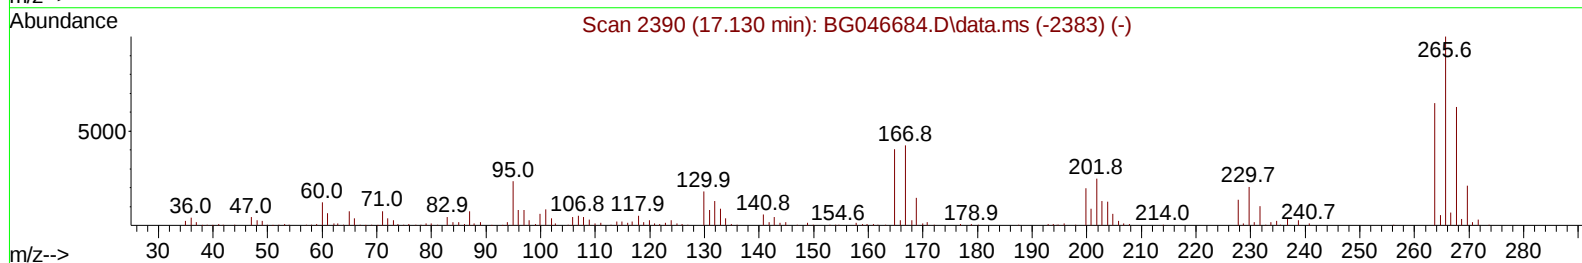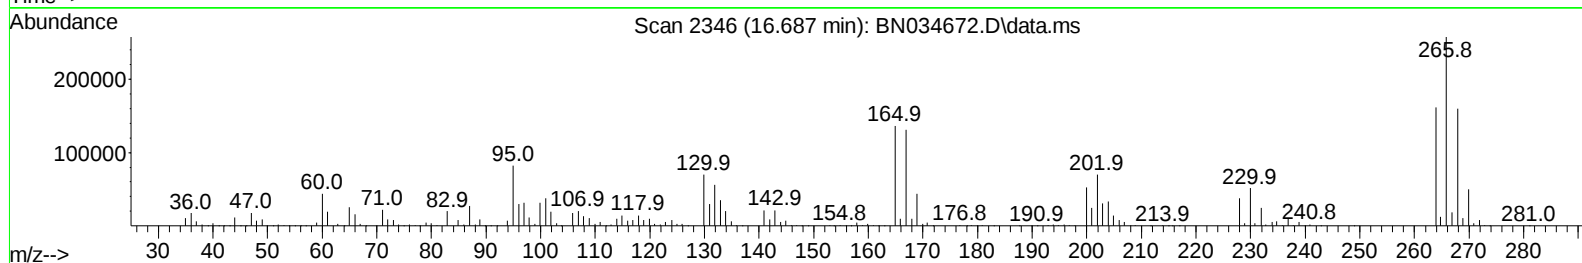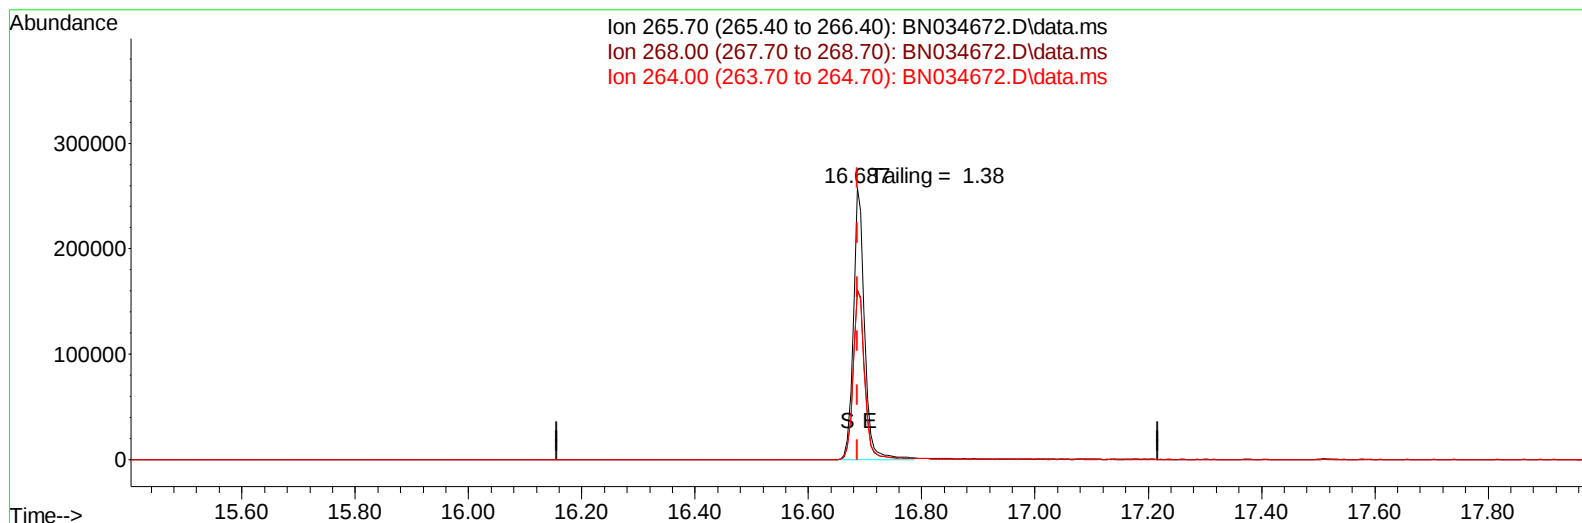

TIC: BN034672.D\data.ms



(70) Pentachlorophenol (C)

16.687min (0.000) 17591.97 ng

response 356188

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.20
264.00	61.60	62.69
0.00	0.00	0.00

Instrument :
BNA_N
ClientSampleId :
DFTPP

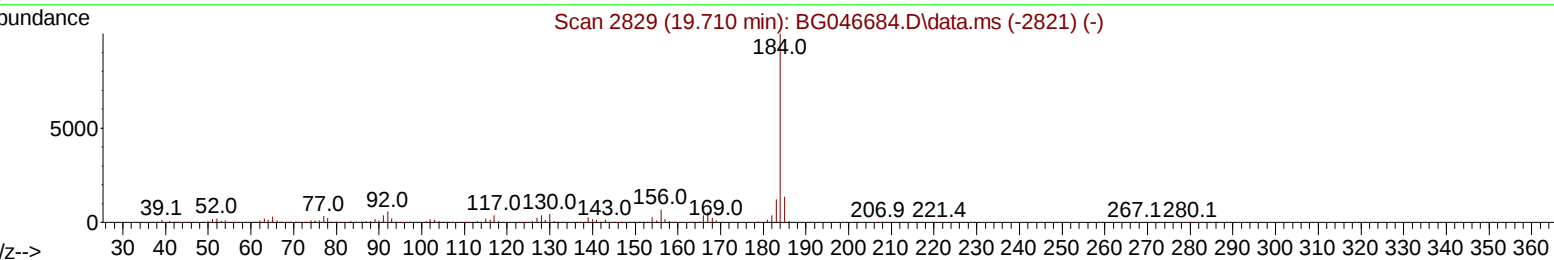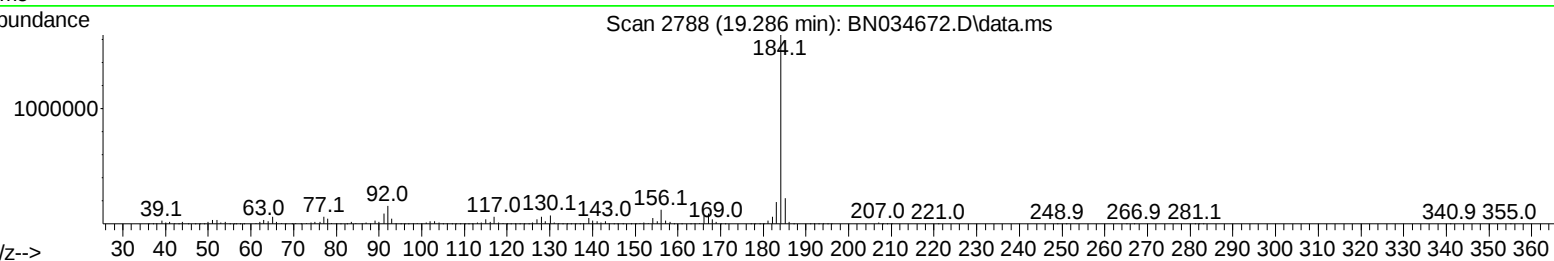

TIC: BN034672.D\data.ms

(77) Benzidine

19.286min (0.000) 0.00 ng

response **2070557**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.42
183.00	13.20	11.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/22/2024	BNA_N	<u>BN034672.D</u>
Compound Name	Response	Retention Time
DDT	785665	20.533
DDD	125523	20.092
DDE	9286	19.586
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
134809	920474	14.65

Instrument :
BNA_N
ClientSampleId :
DFTPP