

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102422\
 Data File : BN022324.D
 Acq On : 25 Oct 2022 14:32
 Operator : CG/JU
 Sample : PB148368BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 27 05:13:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 22 03:40:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.944	152	4443	0.400	ng/ul	0.00
4) Naphthalene-d8	10.772	136	15145	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.618	164	7969	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.374	188	13921	0.400	ng/ul	0.00
17) Chrysene-d12	21.582	240	8156	0.400	ng/ul	0.00
23) Perylene-d12	24.043	264	7757	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.253	96	31560	5.466	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.373	152	6889	0.301	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	9873	0.361	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.779	202	1552	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.882	252	2833	0.091	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102422\
Data File : BN022324.D
Acq On : 25 Oct 2022 14:32
Operator : CG/JU
Sample : PB148368BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 27 05:13:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 22 03:40:14 2022
Response via : Initial Calibration

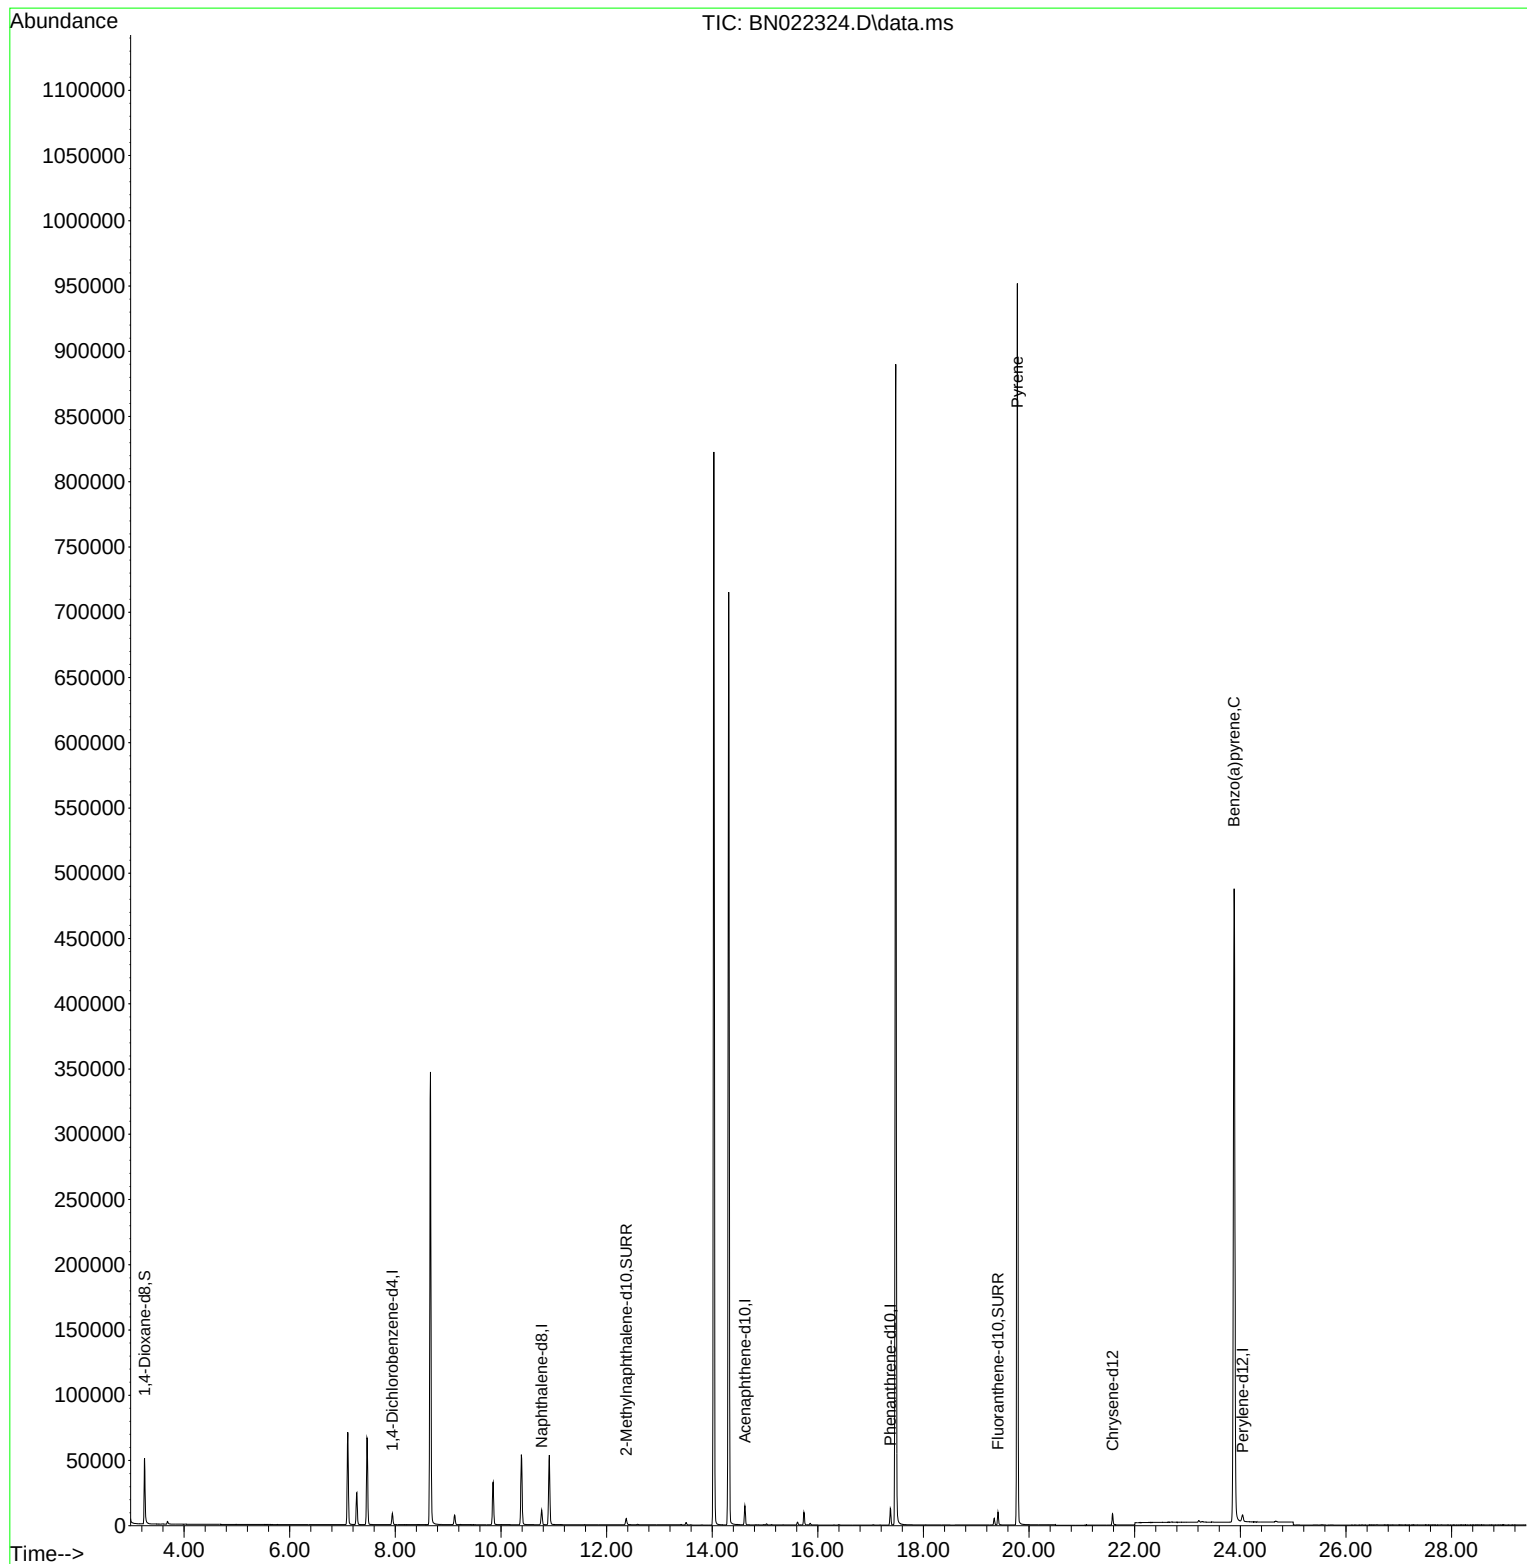

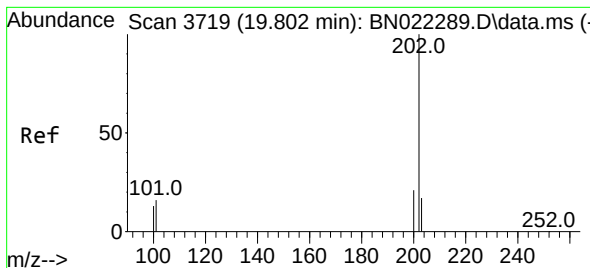

#20

Pyrene

Concen: 0.041 ng/ul

RT: 19.779 min Scan# 31

Delta R.T. -0.023 min

Lab File: BN022324.D

Acq: 25 Oct 2022 14:32





Instrument :

BNA_N

ClientSampleId :

Tgt Ion:202 Resp: 1552

Ion	Ratio	Lower	Upper
202	100		
101	174.1	13.1	19.7#
100	1246.3	10.6	16.0#

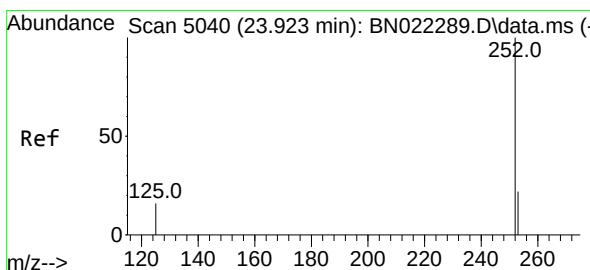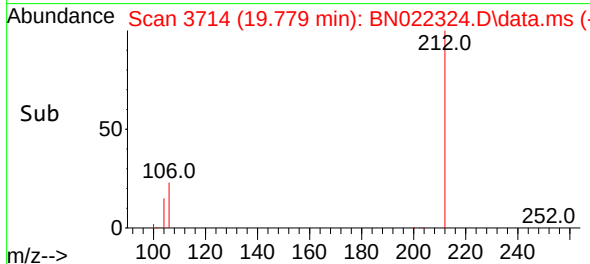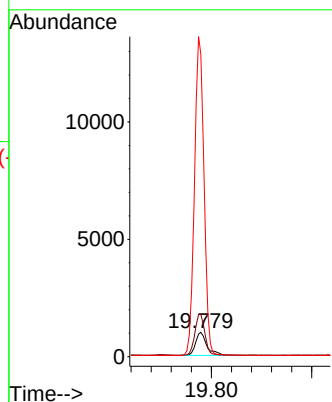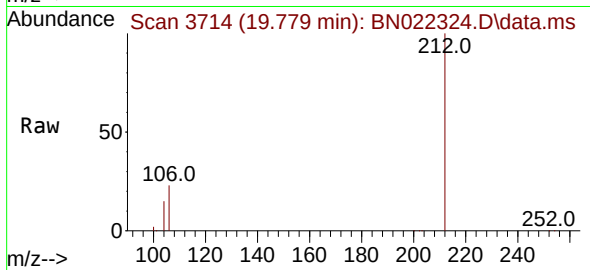

#26

Benzo(a)pyrene

Concen: 0.091 ng/ul

RT: 23.882 min Scan# 5026

Delta R.T. -0.038 min

Lab File: BN022324.D

Acq: 25 Oct 2022 14:32

Tgt Ion:252 Resp: 2833

Ion	Ratio	Lower	Upper
252	100		
253	47.1	21.0	31.6#
125	50.4	17.9	26.9#

