

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102424\
 Data File : BN034688.D
 Acq On : 24 Oct 2024 11:35
 Operator : RC/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Oct 24 12:43:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 24 12:41:40 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.712	152	6253	0.400	ng	0.00
7) Naphthalene-d8	10.479	136	18478	0.400	ng	0.00
13) Acenaphthene-d10	14.329	164	9335	0.400	ng	0.00
19) Phenanthrene-d10	17.069	188	19334	0.400	ng	0.00
29) Chrysene-d12	21.250	240	11924	0.400	ng	0.00
35) Perylene-d12	23.467	264	10103	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.322	112	31333	1.638	ng	0.00
5) Phenol-d6	6.882	99	41454	1.694	ng	0.00
8) Nitrobenzene-d5	8.845	82	25808	1.686	ng	0.00
11) 2-Methylnaphthalene-d10	12.071	152	43281	1.664	ng	0.00
14) 2,4,6-Tribromophenol	15.815	330	4968	1.255	ng	0.00
15) 2-Fluorobiphenyl	12.950	172	62224	1.691	ng	0.00
27) Fluoranthene-d10	19.094	212	73515	1.553	ng	0.00
31) Terphenyl-d14	19.703	244	41261	1.788	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.285	88	13254	1.741	ng	99
3) n-Nitrosodimethylamine	3.581	42	20688	2.247	ng	# 98
6) bis(2-Chloroethyl)ether	7.142	93	33672	1.797	ng	99
9) Naphthalene	10.532	128	85545	1.679	ng	99
10) Hexachlorobutadiene	10.831	225	12572	1.540	ng	# 100
12) 2-Methylnaphthalene	12.147	142	53951	1.675	ng	99
16) Acenaphthylene	14.040	152	76104	1.696	ng	99
17) Acenaphthene	14.393	154	52549	1.718	ng	98
18) Fluorene	15.377	166	65352	1.714	ng	100
20) 4,6-Dinitro-2-methylph...	15.452	198	4583	1.734	ng	# 50
21) 4-Bromophenyl-phenylether	16.275	248	17079	1.615	ng	98
22) Hexachlorobenzene	16.374	284	18410	1.569	ng	99
23) Atrazine	16.548	200	14024	1.516	ng	100
24) Pentachlorophenol	16.721	266	6756	1.467	ng	99
25) Phenanthrene	17.106	178	96240	1.673	ng	100
26) Anthracene	17.193	178	87194	1.695	ng	100
28) Fluoranthene	19.127	202	103093	1.598	ng	100
30) Pyrene	19.489	202	103194	1.936	ng	100
32) Benzo(a)anthracene	21.232	228	76954	1.693	ng	100
33) Chrysene	21.286	228	78358	1.741	ng	99
34) Bis(2-ethylhexyl)phtha...	21.196	149	41892	1.354	ng	# 100
36) Indeno(1,2,3-cd)pyrene	25.697	276	65482	1.682	ng	99
37) Benzo(b)fluoranthene	22.803	252	68644	1.880	ng	# 90
38) Benzo(k)fluoranthene	22.850	252	69183	1.942	ng	# 88
39) Benzo(a)pyrene	23.370	252	55896	1.802	ng	# 85
40) Dibenzo(a,h)anthracene	25.715	278	51867	1.696	ng	95
41) Benzo(g,h,i)perylene	26.373	276	56042	1.661	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102424\
Data File : BN034688.D
Acq On : 24 Oct 2024 11:35
Operator : RC/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Quant Time: Oct 24 12:43:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 24 12:41:40 2024
Response via : Initial Calibration

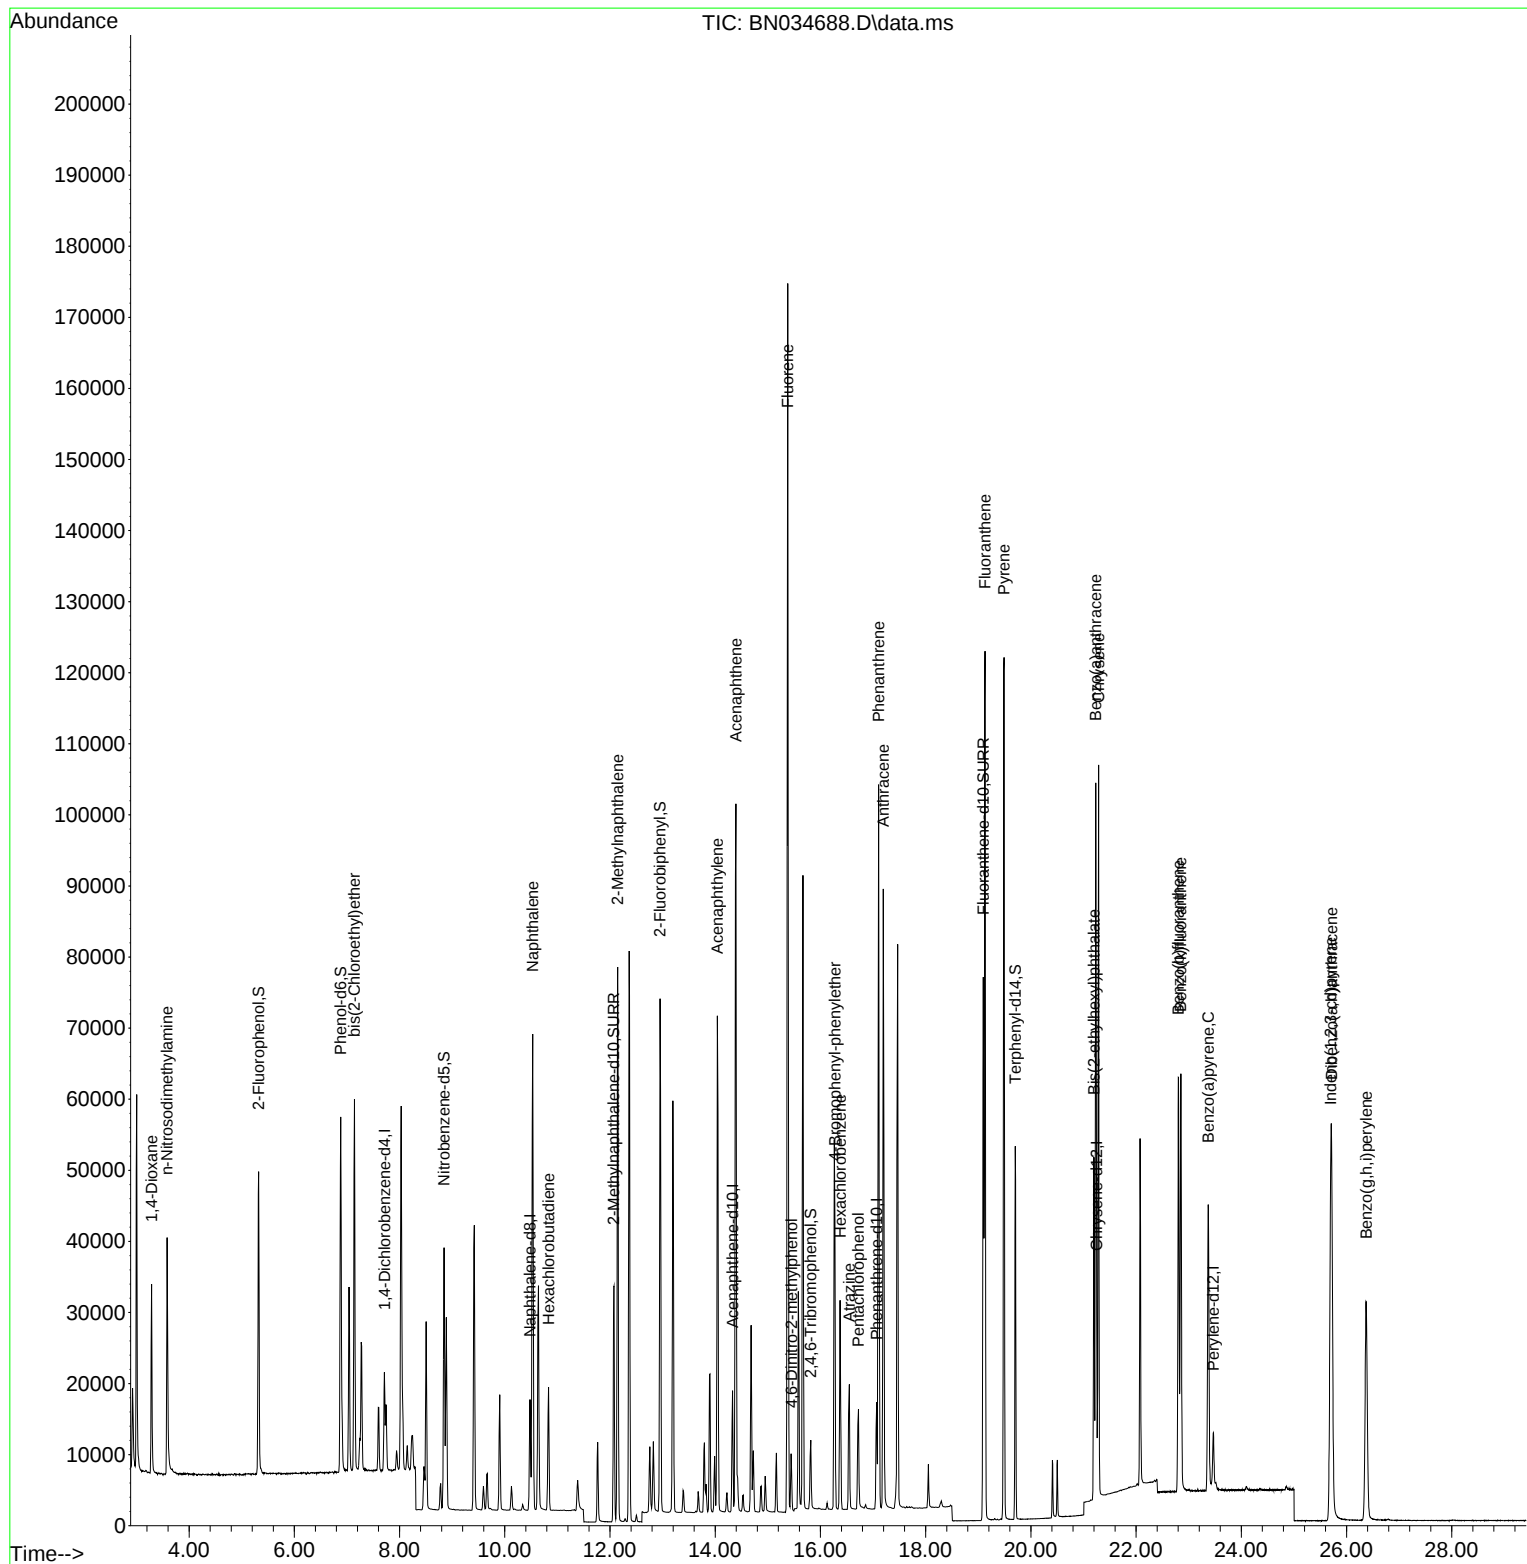






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.712 min Scan# 669
 Delta R.T. 0.000 min
 Lab File: BN034688.D
 Acq: 24 Oct 2024 11:35

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6







Tgt Ion:152 Resp: 6253
 Ion Ratio Lower Upper
 152 100
 150 154.5 122.7 184.1
 115 63.8 51.0 76.6

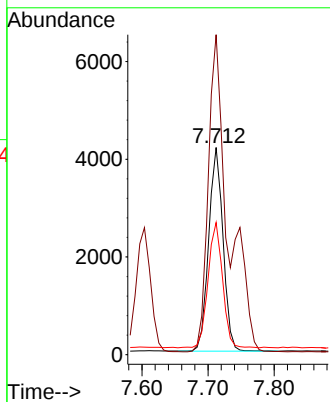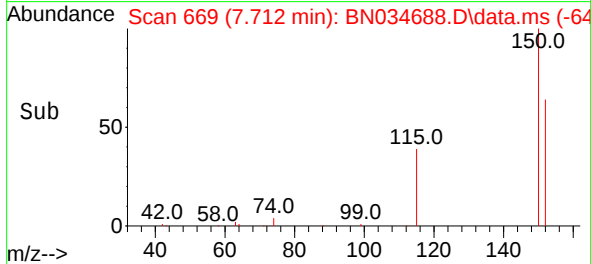

#2
 1,4-Dioxane
 Concen: 1.741 ng
 RT: 3.285 min Scan# 56
 Delta R.T. 0.000 min
 Lab File: BN034688.D
 Acq: 24 Oct 2024 11:35

Tgt Ion: 88 Resp: 13254
 Ion Ratio Lower Upper
 88 100
 43 40.1 32.1 48.1
 58 93.0 73.7 110.5


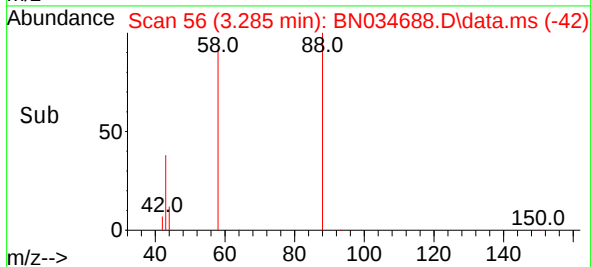
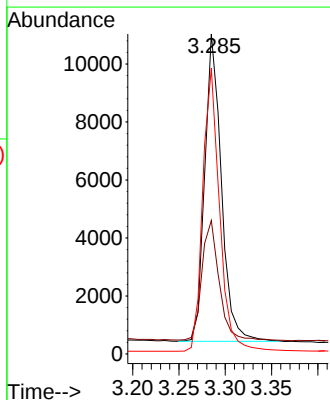
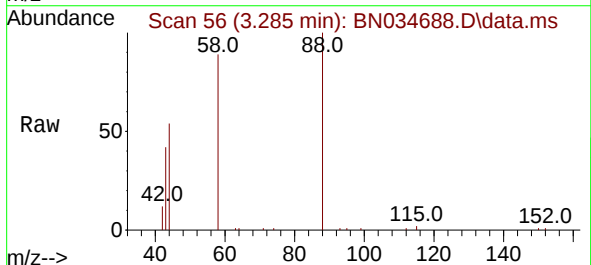


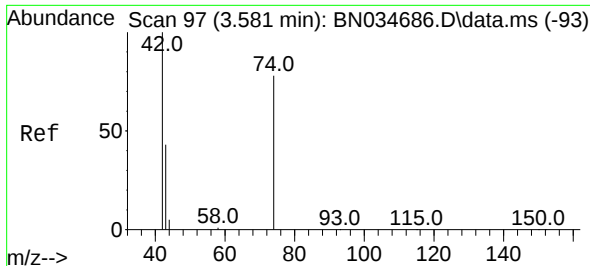

#3
n-Nitrosodimethylamine
Concen: 2.247 ng
RT: 3.581 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 42 Resp: 20688
Ion Ratio Lower Upper
42 100
74 96.2 77.2 115.8
44 11.1 13.4 20.2#

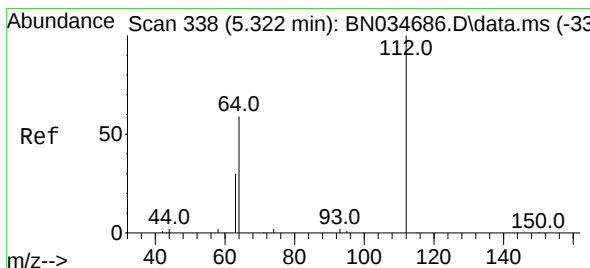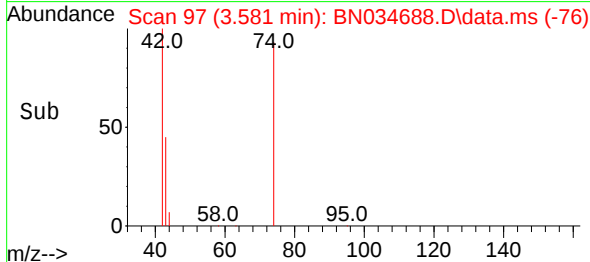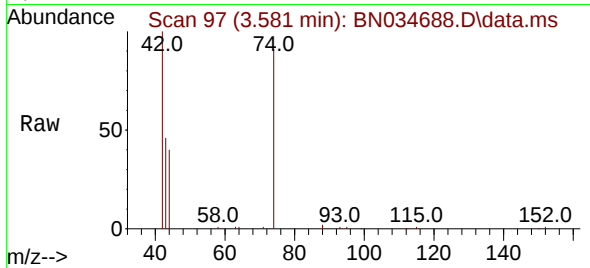

#4
2-Fluorophenol
Concen: 1.638 ng
RT: 5.322 min Scan# 338
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35

Tgt Ion: 112 Resp: 31333
Ion Ratio Lower Upper
112 100
64 65.7 53.0 79.6
63 34.8 27.6 41.4


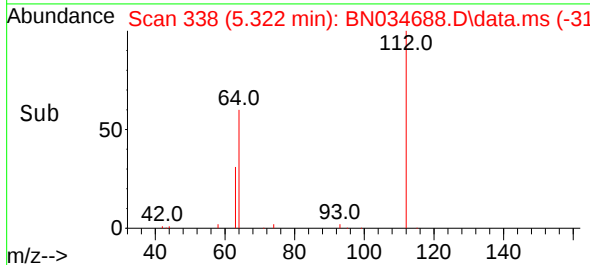

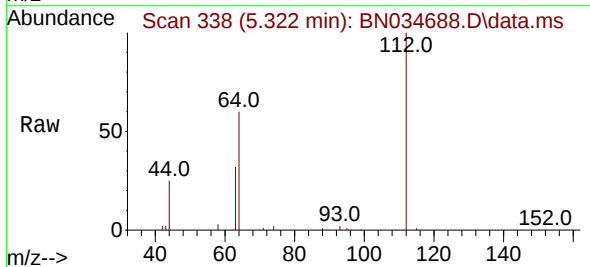




#5
Phenol-d6
Concen: 1.694 ng
RT: 6.882 min Scan# 511
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 99 Resp: 41454
Ion Ratio Lower Upper
99 100
42 27.2 21.8 32.8
71 33.2 26.6 40.0

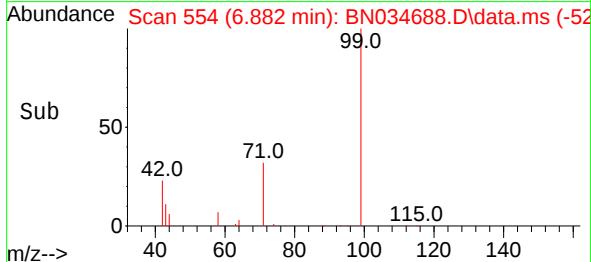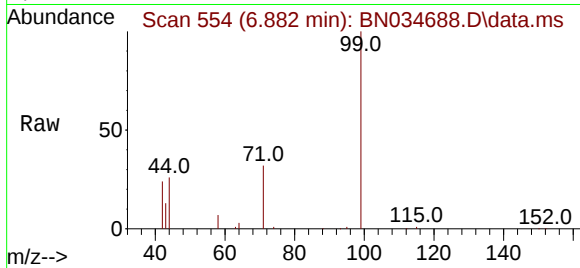

#6
bis(2-Chloroethyl)ether
Concen: 1.797 ng
RT: 7.142 min Scan# 590
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35

Tgt Ion: 93 Resp: 33672
Ion Ratio Lower Upper
93 100
63 88.5 71.5 107.3
95 32.0 25.8 38.6


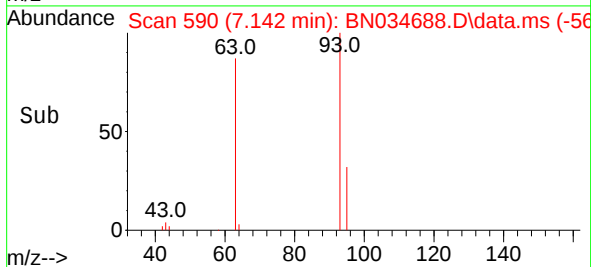

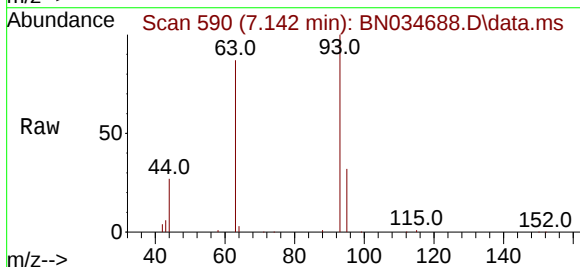




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.479 min Scan# 955
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	136	Resp:	18478
Ion Ratio	Lower	Upper	
136	100		
137	11.4	9.1	13.7
54	12.4	9.8	14.8
68	8.3	6.4	9.6

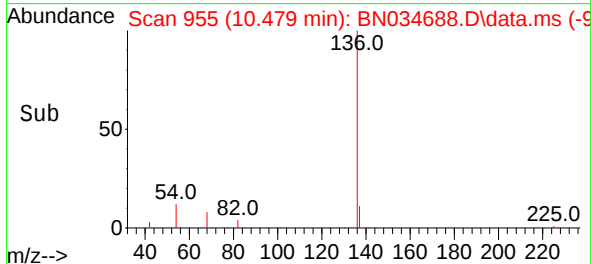

#8
Nitrobenzene-d5
Concen: 1.686 ng
RT: 8.845 min Scan# 802
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35

Tgt Ion:	82	Resp:	25808
Ion Ratio	Lower	Upper	
82	100		
128	35.7	29.7	44.5
54	64.5	53.0	79.6


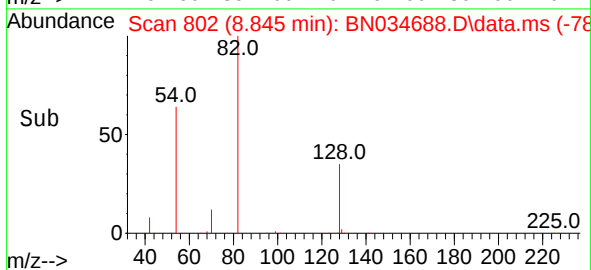

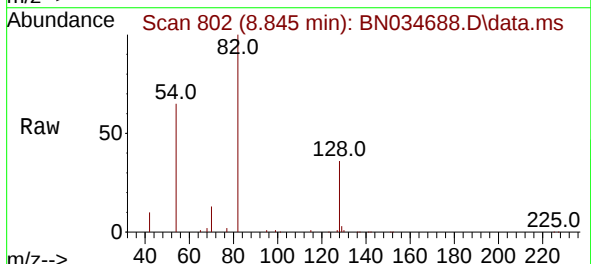


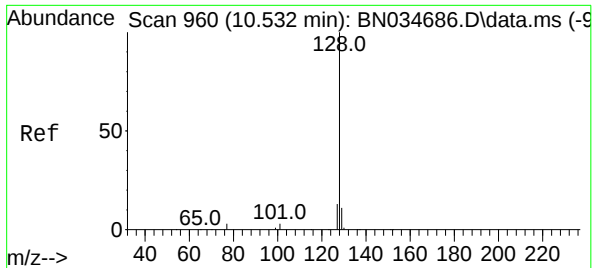

#9
Naphthalene
Concen: 1.679 ng
RT: 10.532 min Scan# 960
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:128 Resp: 85545
Ion Ratio Lower Upper
128 100
129 10.9 9.0 13.6
127 12.6 10.5 15.7

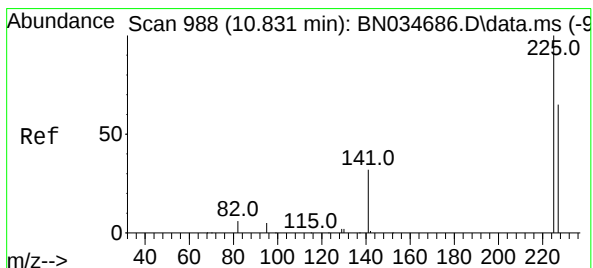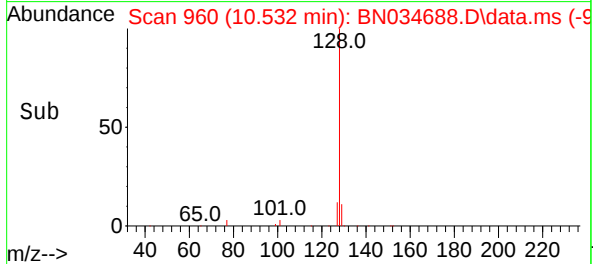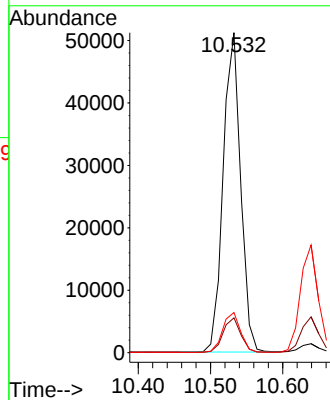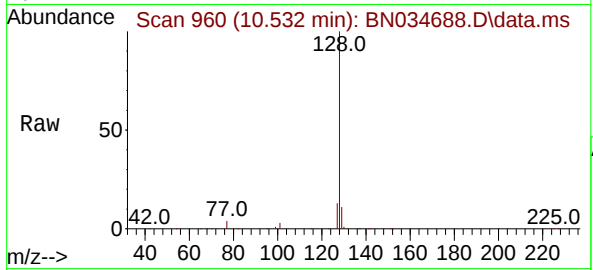

#10
Hexachlorobutadiene
Concen: 1.540 ng
RT: 10.831 min Scan# 988
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35

Tgt Ion:225 Resp: 12572
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.5 51.4 77.0

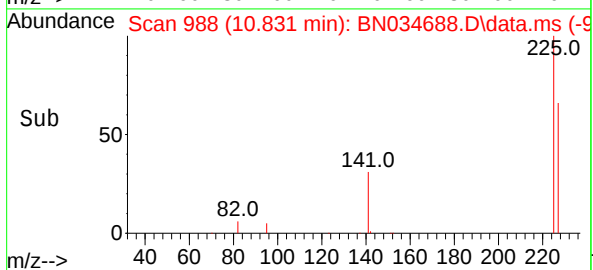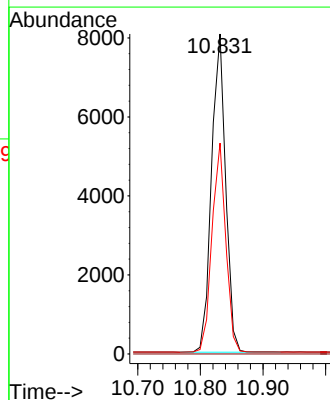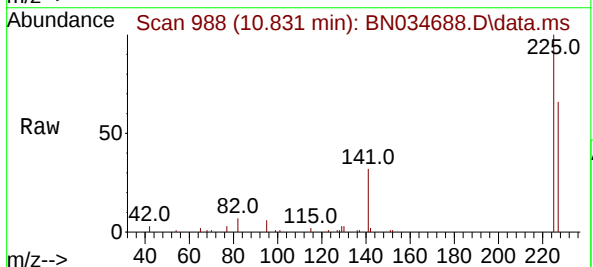



#11

2-Methylnaphthalene-d10

Concen: 1.664 ng

RT: 12.071 min Scan# 1201

Delta R.T. 0.000 min

Lab File: BN034688.D

Acq: 24 Oct 2024 11:35

Instrument :

BNA_N

ClientSampleId :





SSTDICC1.6

Tgt Ion:152 Resp: 43281

Ion Ratio Lower Upper

152 100

151 20.8 16.7 25.1

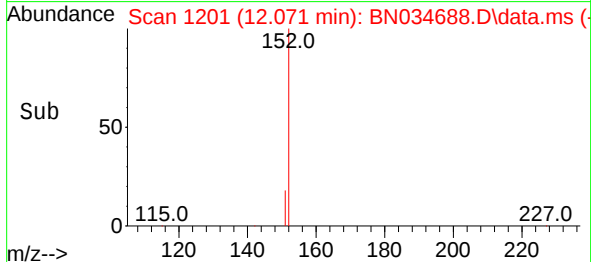

#12

2-Methylnaphthalene

Concen: 1.675 ng

RT: 12.147 min Scan# 1221

Delta R.T. 0.000 min

Lab File: BN034688.D

Acq: 24 Oct 2024 11:35




Tgt Ion:142 Resp: 53951


Ion Ratio Lower Upper

142 100

141 87.5 70.4 105.6

115 36.4 29.8 44.6


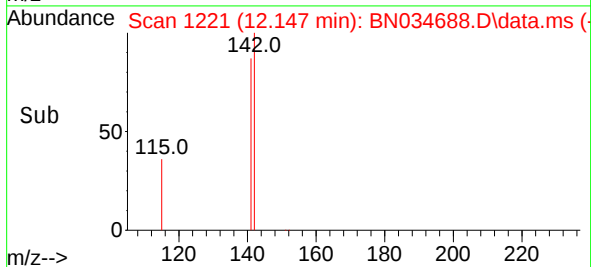

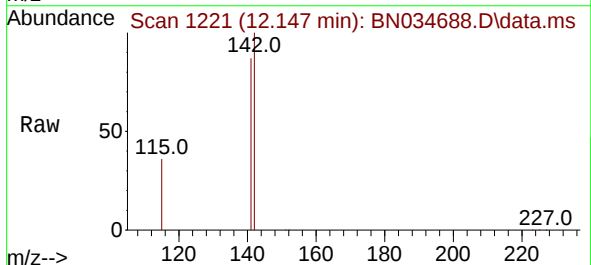




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.329 min Scan# 1504
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:164 Resp: 9335
Ion Ratio Lower Upper
164 100
162 103.4 81.4 122.0
160 50.8 40.6 61.0

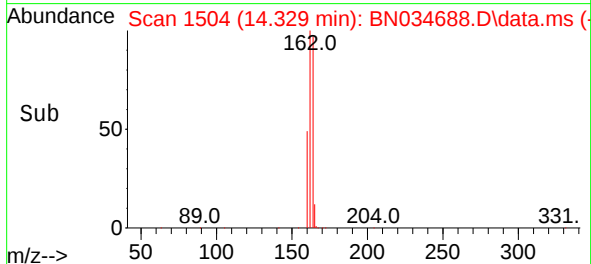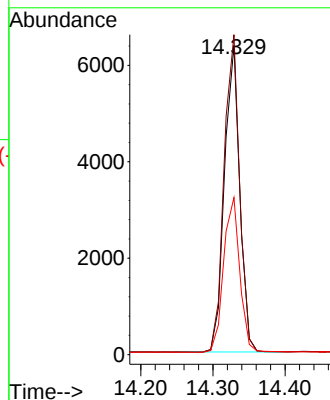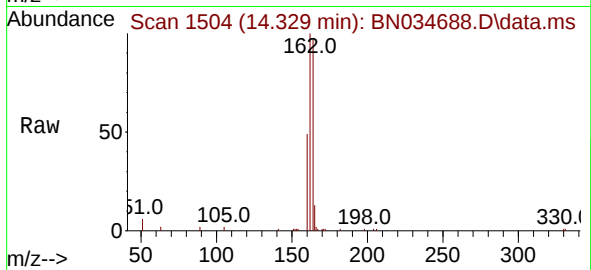

#14
2,4,6-Tribromophenol
Concen: 1.255 ng
RT: 15.815 min Scan# 1639
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35

Tgt Ion:330 Resp: 4968
Ion Ratio Lower Upper
330 100
332 95.6 76.6 115.0
141 66.4 54.6 81.8


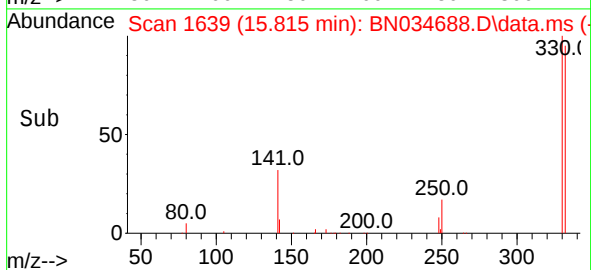
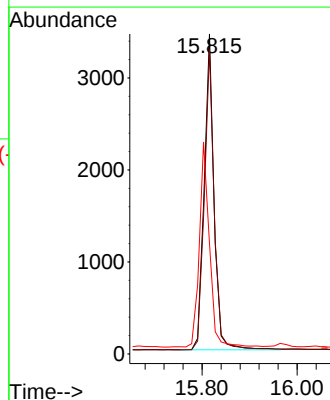
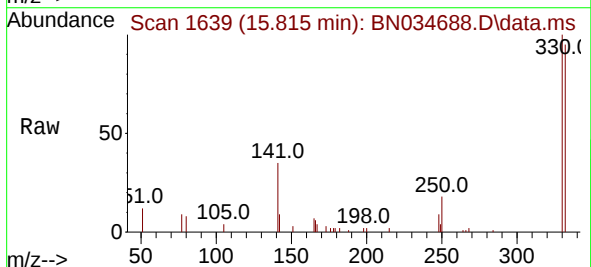


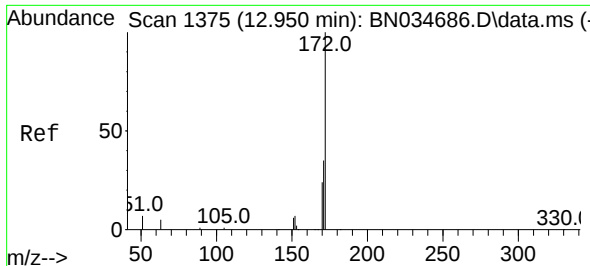

#15
2-Fluorobiphenyl
Concen: 1.691 ng
RT: 12.950 min Scan# 1375
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	172	Resp:	62224
Ion Ratio	Lower	Upper	
172	100		
171	35.5	28.3	42.5
170	24.8	19.8	29.6

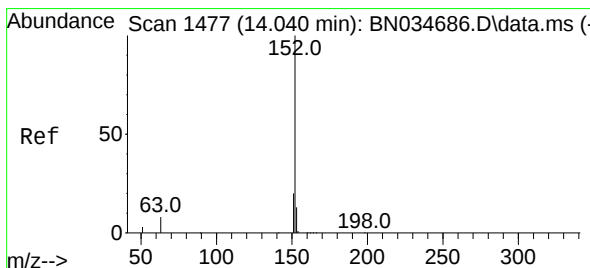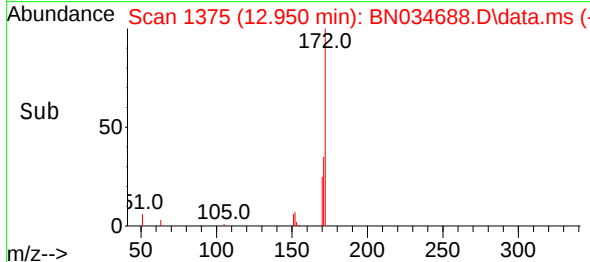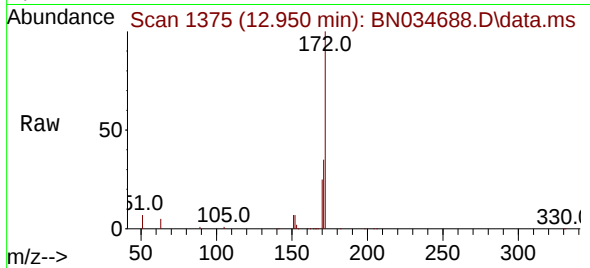

#16
Acenaphthylene
Concen: 1.696 ng
RT: 14.040 min Scan# 1477
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35

Tgt Ion:	152	Resp:	76104
Ion Ratio	Lower	Upper	
152	100		
151	19.3	15.6	23.4
153	12.9	10.6	15.8


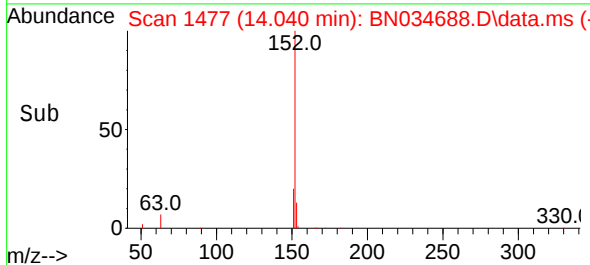

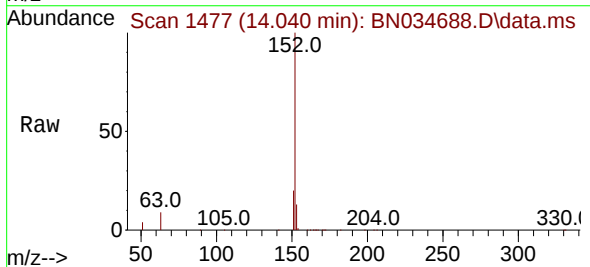




#17
Acenaphthene
Concen: 1.718 ng
RT: 14.393 min Scan# 1510
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:154 Resp: 52549
Ion Ratio Lower Upper
154 100
153 108.8 88.2 132.2
152 56.9 46.9 70.3

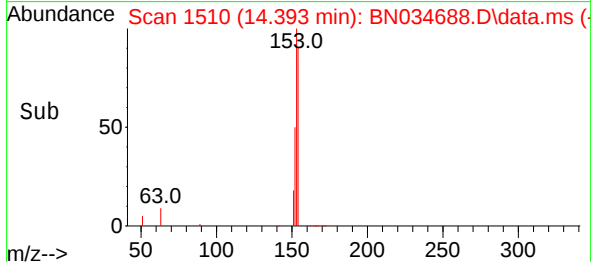

#18
Fluorene
Concen: 1.714 ng
RT: 15.377 min Scan# 1602
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35

Tgt Ion:166 Resp: 65352
Ion Ratio Lower Upper
166 100
165 98.1 78.8 118.2
167 13.2 10.6 16.0

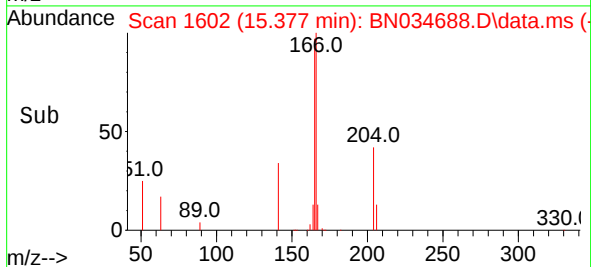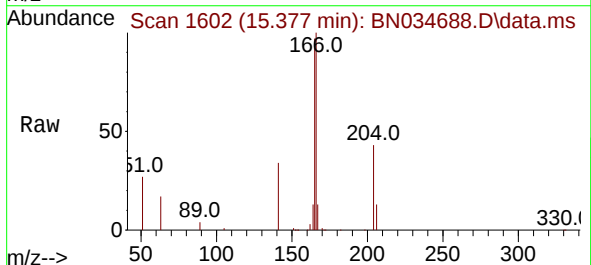

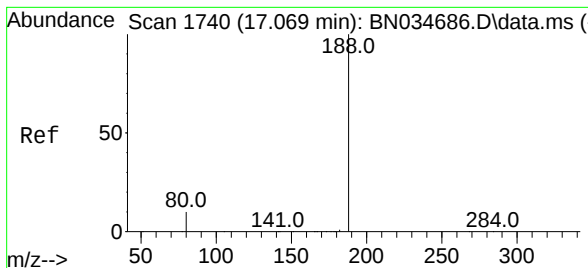

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.069 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN034688.D

Acq: 24 Oct 2024 11:35

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:188 Resp: 19334

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 11.3 8.9 13.3

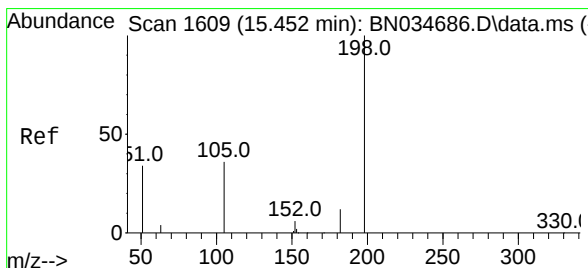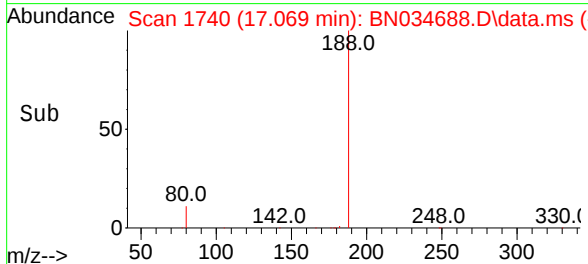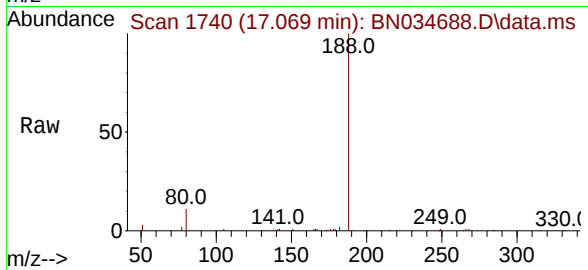

#20

4,6-Dinitro-2-methylphenol

Concen: 1.734 ng

RT: 15.452 min Scan# 1609

Delta R.T. 0.000 min

Lab File: BN034688.D

Acq: 24 Oct 2024 11:35




Tgt Ion:198 Resp: 4583


Ion Ratio Lower Upper

198 100

51 48.7 91.8 137.8#

105 35.4 44.3 66.5#


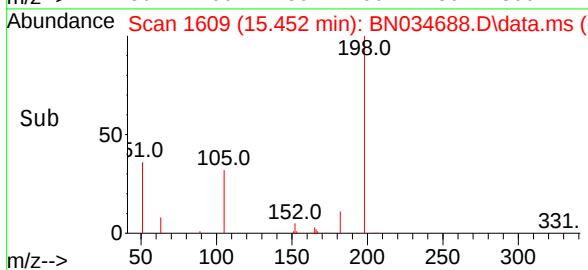

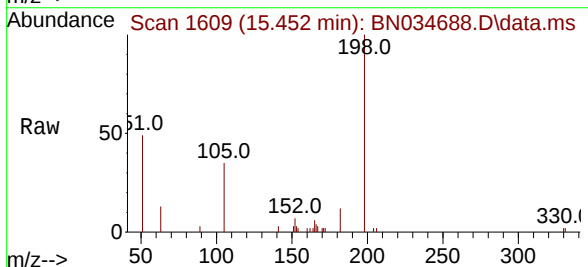




#21
4-Bromophenyl-phenylether
Concen: 1.615 ng
RT: 16.275 min Scan# 1676
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:248 Resp: 17079
Ion Ratio Lower Upper
248 100
250 101.1 80.9 121.3
141 47.4 40.5 60.7

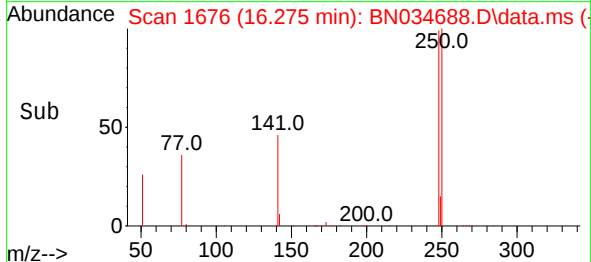

#22
Hexachlorobenzene
Concen: 1.569 ng
RT: 16.374 min Scan# 1684
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35

Tgt Ion:284 Resp: 18410
Ion Ratio Lower Upper
284 100
142 55.6 43.6 65.4
249 33.9 26.6 40.0

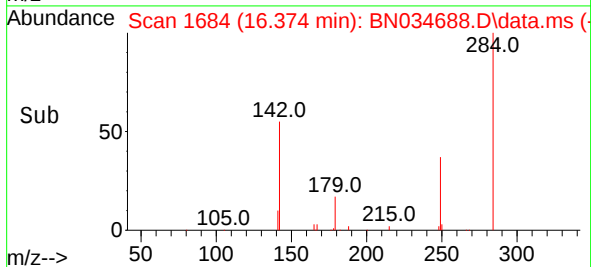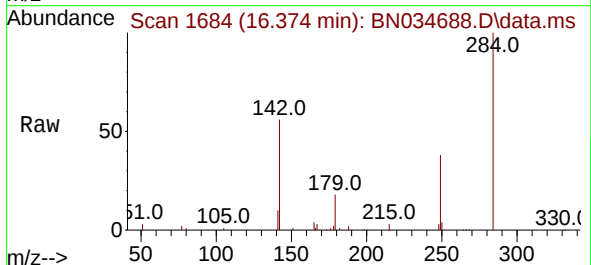

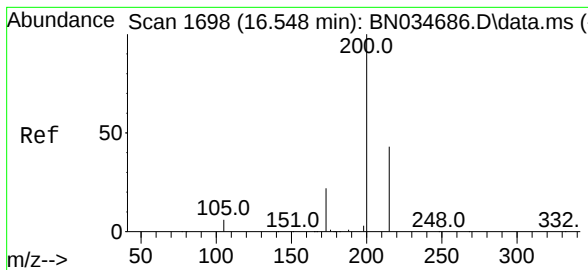

#23

Atrazine

Concen: 1.516 ng

RT: 16.548 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN034688.D

Acq: 24 Oct 2024 11:35

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:200 Resp: 14024

Ion Ratio Lower Upper

200 100

173 24.5 19.7 29.5

215 44.3 35.7 53.5

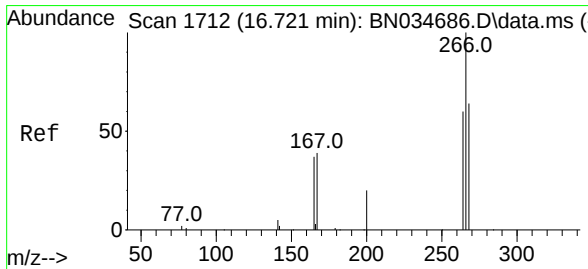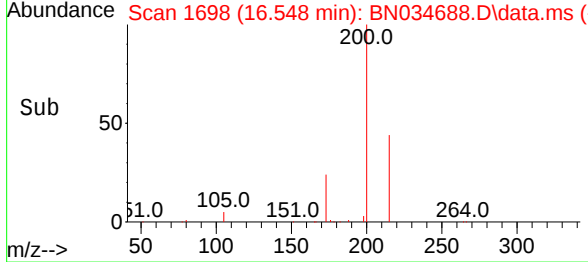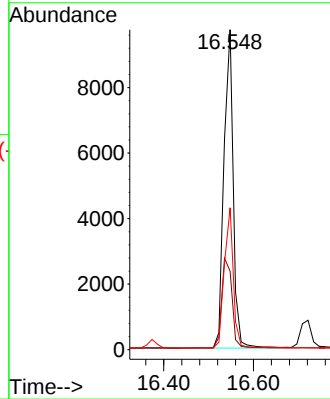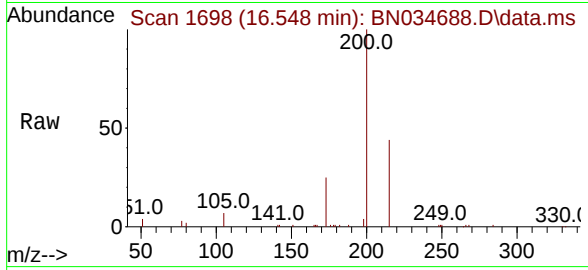

#24

Pentachlorophenol

Concen: 1.467 ng

RT: 16.721 min Scan# 1712

Delta R.T. 0.000 min

Lab File: BN034688.D

Acq: 24 Oct 2024 11:35




Tgt Ion:266 Resp: 6756


Ion Ratio Lower Upper

266 100

264 62.2 49.4 74.2

268 63.5 50.5 75.7


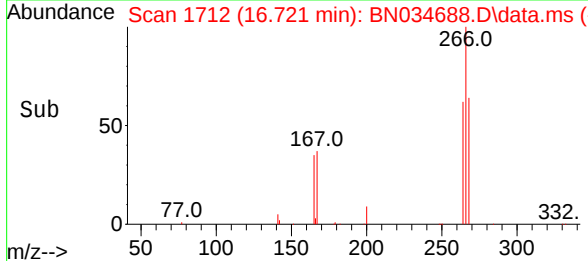
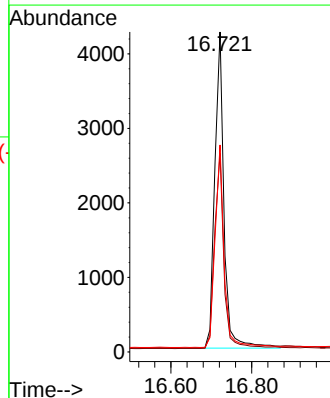
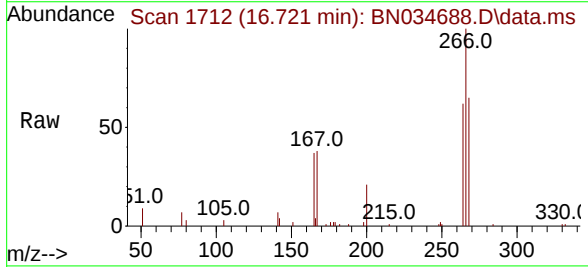


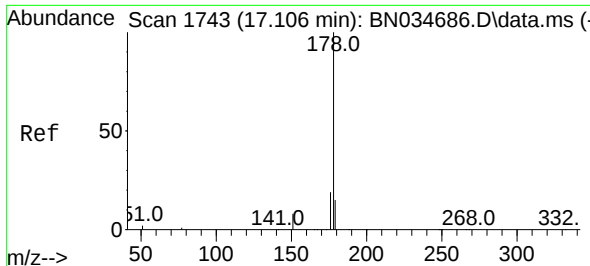

#25
Phenanthrene
Concen: 1.673 ng
RT: 17.106 min Scan# 1743
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:178 Resp: 96240
Ion Ratio Lower Upper
178 100
176 19.2 15.4 23.2
179 15.2 12.2 18.4

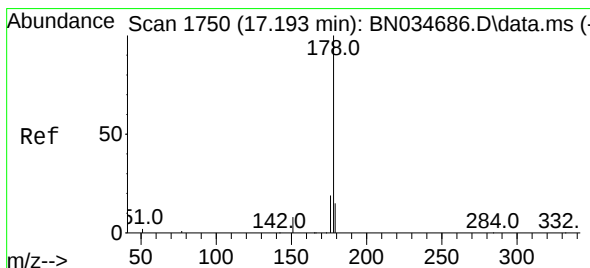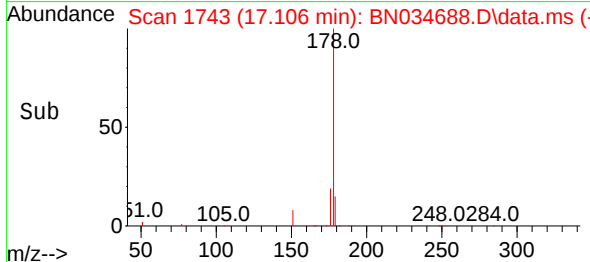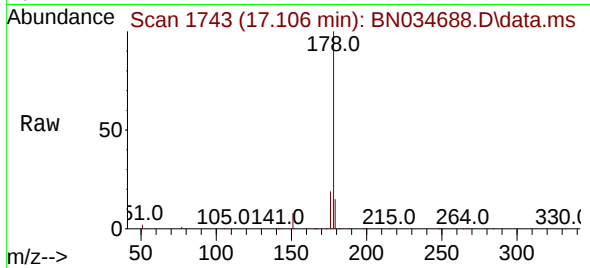

#26
Anthracene
Concen: 1.695 ng
RT: 17.193 min Scan# 1750
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35

Tgt Ion:178 Resp: 87194
Ion Ratio Lower Upper
178 100
176 18.7 14.9 22.3
179 15.1 12.2 18.2

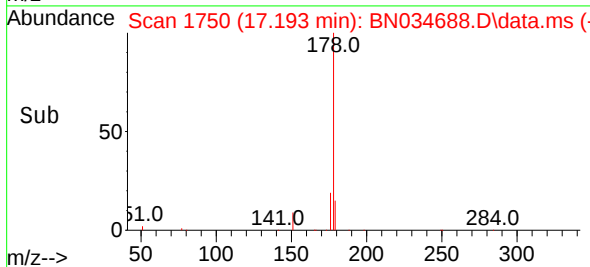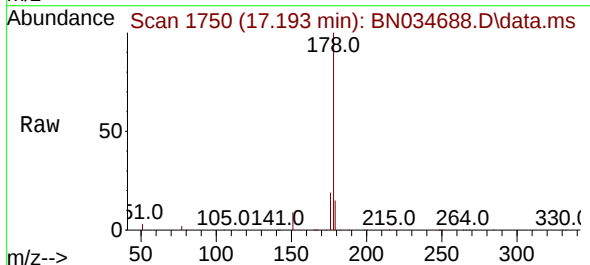

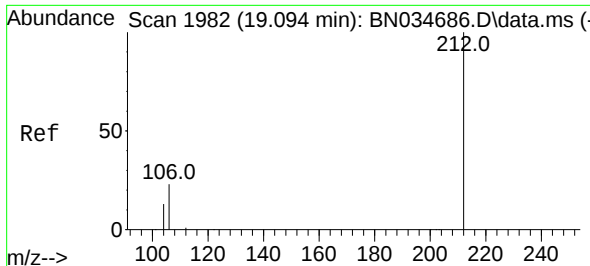

#27

Fluoranthene-d10

Concen: 1.553 ng

RT: 19.094 min Scan# 1982

Delta R.T. 0.000 min

Lab File: BN034688.D

Acq: 24 Oct 2024 11:35

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:212 Resp: 73515

Ion Ratio Lower Upper

212 100

106 22.2 17.8 26.8

104 12.6 10.2 15.4

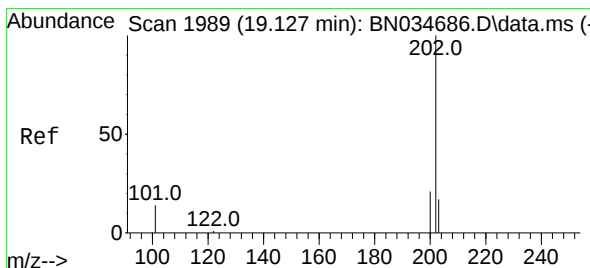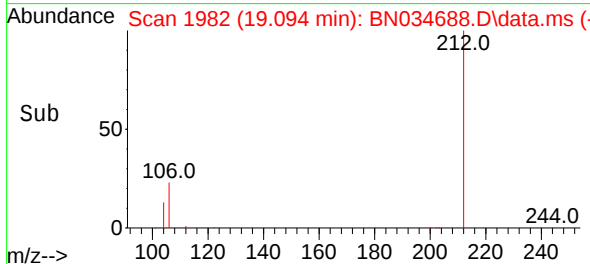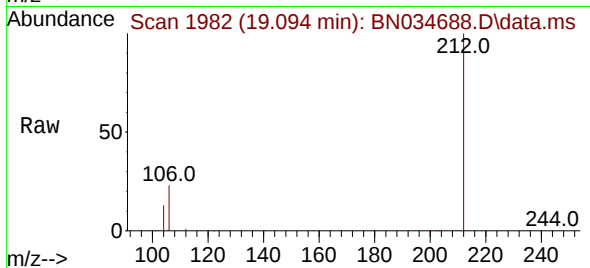

#28

Fluoranthene

Concen: 1.598 ng

RT: 19.127 min Scan# 1989

Delta R.T. 0.000 min

Lab File: BN034688.D

Acq: 24 Oct 2024 11:35




Tgt Ion:202 Resp: 103093


Ion Ratio Lower Upper

202 100

101 16.0 12.8 19.2

203 17.2 13.5 20.3

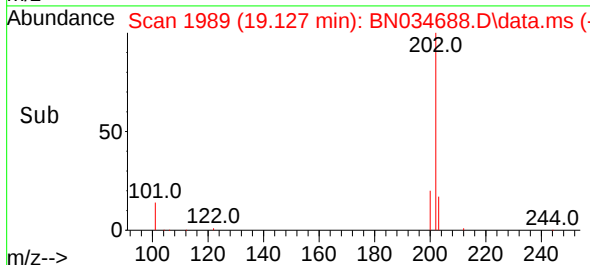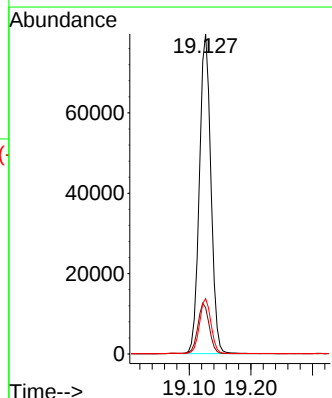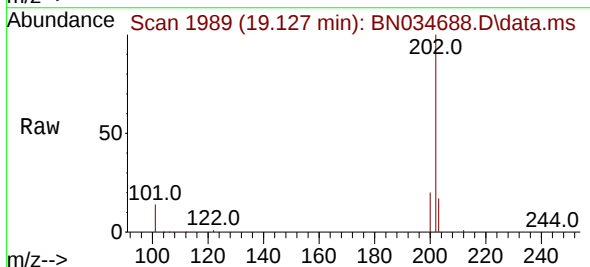

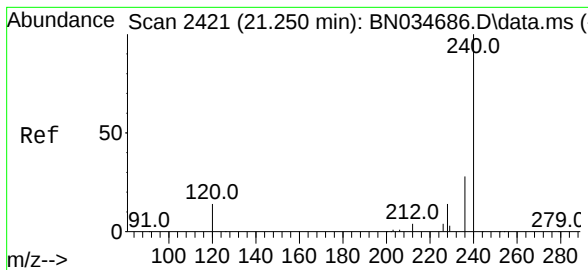

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.250 min Scan# 2421

Delta R.T. 0.000 min

Lab File: BN034688.D

Acq: 24 Oct 2024 11:35

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:240 Resp: 11924

Ion Ratio Lower Upper

240 100

120 18.2 14.2 21.2

236 28.6 23.1 34.7

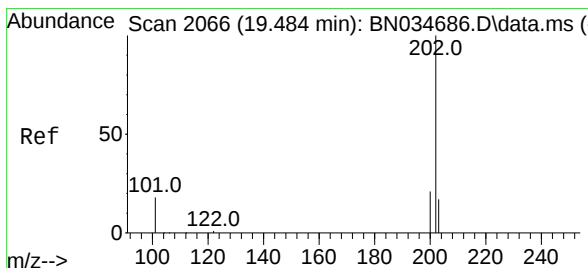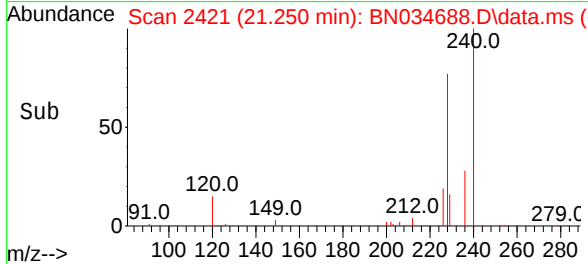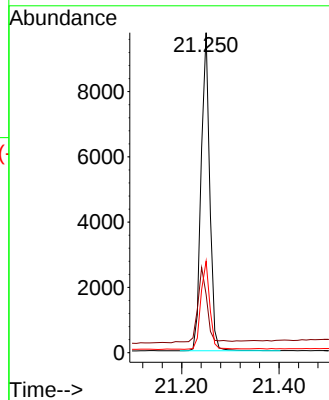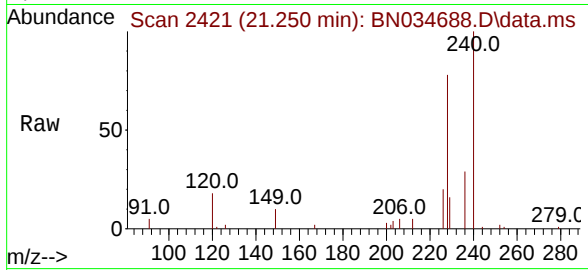

#30

Pyrene

Concen: 1.936 ng

RT: 19.489 min Scan# 2067

Delta R.T. 0.005 min

Lab File: BN034688.D

Acq: 24 Oct 2024 11:35




Tgt Ion:202 Resp: 103194


Ion Ratio Lower Upper

202 100

200 21.0 16.6 25.0

203 17.7 14.2 21.4


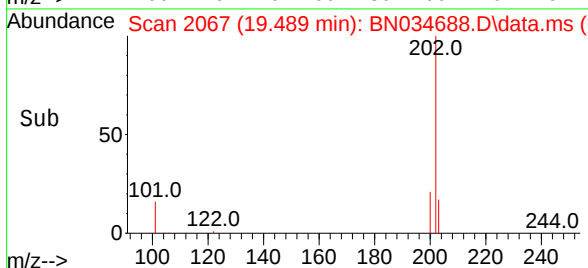
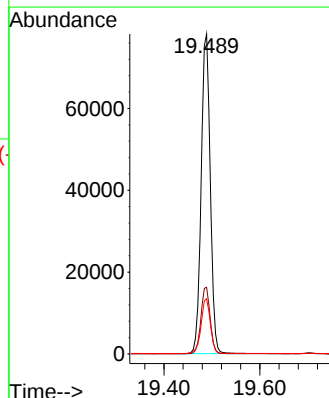
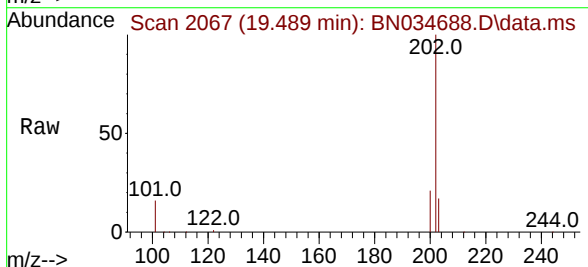




#31
 Terphenyl-d14
 Concen: 1.788 ng
 RT: 19.703 min Scan# 2113
 Delta R.T. 0.000 min
 Lab File: BN034688.D
 Acq: 24 Oct 2024 11:35




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:244 Resp: 41261
 Ion Ratio Lower Upper
 244 100
 212 10.5 8.6 13.0
 122 28.7 22.3 33.5

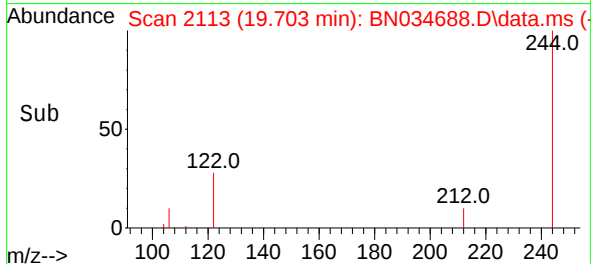

#32
 Benzo(a)anthracene
 Concen: 1.693 ng
 RT: 21.232 min Scan# 2419
 Delta R.T. 0.000 min
 Lab File: BN034688.D
 Acq: 24 Oct 2024 11:35

Tgt Ion:228 Resp: 76954
 Ion Ratio Lower Upper
 228 100
 226 27.4 22.0 33.0
 229 19.1 15.6 23.4


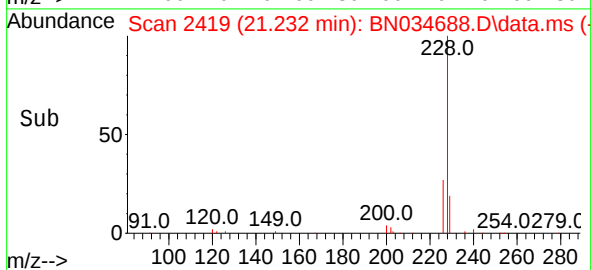

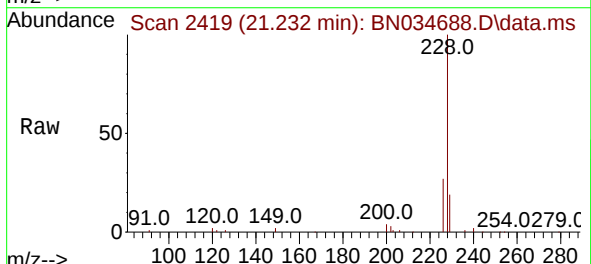


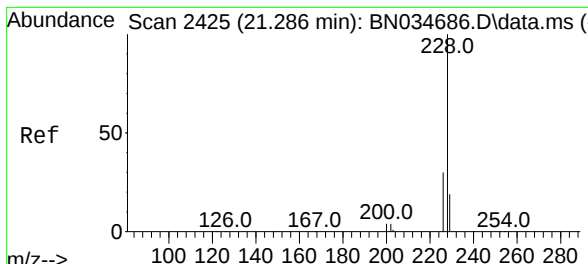

#33
 Chrysene
 Concen: 1.741 ng
 RT: 21.286 min Scan# 2425
 Delta R.T. 0.000 min
 Lab File: BN034688.D
 Acq: 24 Oct 2024 11:35




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:	228	Resp:	78358
Ion Ratio	Lower	Upper	
228	100		
226	30.4	24.1	36.1
229	19.1	15.8	23.8

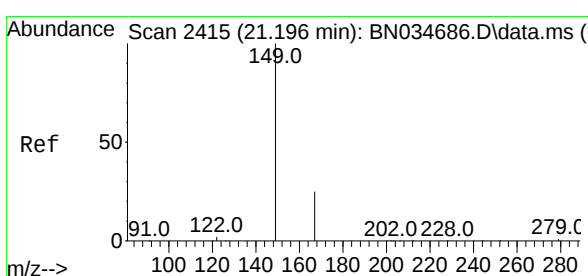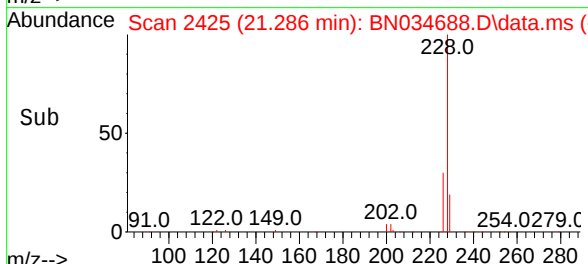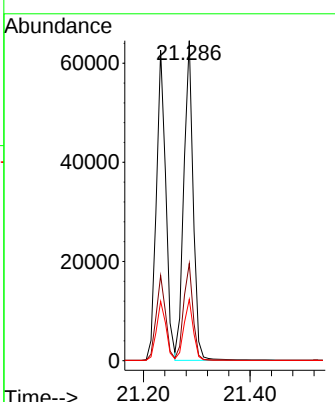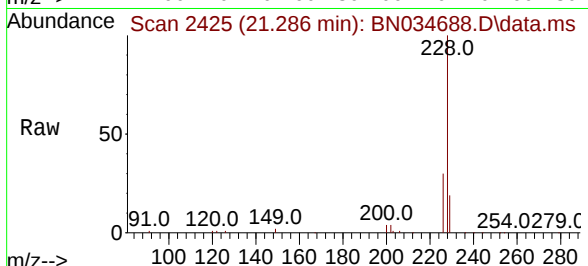

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 1.354 ng
 RT: 21.196 min Scan# 2415
 Delta R.T. 0.000 min
 Lab File: BN034688.D
 Acq: 24 Oct 2024 11:35

Tgt Ion:	149	Resp:	41892
Ion Ratio	Lower	Upper	
149	100		
167	24.7	19.7	29.5
279	1.7	1.8	2.6


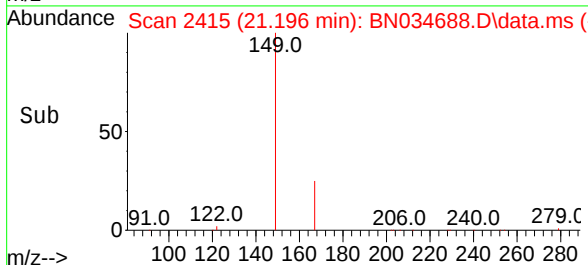
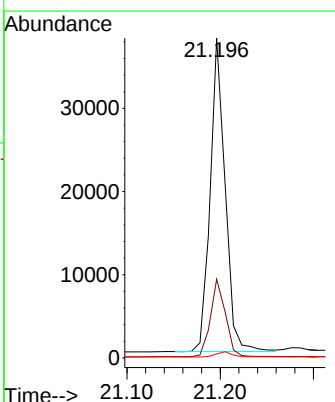
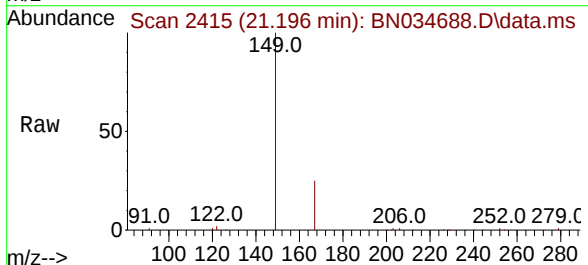


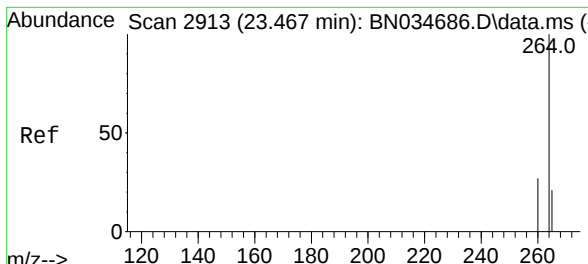

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.467 min Scan# 2913
 Delta R.T. 0.000 min
 Lab File: BN034688.D
 Acq: 24 Oct 2024 11:35




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:	264	Resp:	10103
Ion Ratio	Lower	Upper	
264	100		
260	26.9	21.9	32.9
265	75.7	60.6	91.0

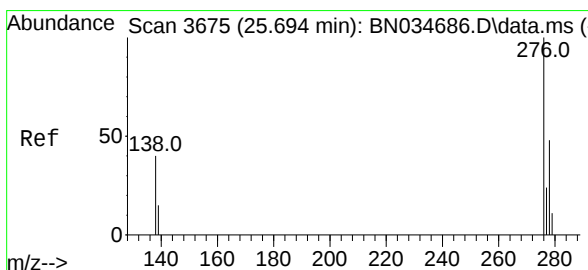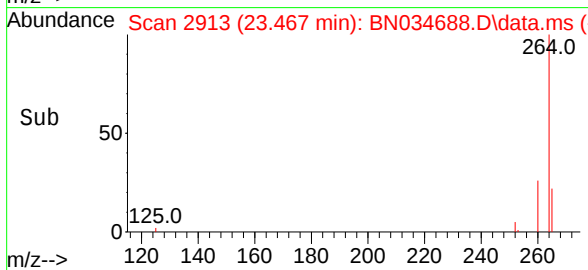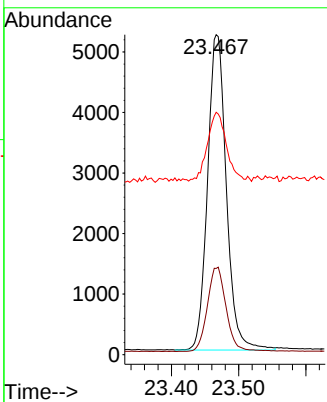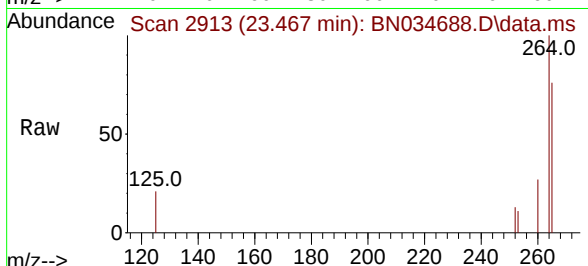

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 1.682 ng
 RT: 25.697 min Scan# 3676
 Delta R.T. 0.003 min
 Lab File: BN034688.D
 Acq: 24 Oct 2024 11:35

Tgt Ion:	276	Resp:	65482
Ion Ratio	Lower	Upper	
276	100		
138	43.4	35.1	52.7
277	24.3	19.7	29.5

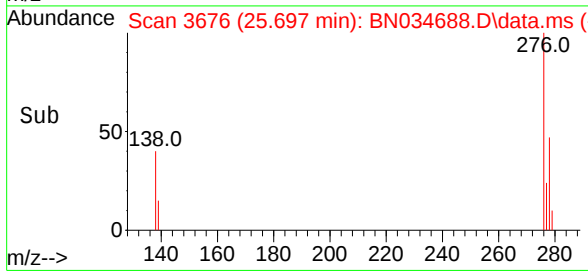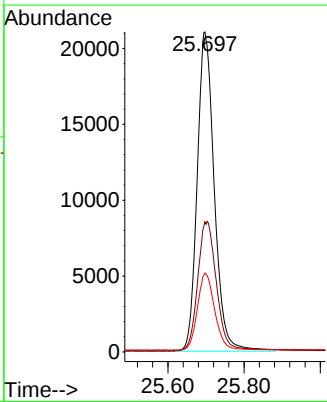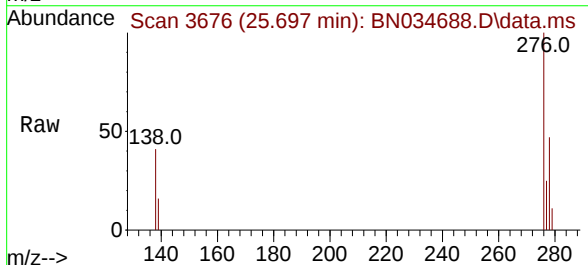



#37

Benzo(b)fluoranthene

Concen: 1.880 ng

RT: 22.803 min Scan# 2686

Delta R.T. 0.000 min

Lab File: BN034688.D

Acq: 24 Oct 2024 11:35

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:252 Resp: 68644

Ion Ratio Lower Upper

252 100

253 22.3 20.0 30.0

125 18.9 20.9 31.3#

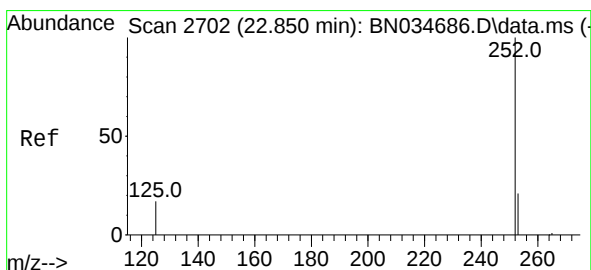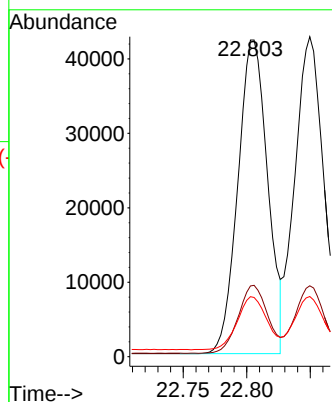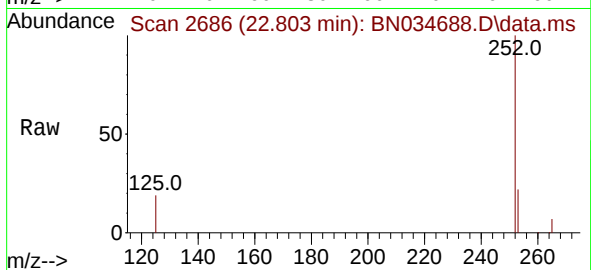

#38

Benzo(k)fluoranthene

Concen: 1.942 ng

RT: 22.850 min Scan# 2702

Delta R.T. 0.000 min

Lab File: BN034688.D

Acq: 24 Oct 2024 11:35




Tgt Ion:252 Resp: 69183


Ion Ratio Lower Upper

252 100

253 22.1 20.6 31.0

125 18.8 21.6 32.4#

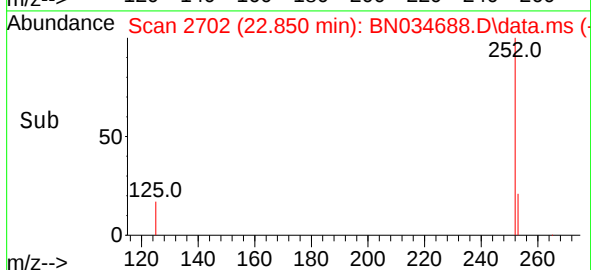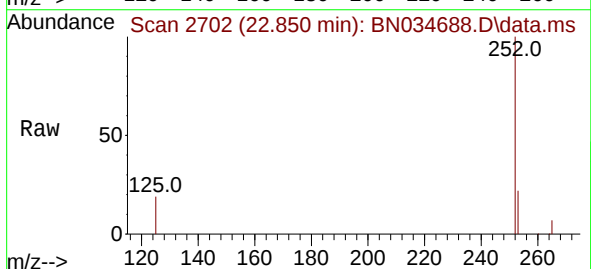



#39

Benzo(a)pyrene

Concen: 1.802 ng

RT: 23.370 min Scan# 21

Delta R.T. 0.003 min

Lab File: BN034688.D


Acq: 24 Oct 2024 11:35

Instrument :

BN034688.D

ClientSampleId :

SSTDICC1.6






Tgt Ion:252 Resp: 55896

Ion Ratio Lower Upper

252 100

253 22.8 22.2 33.4

125 21.7 26.0 39.0#

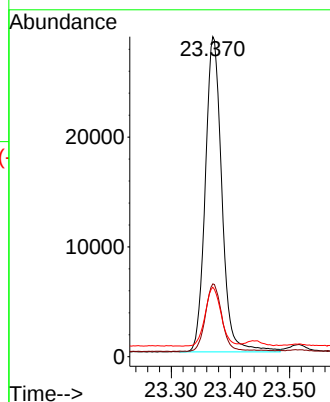

#40

Dibenzo(a,h)anthracene

Concen: 1.696 ng

RT: 25.715 min Scan# 3682

Delta R.T. 0.000 min

Lab File: BN034688.D

Acq: 24 Oct 2024 11:35




Tgt Ion:278 Resp: 51867


Ion Ratio Lower Upper

278 100

139 29.7 25.4 38.2


279 24.2 22.4 33.6

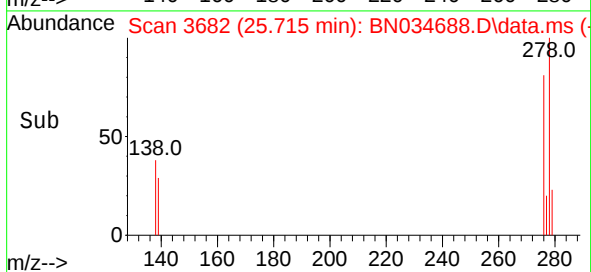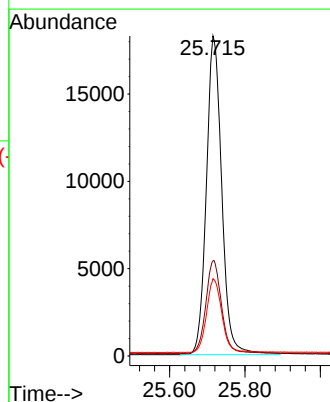

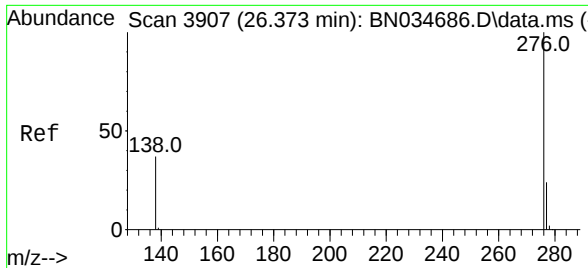

#41
Benzo(g,h,i)perylene
Concen: 1.661 ng
RT: 26.373 min Scan# 3907
Delta R.T. 0.000 min
Lab File: BN034688.D
Acq: 24 Oct 2024 11:35

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

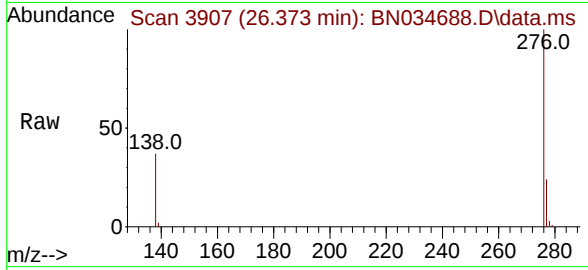

Tgt Ion:276 Resp: 56042
Ion Ratio Lower Upper
276 100
277 23.8 21.3 31.9
138 37.5 31.9 47.9

