

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102424\
 Data File : BN034702.D
 Acq On : 24 Oct 2024 21:38
 Operator : RC/JU
 Sample : PB164230BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB164230BL

Quant Time: Oct 25 02:07:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 24 13:17:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.712	152	6089	0.400	ng	0.00
7) Naphthalene-d8	10.479	136	16910	0.400	ng	0.00
13) Acenaphthene-d10	14.329	164	7332	0.400	ng	0.00
19) Phenanthrene-d10	17.069	188	12991	0.400	ng	0.00
29) Chrysene-d12	21.241	240	7046	0.400	ng	# 0.00
35) Perylene-d12	23.461	264	6436	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.322	112	5589	0.309	ng	0.00
5) Phenol-d6	6.882	99	7556	0.317	ng	0.00
8) Nitrobenzene-d5	8.845	82	4807	0.339	ng	0.00
11) 2-Methylnaphthalene-d10	12.071	152	7776	0.334	ng	0.00
14) 2,4,6-Tribromophenol	15.815	330	482	0.213	ng	0.00
15) 2-Fluorobiphenyl	12.950	172	10830	0.372	ng	0.00
27) Fluoranthene-d10	19.094	212	9762	0.334	ng	0.00
31) Terphenyl-d14	19.703	244	5518	0.383	ng	0.00
Target Compounds						
34) Bis(2-ethylhexyl)phtha...	21.196	149	397	0.026	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102424\
Data File : BN034702.D
Acq On : 24 Oct 2024 21:38
Operator : RC/JU
Sample : PB164230BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB164230BL


Quant Time: Oct 25 02:07:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 24 13:17:02 2024
Response via : Initial Calibration

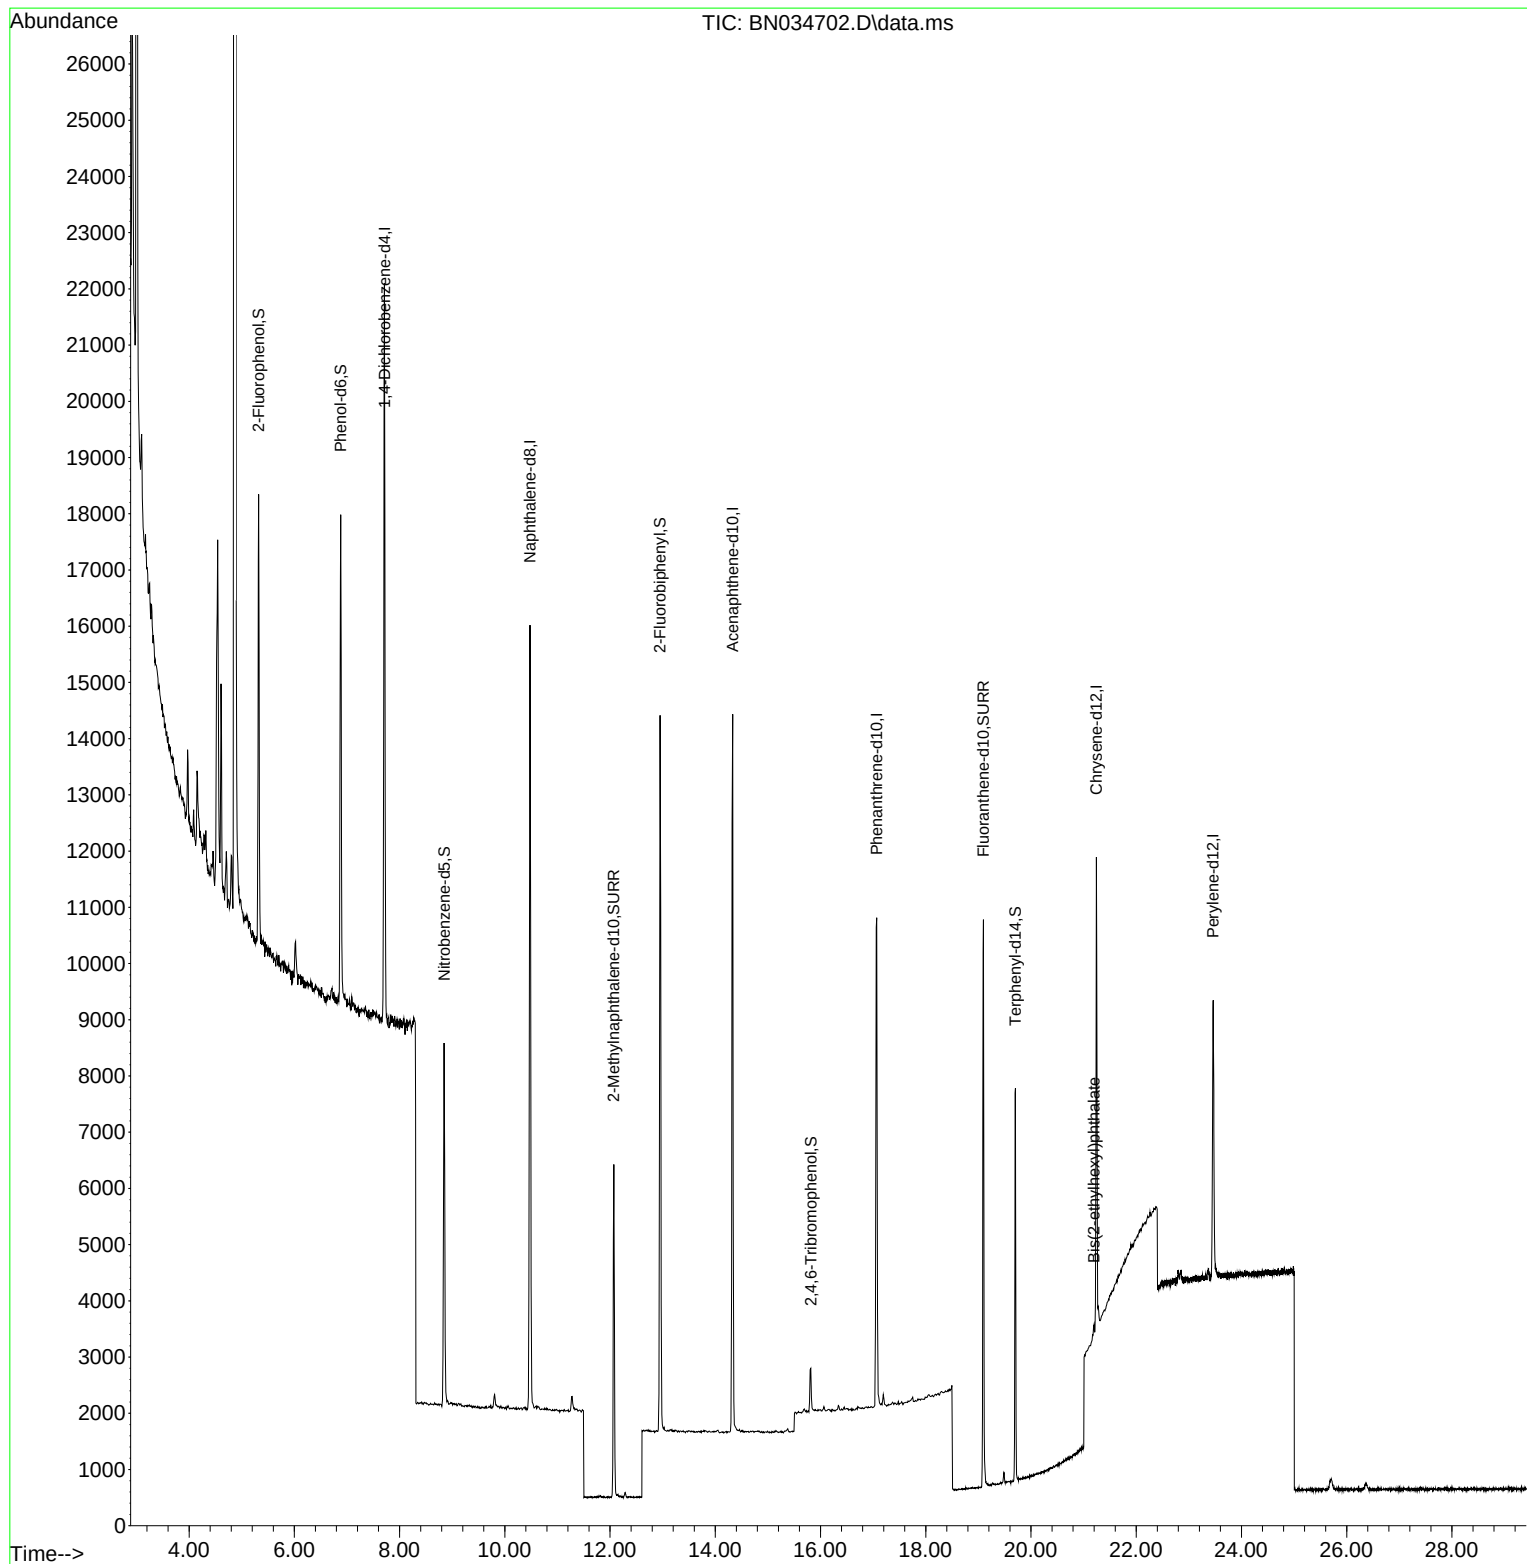



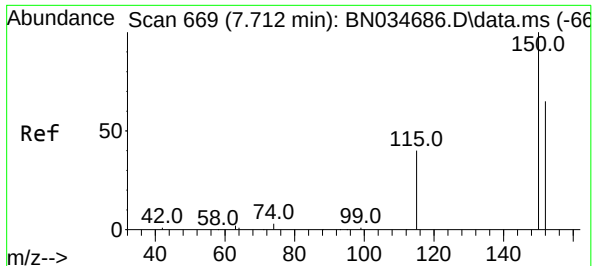


#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.712 min Scan# 669
Delta R.T. 0.000 min
Lab File: BN034702.D
Acq: 24 Oct 2024 21:38


Instrument :
BNA_N
ClientSampleId :
PB164230BL

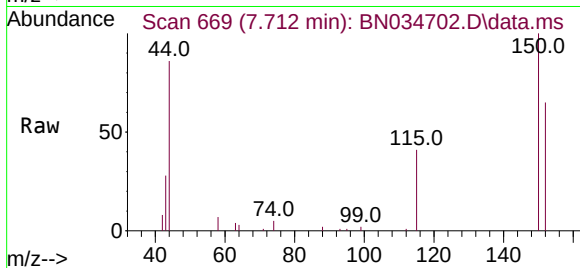



Tgt Ion:152 Resp: 6089
Ion Ratio Lower Upper
152 100
150 153.3 122.7 184.1
115 62.3 51.0 76.6

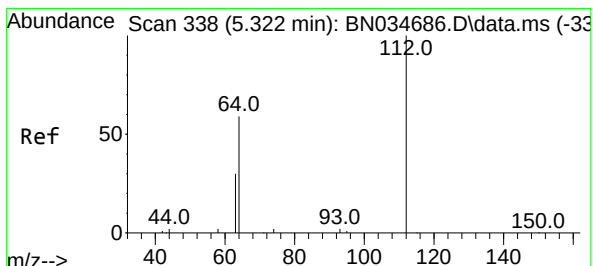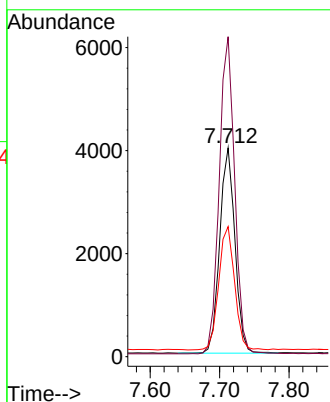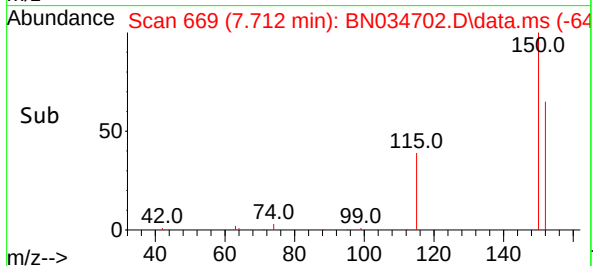


#4
2-Fluorophenol
Concen: 0.309 ng
RT: 5.322 min Scan# 338
Delta R.T. 0.000 min
Lab File: BN034702.D
Acq: 24 Oct 2024 21:38

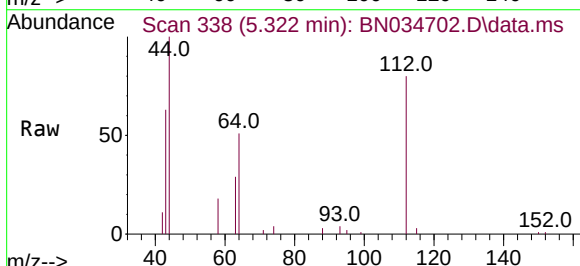

Tgt Ion:112 Resp: 5589
Ion Ratio Lower Upper
112 100
64 66.6 53.0 79.6
63 36.7 27.6 41.4



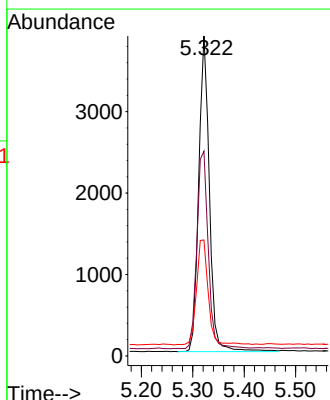
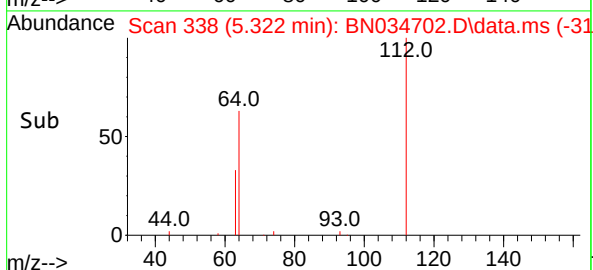


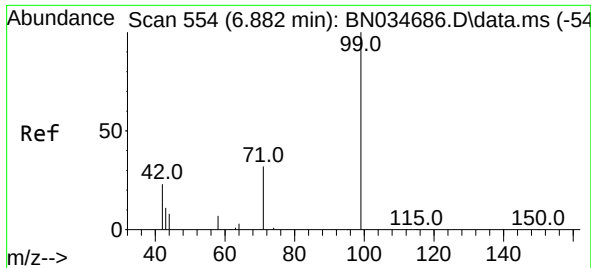

#5
Phenol-d6
Concen: 0.317 ng
RT: 6.882 min Scan# 511
Delta R.T. 0.000 min
Lab File: BN034702.D
Acq: 24 Oct 2024 21:38




Instrument :
BNA_N
ClientSampleId :
PB164230BL


Tgt Ion: 99 Resp: 7556
Ion Ratio Lower Upper
99 100
42 27.2 21.8 32.8
71 33.2 26.6 40.0

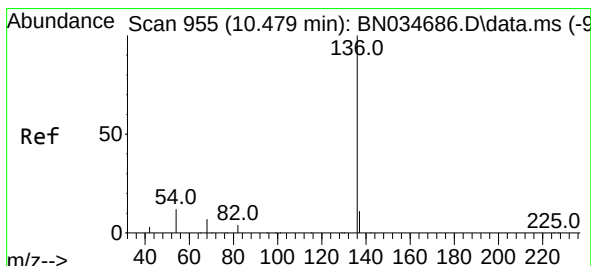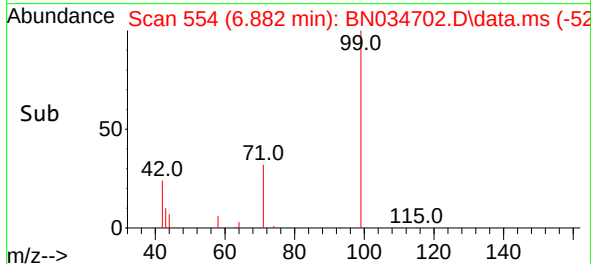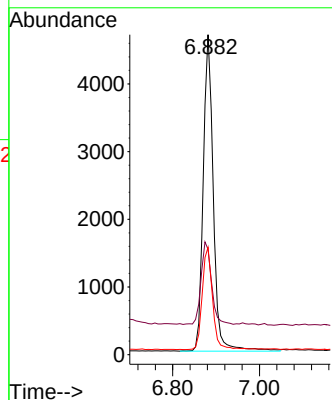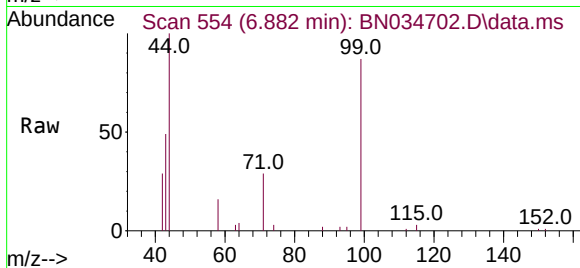

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.479 min Scan# 955
Delta R.T. 0.000 min
Lab File: BN034702.D
Acq: 24 Oct 2024 21:38

Tgt Ion: 136 Resp: 16910
Ion Ratio Lower Upper
136 100
137 11.5 9.1 13.7
54 12.1 9.8 14.8
68 7.9 6.4 9.6


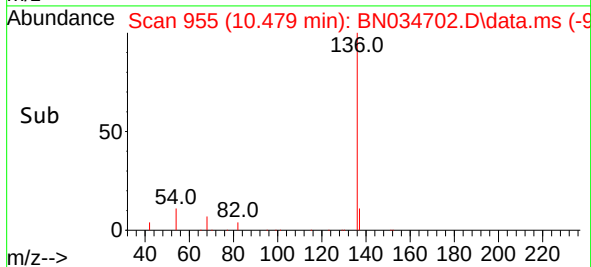
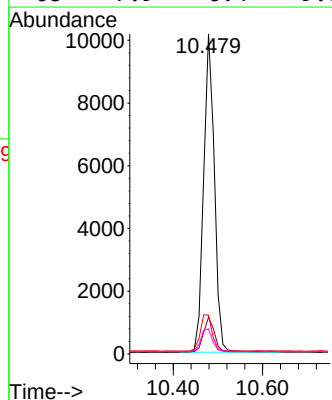
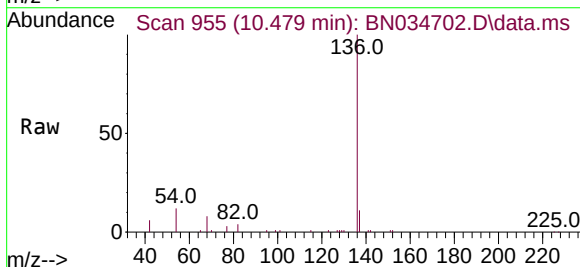


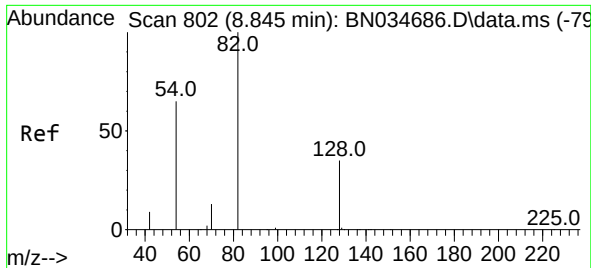

#8
Nitrobenzene-d5
Concen: 0.339 ng
RT: 8.845 min Scan# 802
Delta R.T. 0.000 min
Lab File: BN034702.D
Acq: 24 Oct 2024 21:38




Instrument :
BNA_N
ClientSampleId :
PB164230BL


Tgt Ion: 82 Resp: 4807
Ion Ratio Lower Upper
82 100
128 36.4 29.7 44.5
54 66.7 53.0 79.6

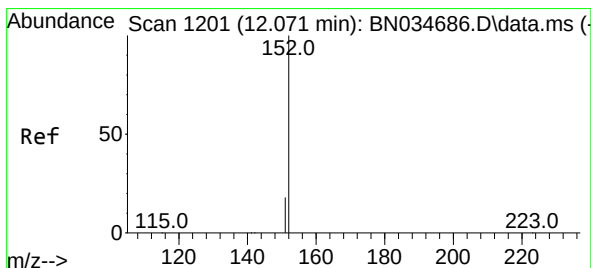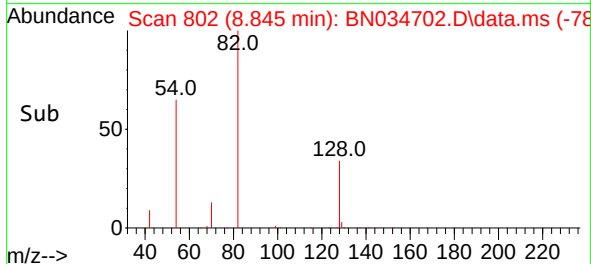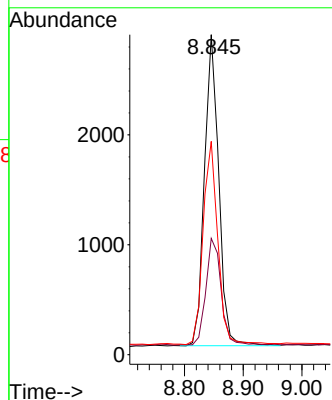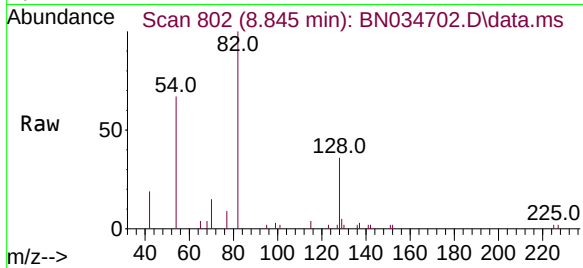

#11
2-Methylnaphthalene-d10
Concen: 0.334 ng
RT: 12.071 min Scan# 1201
Delta R.T. 0.000 min
Lab File: BN034702.D
Acq: 24 Oct 2024 21:38

Tgt Ion: 152 Resp: 7776
Ion Ratio Lower Upper
152 100
151 20.6 16.7 25.1

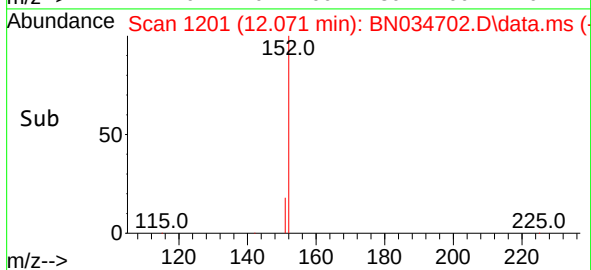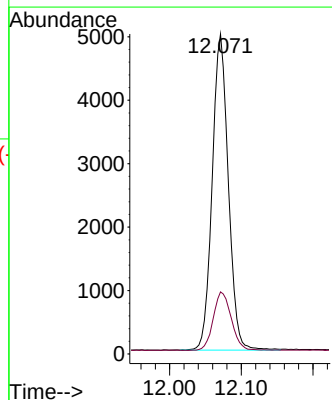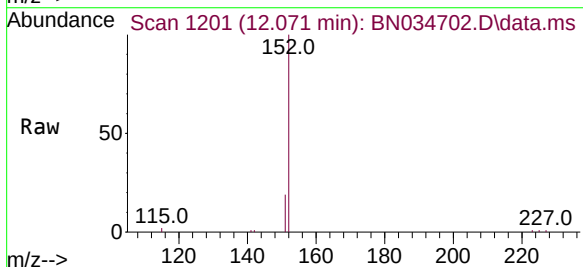

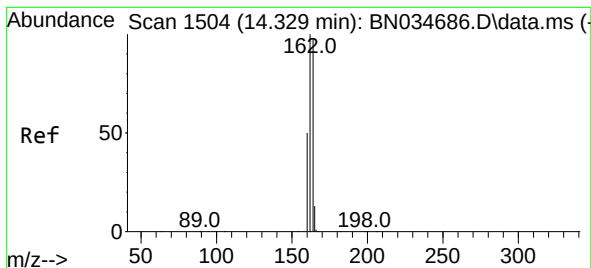

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.329 min Scan# 1504

Delta R.T. 0.000 min

Lab File: BN034702.D

Acq: 24 Oct 2024 21:38

Instrument :

BNA_N

ClientSampleId :

PB164230BL





Tgt Ion:164 Resp: 7332

Ion Ratio Lower Upper

164 100

162 103.3 81.4 122.0

160 52.5 40.6 61.0

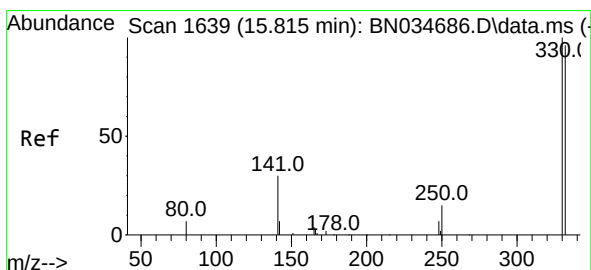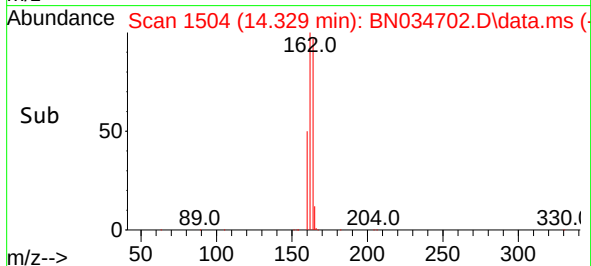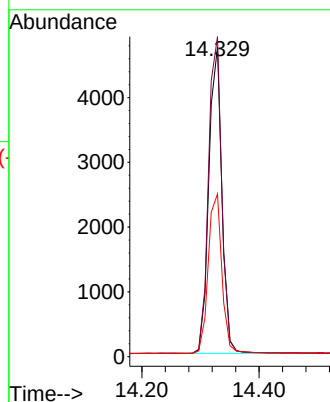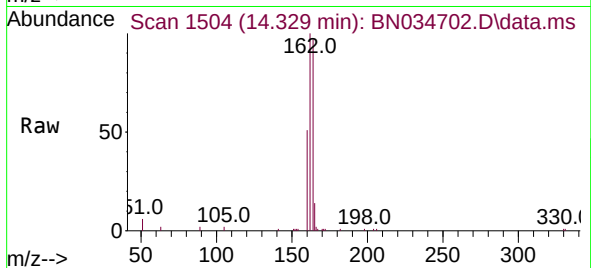

#14

2,4,6-Tribromophenol

Concen: 0.213 ng

RT: 15.815 min Scan# 1639

Delta R.T. 0.000 min

Lab File: BN034702.D

Acq: 24 Oct 2024 21:38




Tgt Ion:330 Resp: 482


Ion Ratio Lower Upper

330 100

332 91.1 76.6 115.0

141 71.2 54.6 81.8


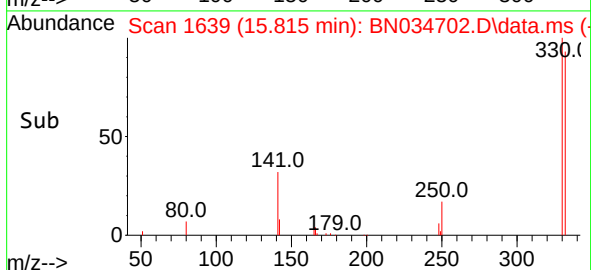
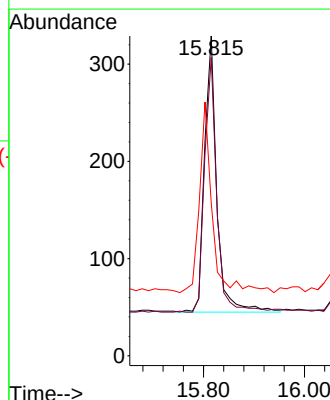
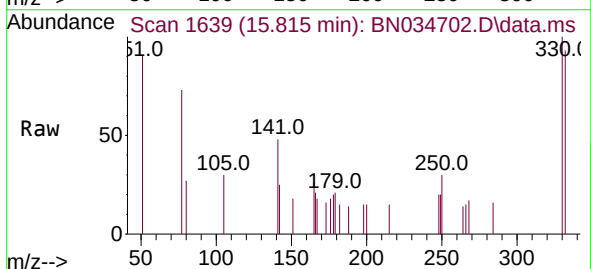


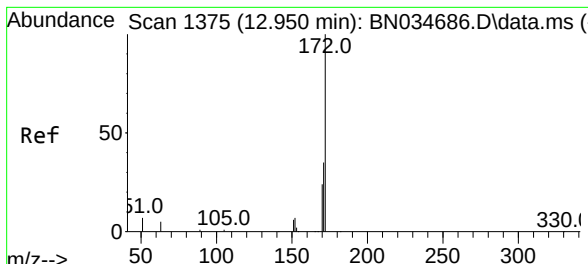

#15
 2-Fluorobiphenyl
 Concen: 0.372 ng
 RT: 12.950 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN034702.D
 Acq: 24 Oct 2024 21:38




Instrument :
 BNA_N
 ClientSampleId :
 PB164230BL


Tgt Ion:	172	Resp:	10830
Ion	Ratio	Lower	Upper
172	100		
171	34.7	28.3	42.5
170	24.8	19.8	29.6

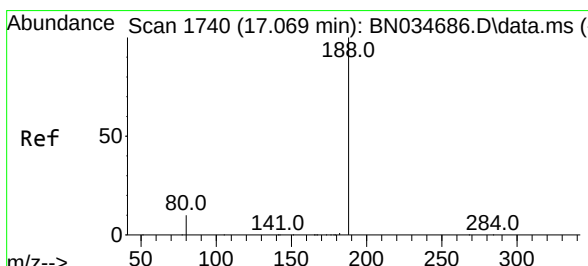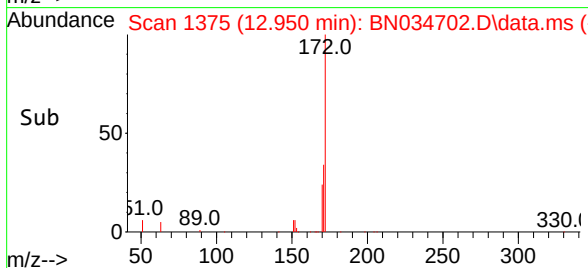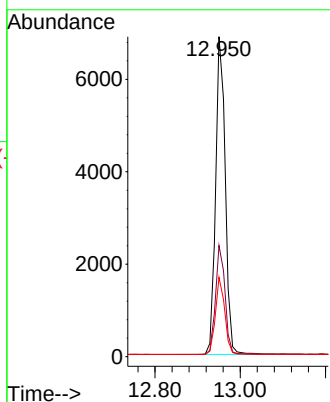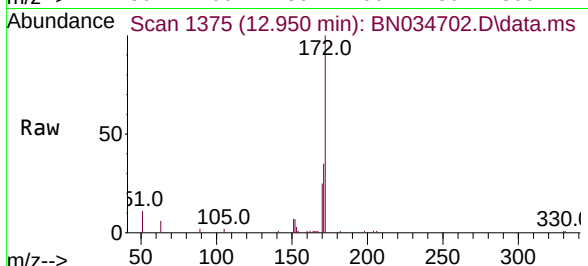

#19
 Phenanthrene-d10
 Concen: 0.400 ng
 RT: 17.069 min Scan# 1740
 Delta R.T. -0.000 min
 Lab File: BN034702.D
 Acq: 24 Oct 2024 21:38

Tgt Ion:	188	Resp:	12991
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	11.2	8.9	13.3


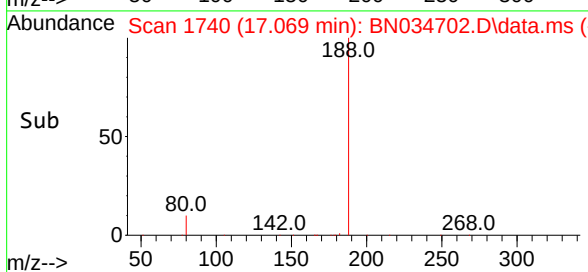
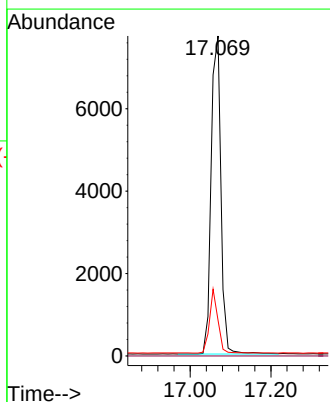
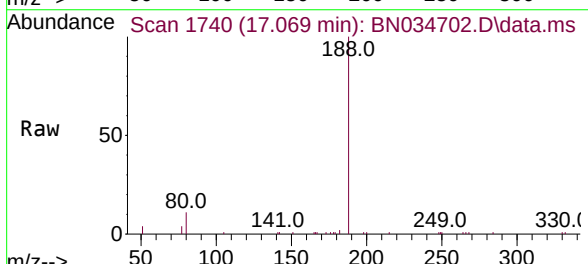


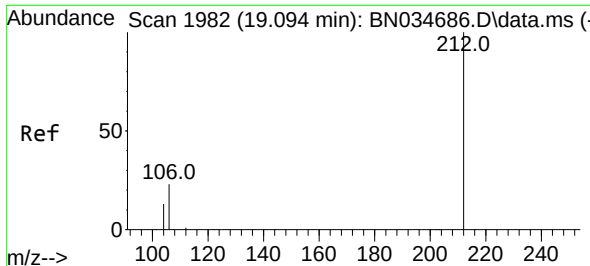

#27
Fluoranthene-d10
Concen: 0.334 ng
RT: 19.094 min Scan# 1982
Delta R.T. 0.000 min
Lab File: BN034702.D
Acq: 24 Oct 2024 21:38




Instrument :
BNA_N
ClientSampleId :
PB164230BL


Tgt Ion:212 Resp: 9762
Ion Ratio Lower Upper
212 100
106 23.3 17.8 26.8
104 13.7 10.2 15.4

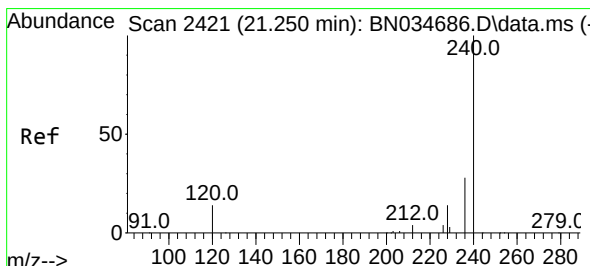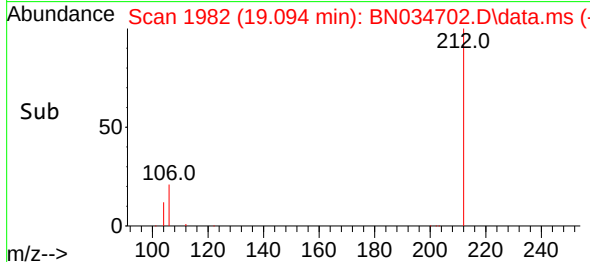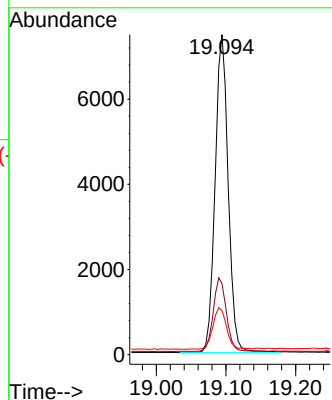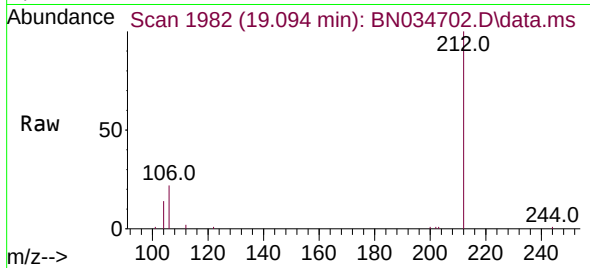

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.241 min Scan# 2420
Delta R.T. -0.009 min
Lab File: BN034702.D
Acq: 24 Oct 2024 21:38

Tgt Ion:240 Resp: 7046
Ion Ratio Lower Upper
240 100
120 33.2 14.2 21.2#
236 31.7 23.1 34.7

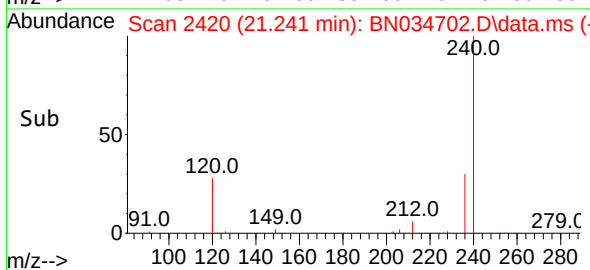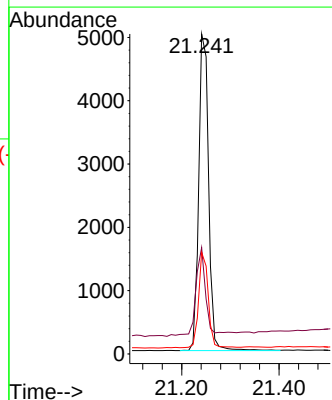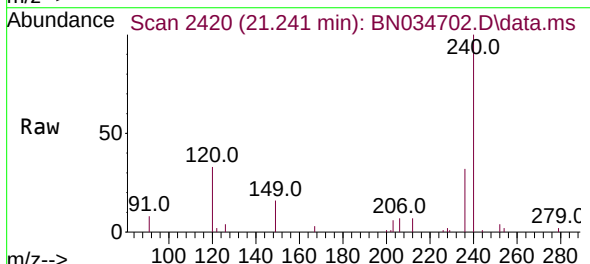

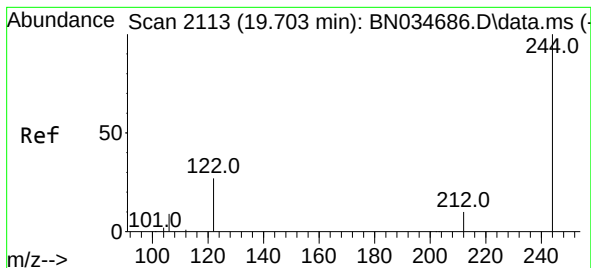

#31

Terphenyl-d14

Concen: 0.383 ng

RT: 19.703 min Scan# 2113

Delta R.T. 0.000 min

Lab File: BN034702.D

Acq: 24 Oct 2024 21:38

Instrument :

BNA_N

ClientSampleId :

PB164230BL





Tgt Ion:244 Resp: 5518

Ion Ratio Lower Upper

244 100

212 11.4 8.6 13.0

122 27.0 22.3 33.5

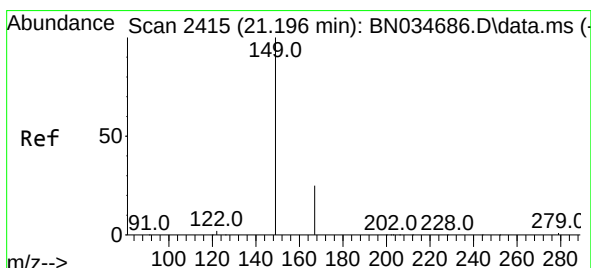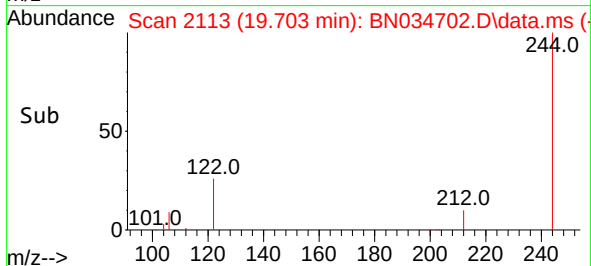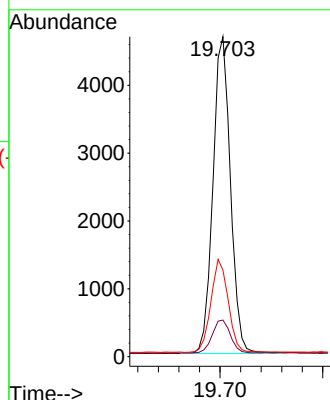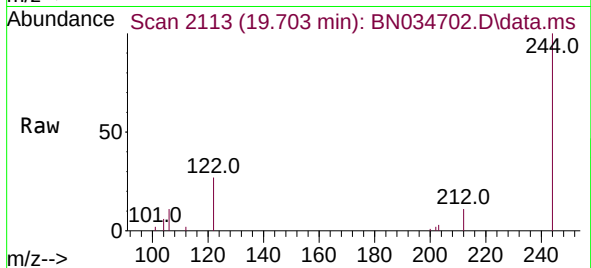

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.026 ng

RT: 21.196 min Scan# 2415

Delta R.T. 0.000 min

Lab File: BN034702.D

Acq: 24 Oct 2024 21:38




Tgt Ion:149 Resp: 397


Ion Ratio Lower Upper

149 100

167 22.4 19.7 29.5


279 0.0 1.8 2.6

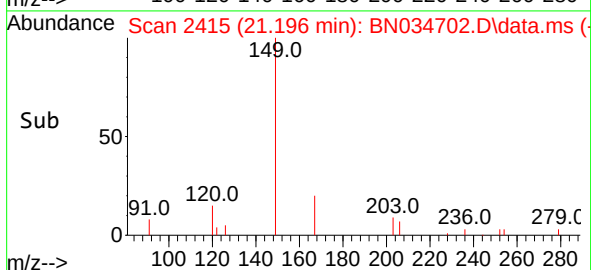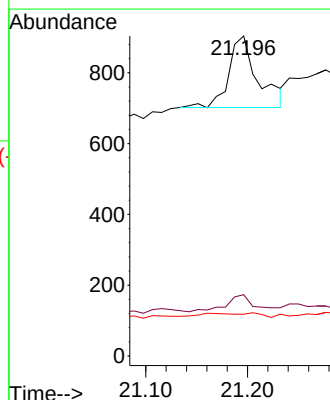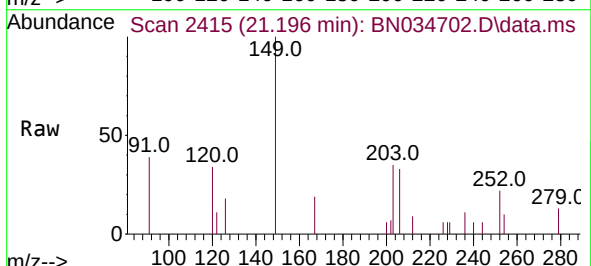

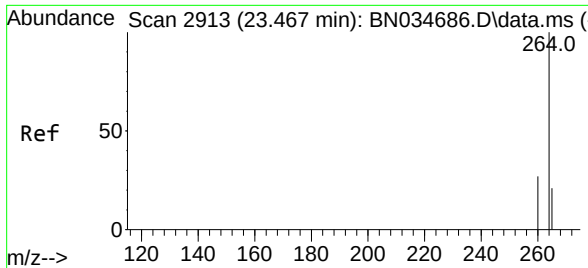

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.461 min Scan# 2911
 Delta R.T. -0.006 min
 Lab File: BN034702.D
 Acq: 24 Oct 2024 21:38

Instrument :
 BNA_N
 ClientSampleId :
 PB164230BL

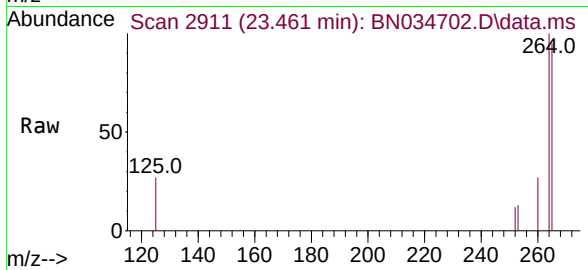

Tgt Ion:264 Resp: 6436
 Ion Ratio Lower Upper
 264 100
 260 26.9 21.9 32.9
 265 94.6 60.6 91.0#

