
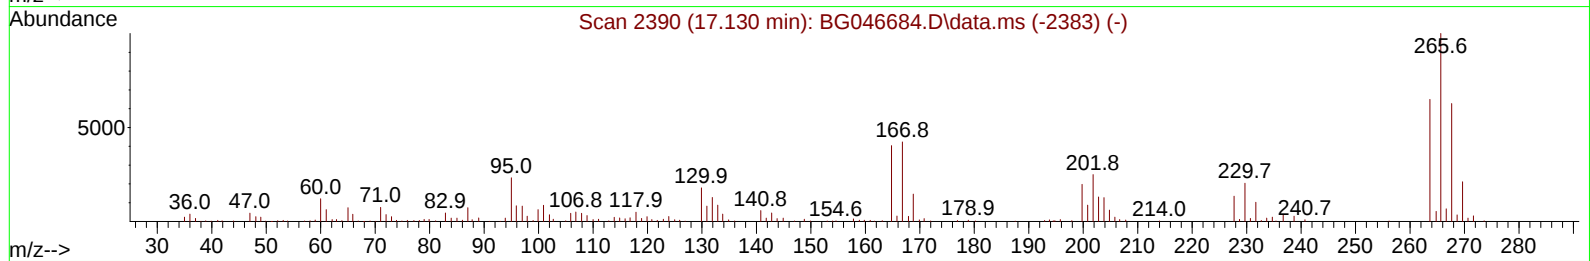
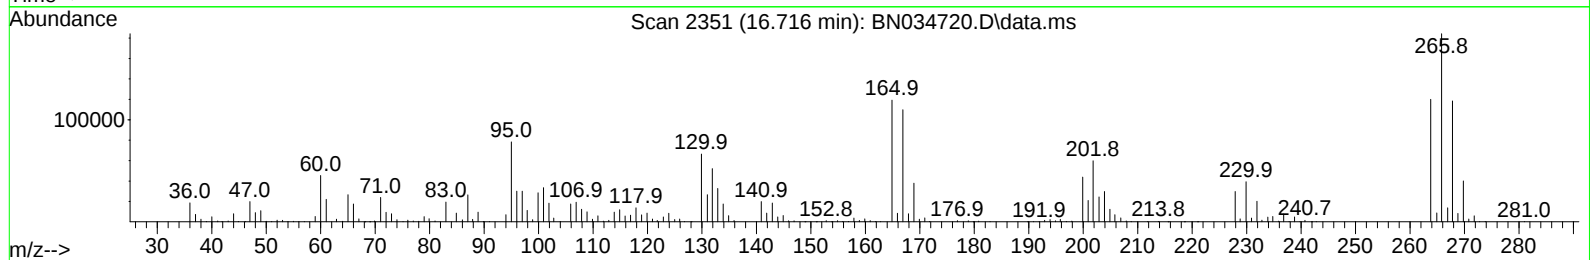


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102524\
Data File : BN034720.D
Acq On : 25 Oct 2024 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 14:47:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 02:24:36 2024
Response via : Initial Calibration

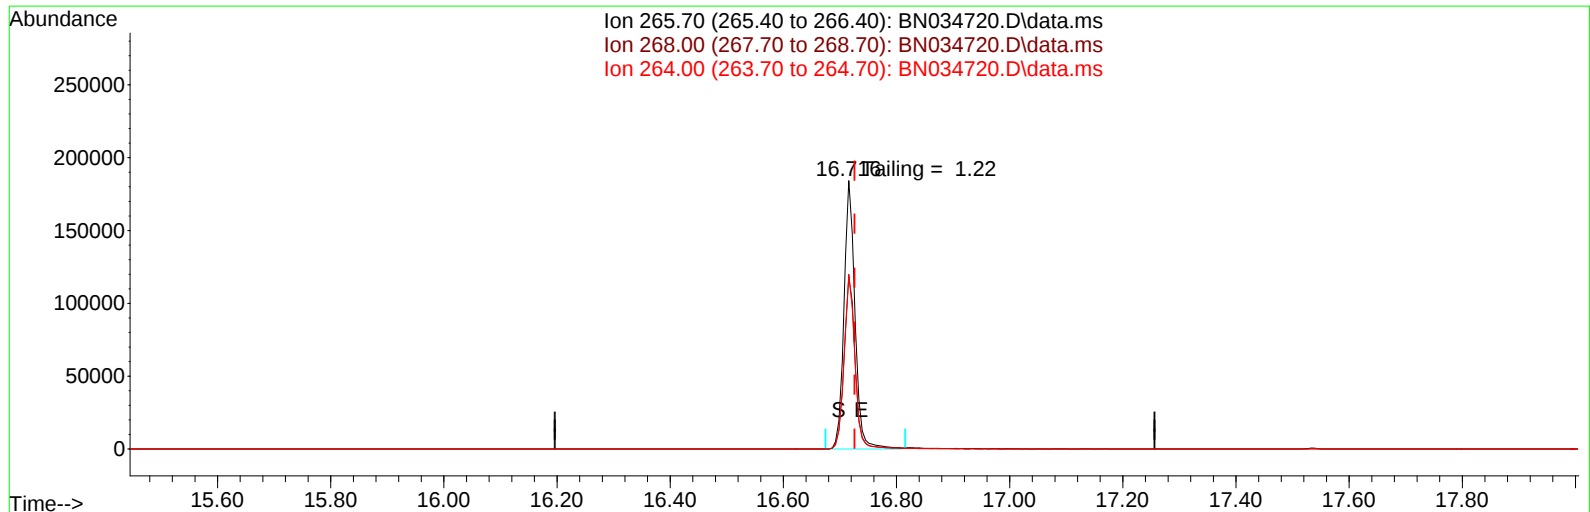

TIC: BN034720.D\data.ms

(70) Pentachlorophenol (C)




16.716min (-0.010) 16177.27 ng

response 249213

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.29
264.00	61.60	65.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102524\
Data File : BN034720.D
Acq On : 25 Oct 2024 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 14:47:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 02:24:36 2024
Response via : Initial Calibration

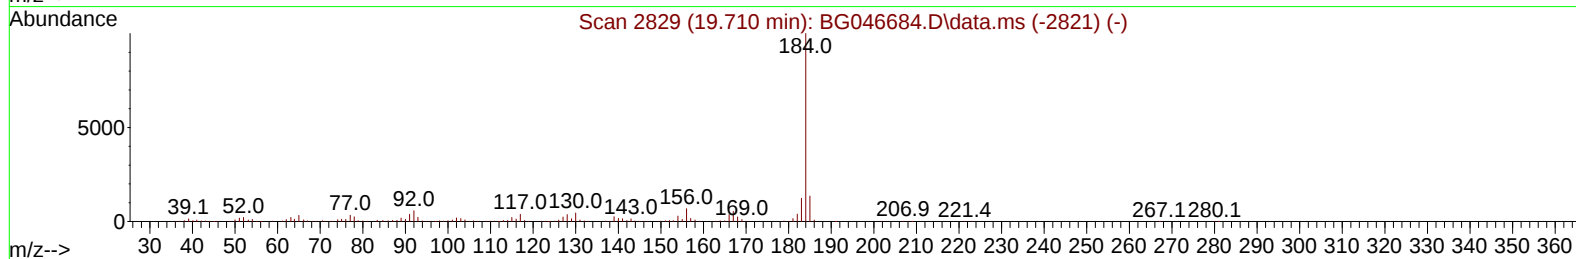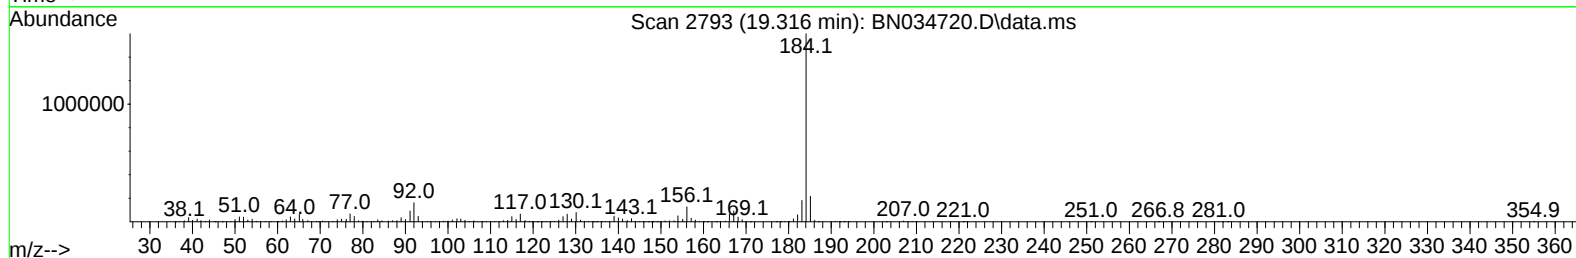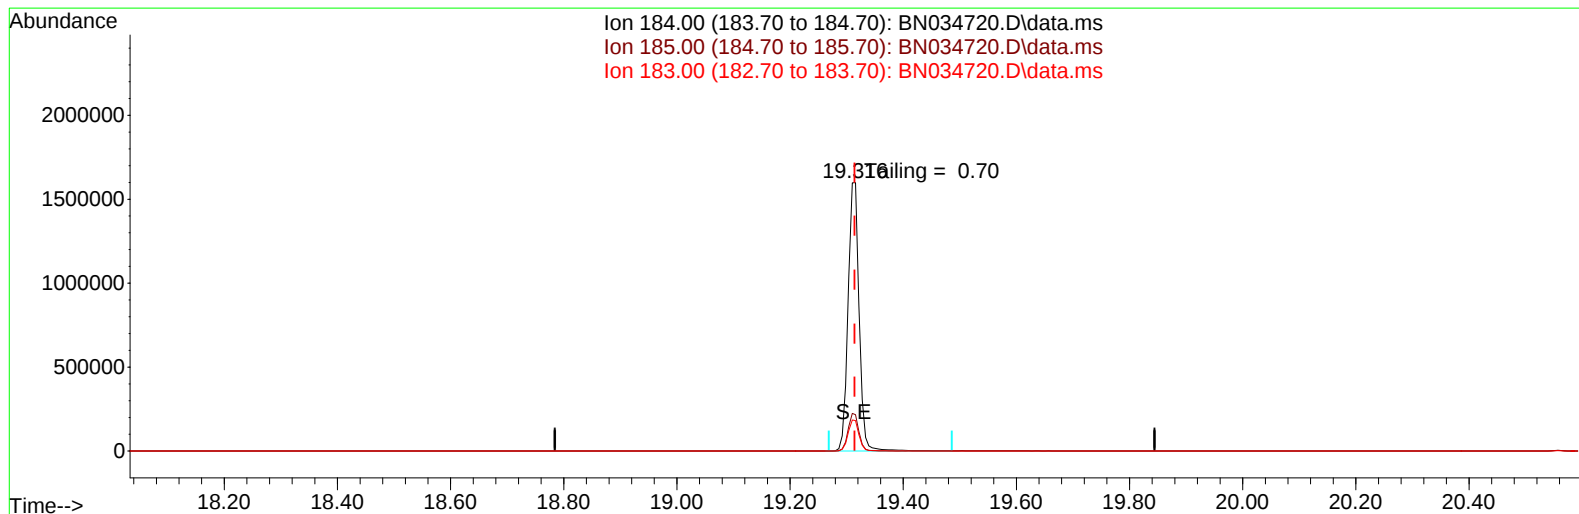

TIC: BN034720.D\data.ms

(77) Benzidine

19.316min (+ 0.002) 0.00 ng

response 2170006

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.53
183.00	13.20	11.36
0.00	0.00	0.00