


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102524\
Data File : BN034720.D
Acq On : 25 Oct 2024 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 25 22:11:36 2024

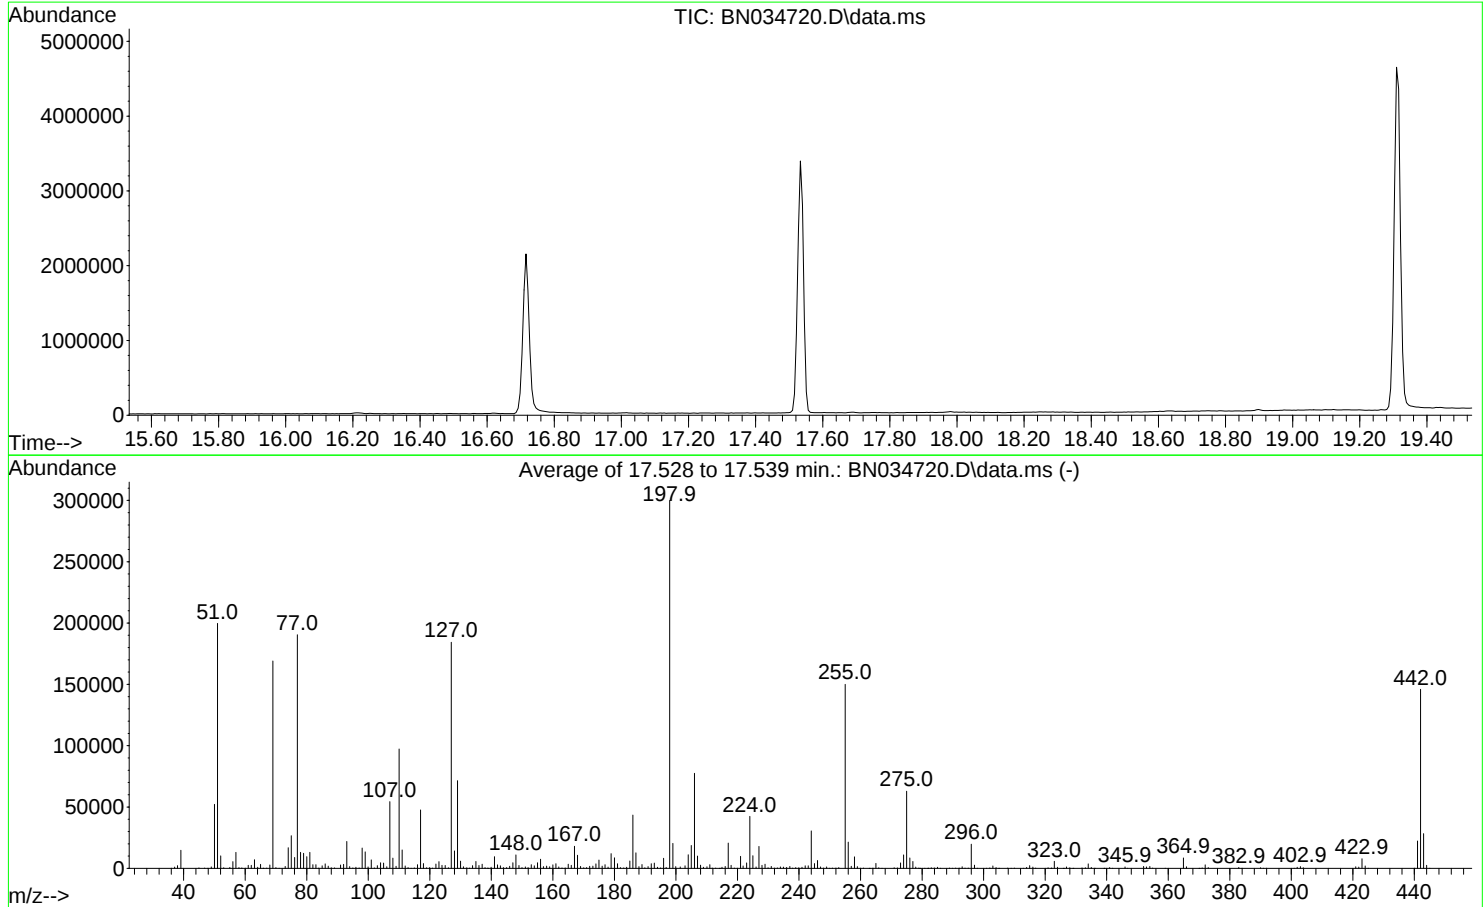

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	66.6	199713	PASS
68	69	0.00	2	1.6	2696	PASS
69	198	0.00	100	56.4	169054	PASS
70	69	0.00	2	0.4	594	PASS
127	198	10	80	61.5	184363	PASS
197	198	0.00	2	0.3	764	PASS
198	198	100	100	100.0	299904	PASS
199	198	5	9	6.8	20312	PASS
275	198	10	60	21.0	62957	PASS
365	198	1	100	2.8	8432	PASS
441	198	0.01	100	7.4	22267	PASS
442	442	50	100	100.0	145949	PASS
443	442	15	24	19.4	28343	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/25/2024	BNA_N	<u>BN034720.D</u>
Compound Name	Response	Retention Time
DDT	888185	20.557
DDD	14092	20.169
DDE	315	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14407	902592	1.60

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102524\
Data File : BN034720.D
Acq On : 25 Oct 2024 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 25 14:47:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 02:24:36 2024
Response via : Initial Calibration

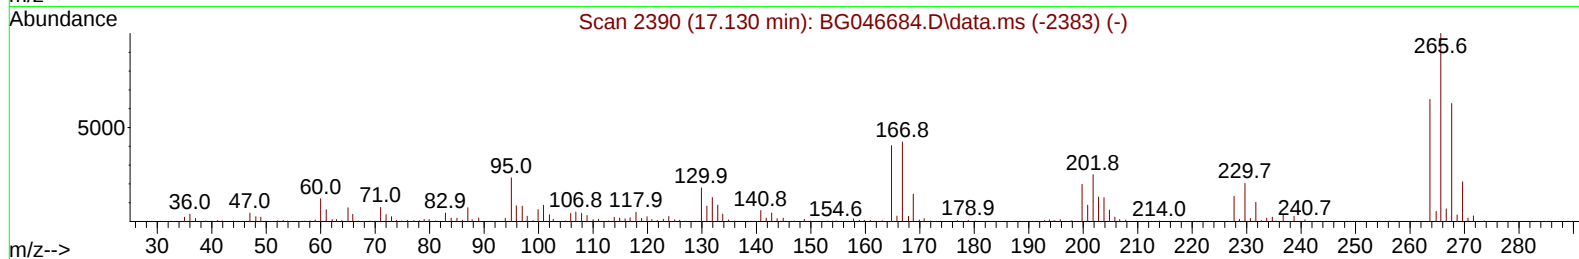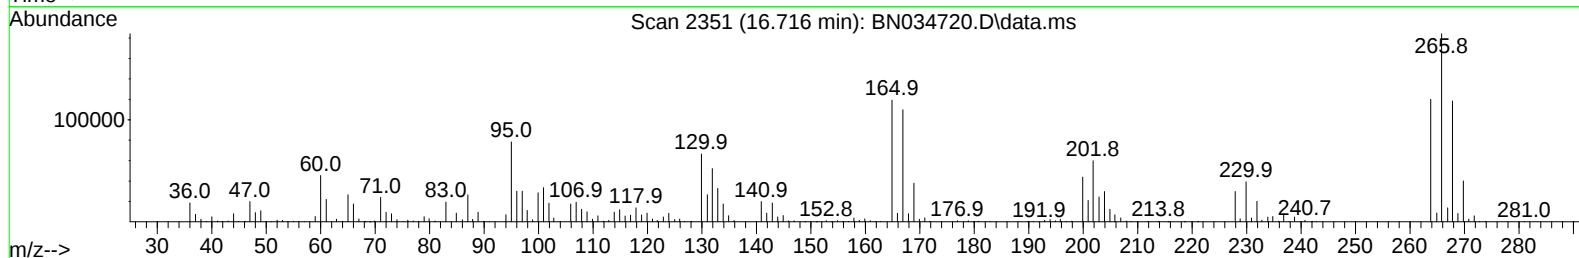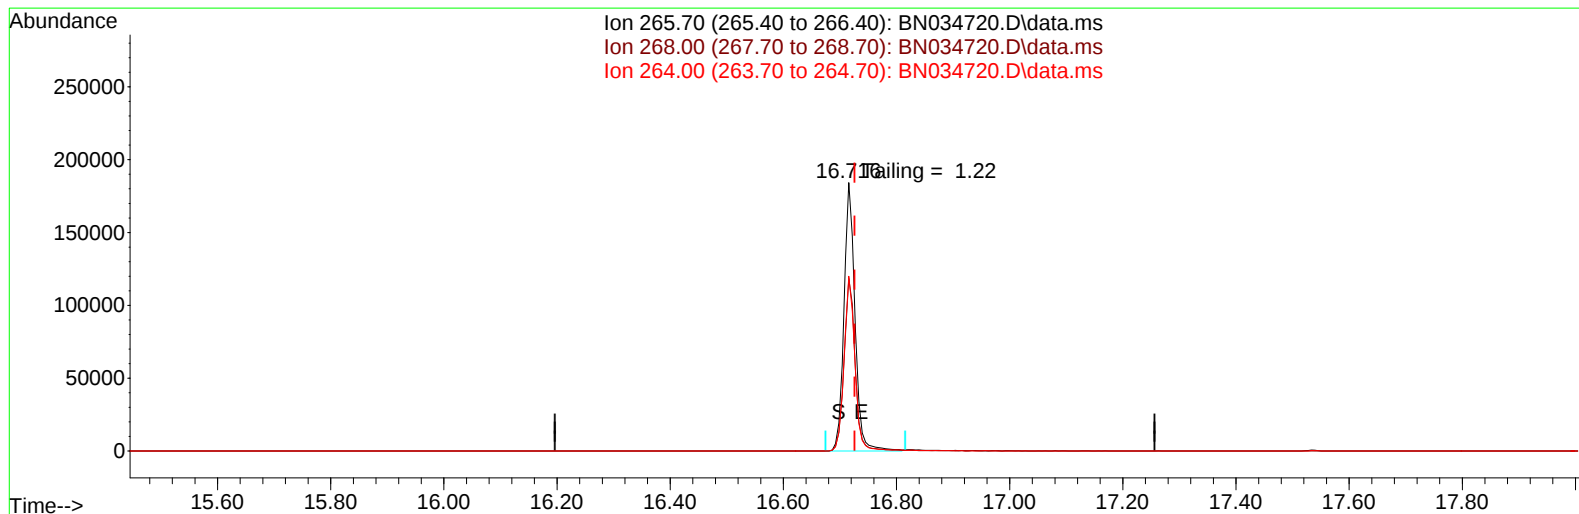

TIC: BN034720.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.010) 16177.27 ng




response 249213

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.29
264.00	61.60	65.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102524\
Data File : BN034720.D
Acq On : 25 Oct 2024 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 25 14:47:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 02:24:36 2024
Response via : Initial Calibration

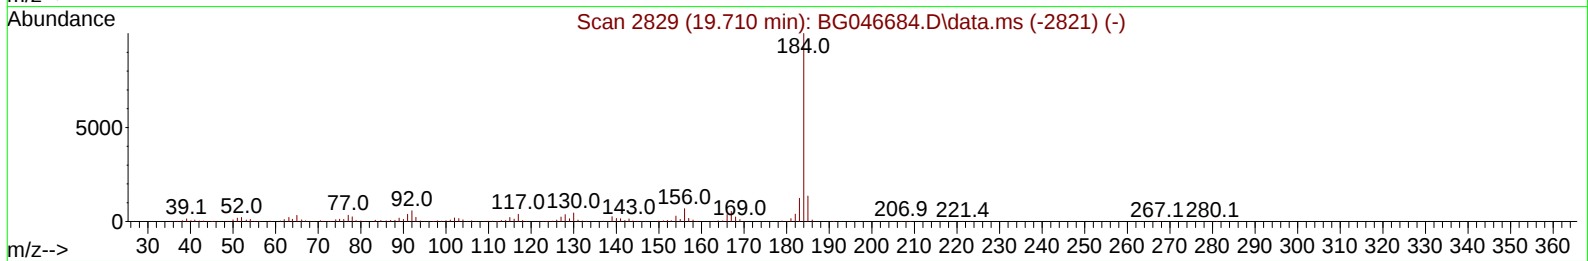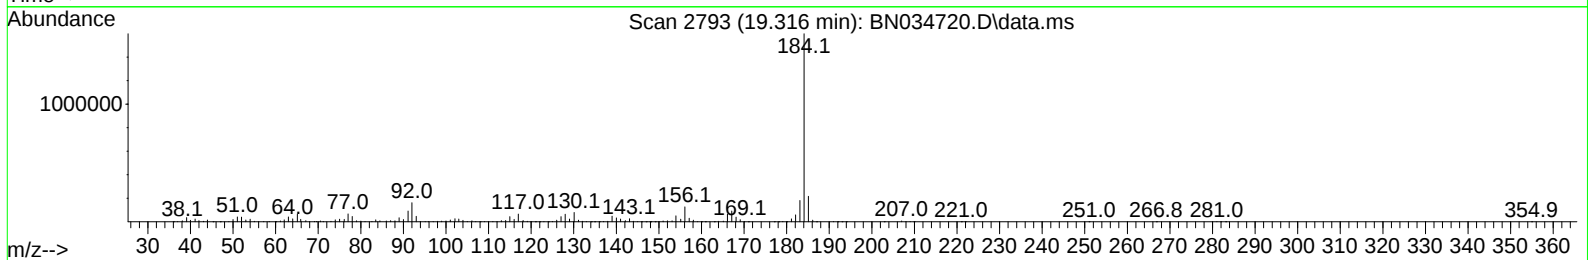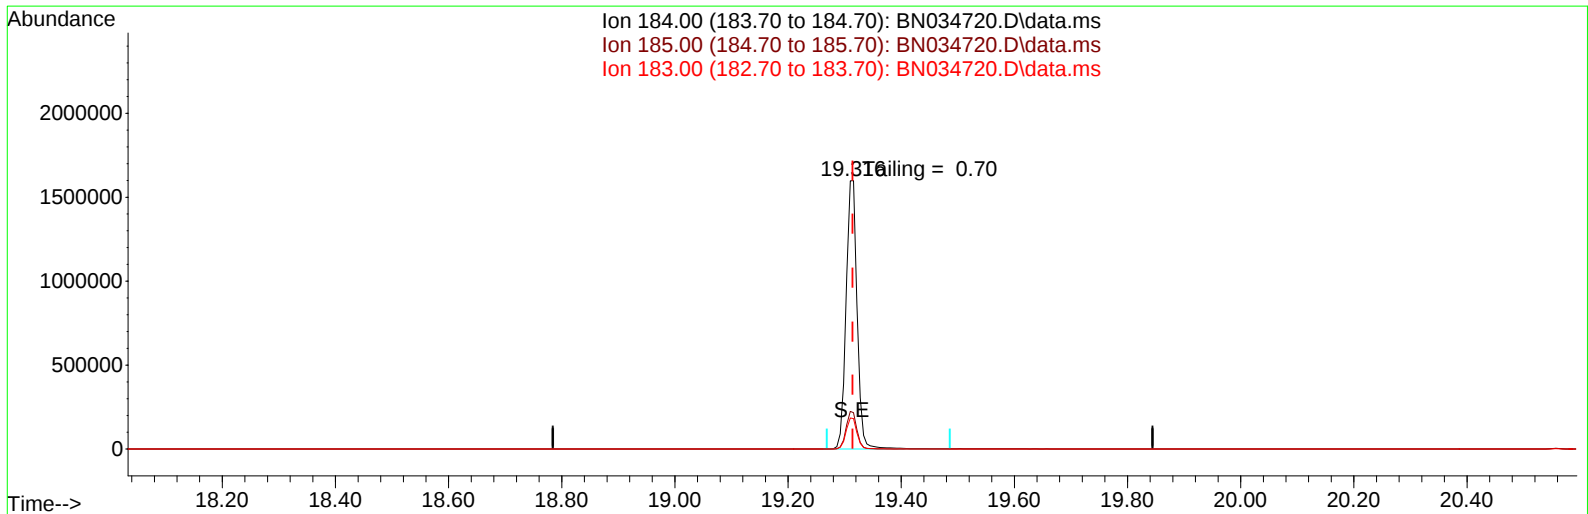

TIC: BN034720.D\data.ms

(77) Benzidine

19.316min (+ 0.002) 0.00 ng

response 2170006

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.53
183.00	13.20	11.36
0.00	0.00	0.00