


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102622\
 Data File : BN022329.D
 Acq On : 26 Oct 2022 09:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 27 05:55:40 2022

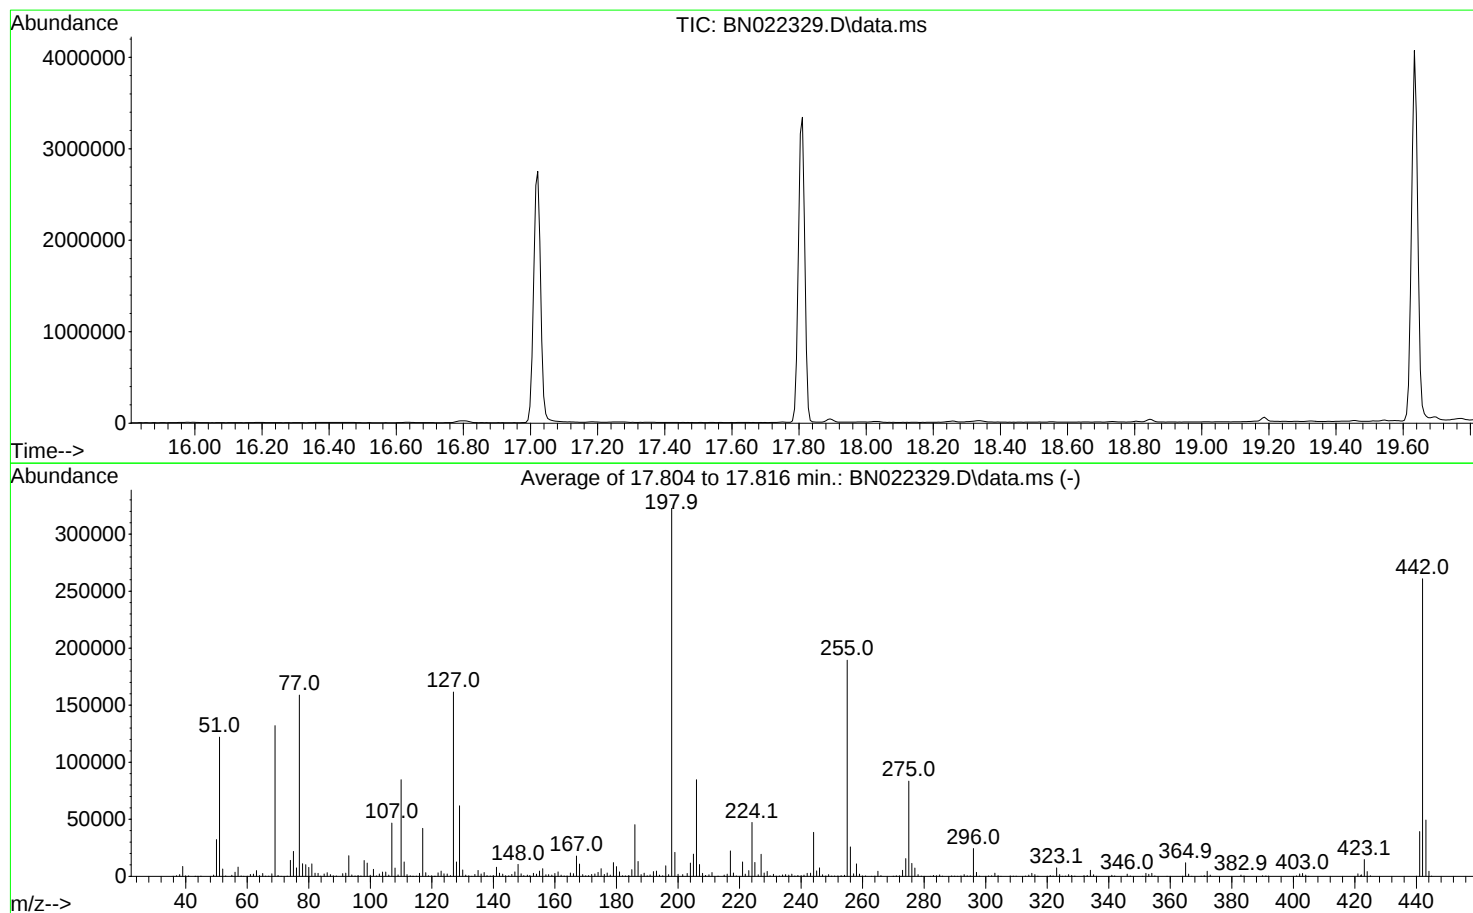

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	122011	PASS
68	69	0.00	2	1.6	2156	PASS
69	198	0.00	100	41.0	132173	PASS
70	69	0.00	2	0.6	804	PASS
127	198	10	80	50.1	161539	PASS
197	198	0.00	2	0.5	1547	PASS
198	198	100	100	100.0	322560	PASS
199	198	5	9	6.5	21030	PASS
275	198	10	60	25.9	83467	PASS
365	198	1	100	3.7	11905	PASS
441	198	0.01	100	12.2	39267	PASS
442	442	50	100	100.0	260885	PASS
443	442	15	24	18.9	49312	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/26/2022	BNA_N	<u>BN022329.D</u>
Compound Name	Response	Retention Time
DDT	925425	20.869
DDD	74305	20.427
DDE	3074	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
77379	1002804	7.72

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102622\
 Data File : BN022329.D
 Acq On : 26 Oct 2022 09:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 28 08:50:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 28 08:50:52 2022
 Response via : Initial Calibration

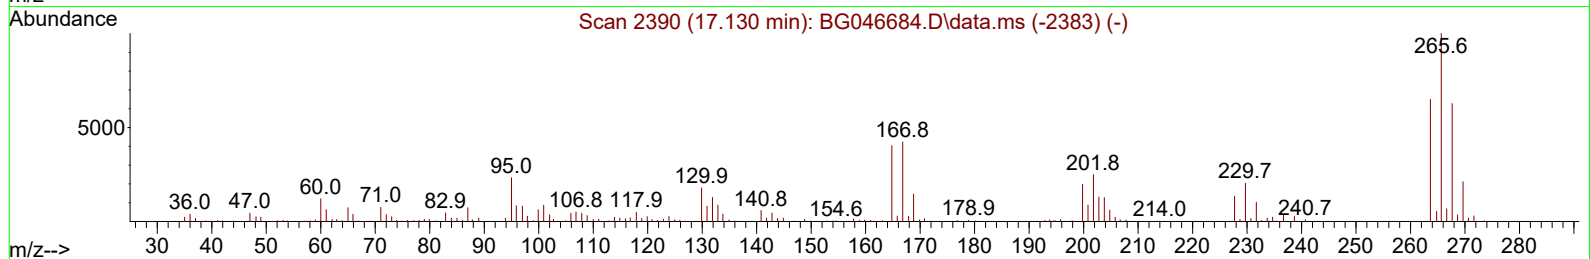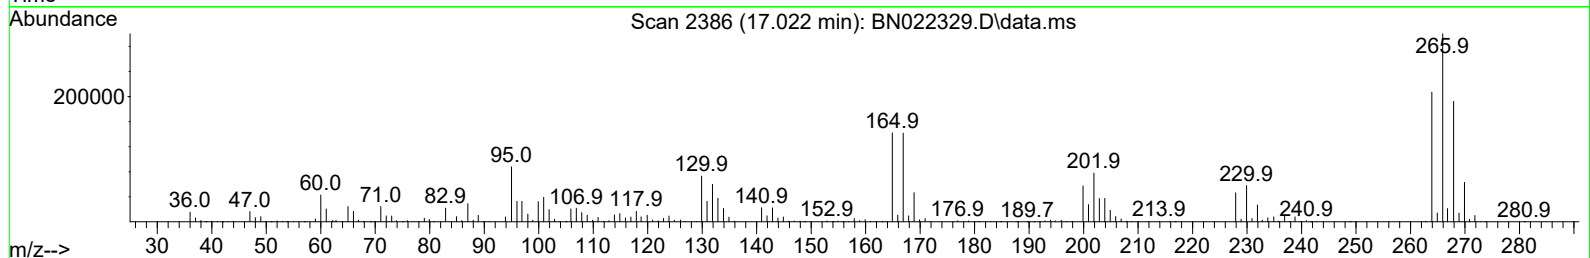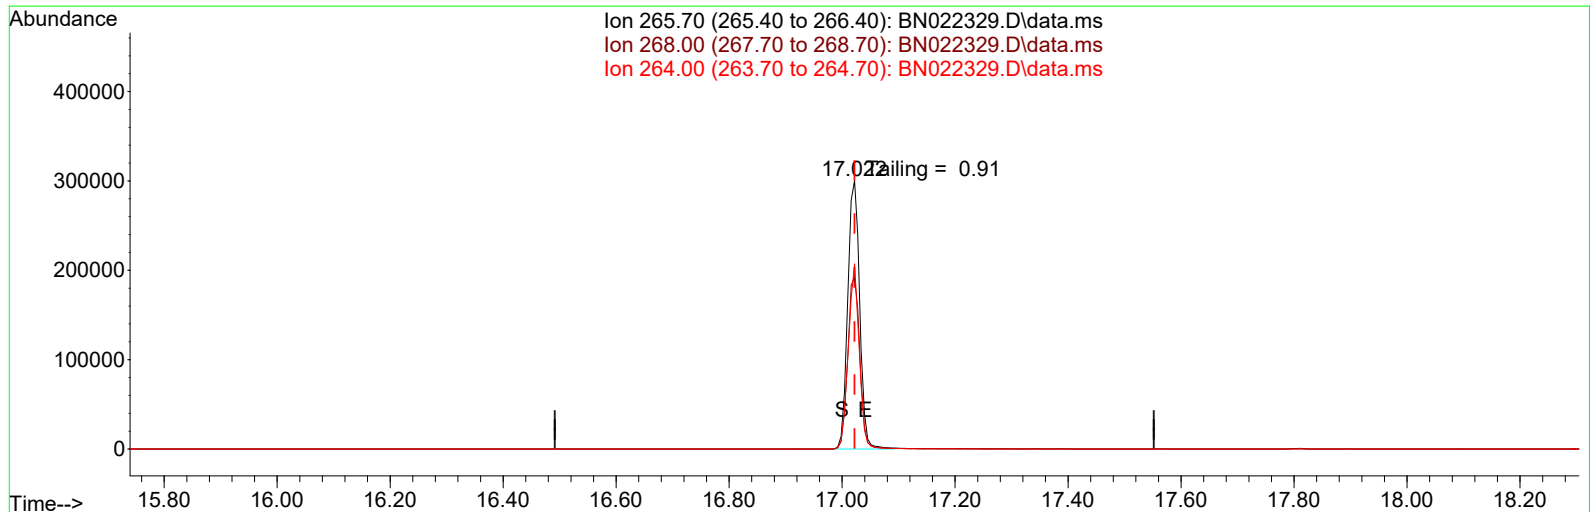

TIC: BN022329.D\data.ms

(70) Pentachlorophenol (C)

17.022min (0.000) 24965.42 ng




response 443764

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.05
264.00	61.60	69.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102622\
Data File : BN022329.D
Acq On : 26 Oct 2022 09:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 28 08:50:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 28 08:50:52 2022
Response via : Initial Calibration

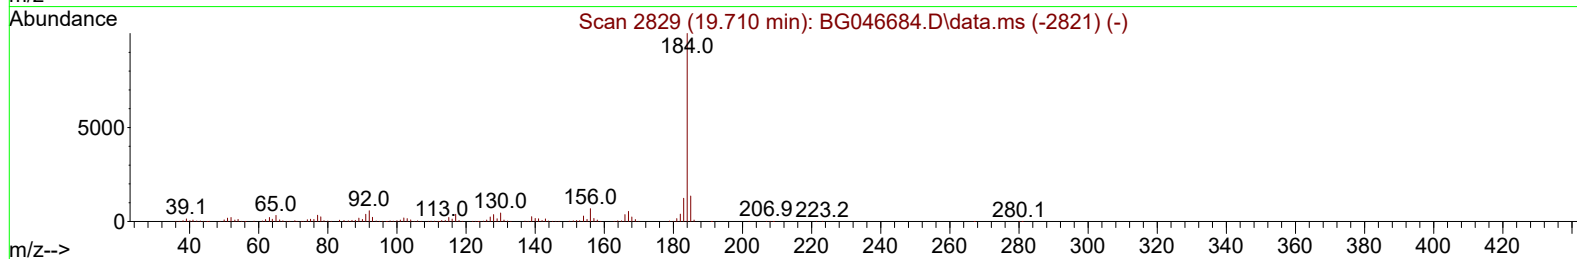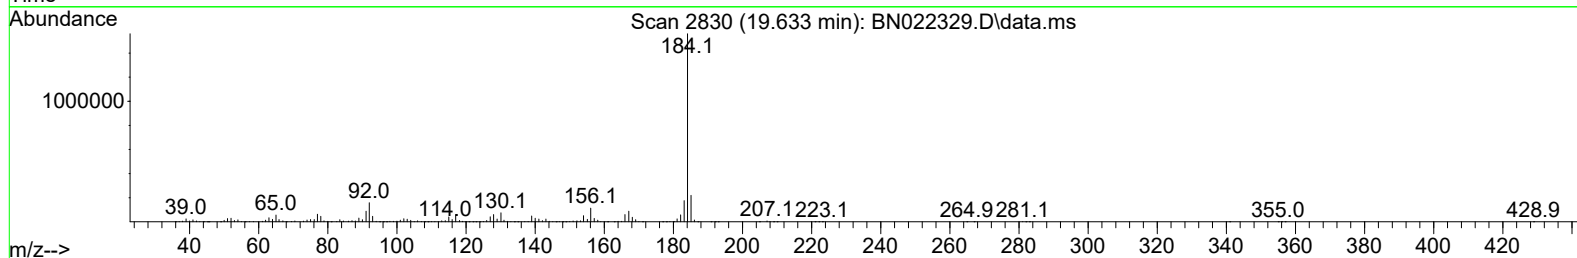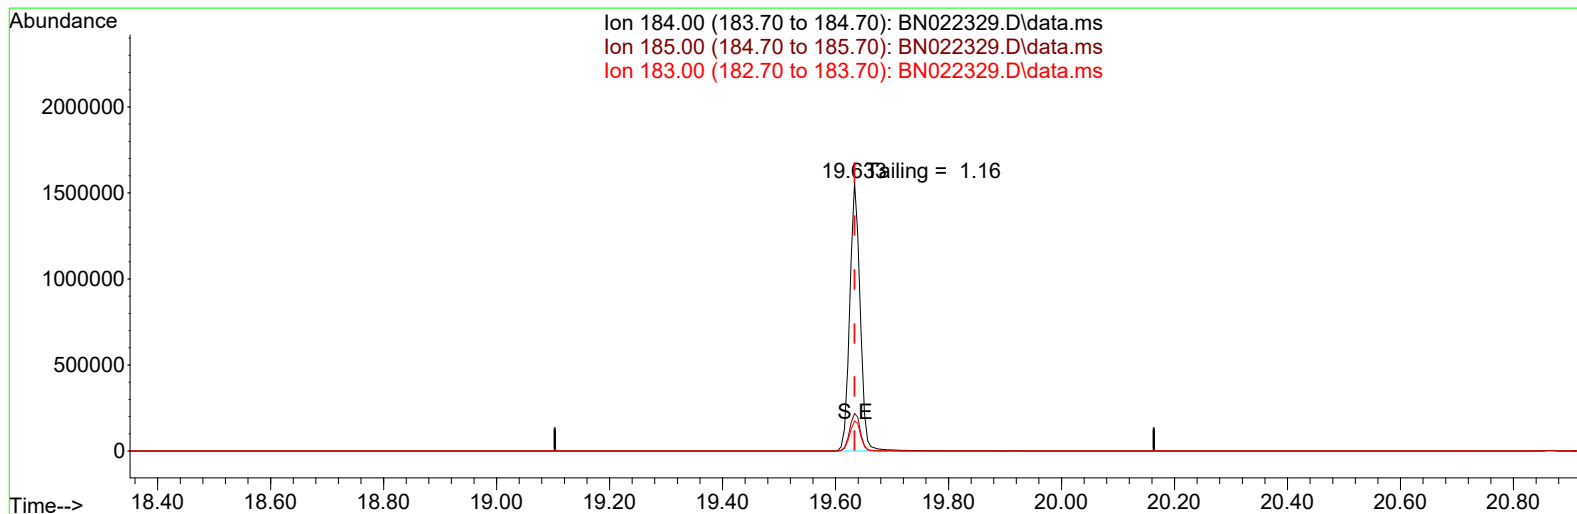

TIC: BN022329.D\data.ms

(77) Benzidine

19.633min (0.000) 36841.82 ng

response 1984003

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.05
183.00	13.20	11.26
0.00	0.00	0.00