
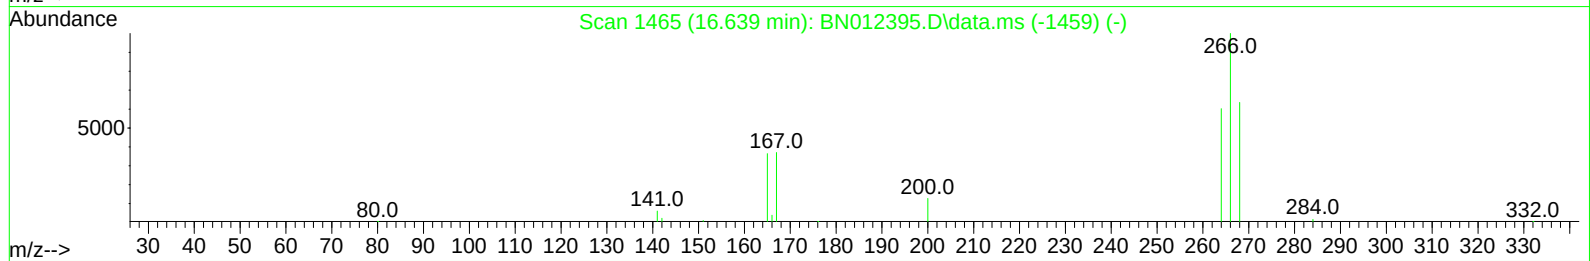
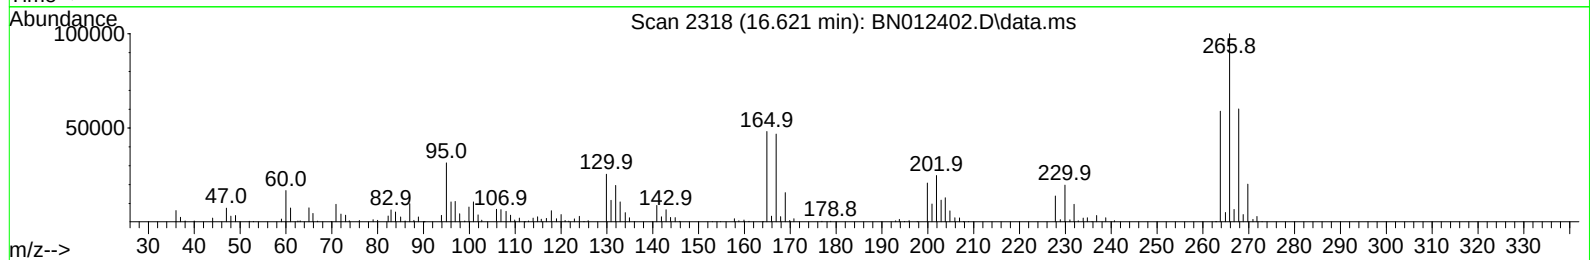


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102720\
Data File : BN012402.D
Acq On : 27 Oct 2020 09:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 02:57:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 27 11:36:24 2020
Response via : Initial Calibration

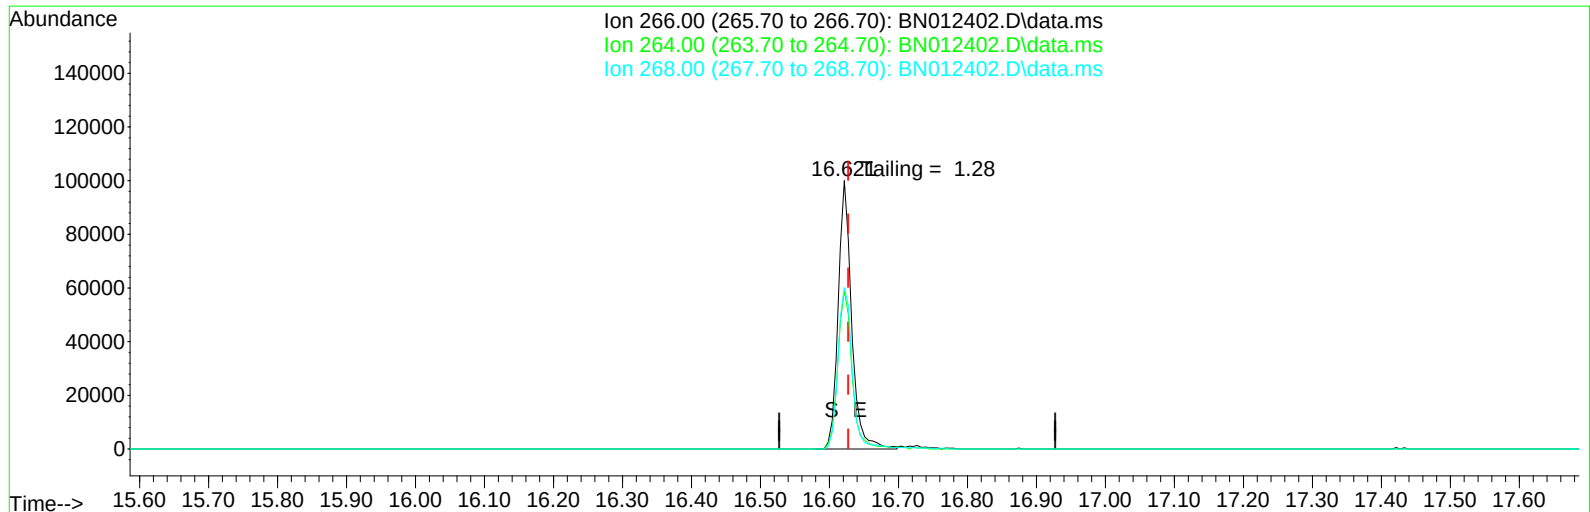

TIC: BN012402.D\data.ms

(24) Pentachlorophenol

16.621min (-0.006) 0.00 ng

response 135506

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	62.39
268.00	64.40	64.11
0.00	0.00	0.00